

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041421\
 Data File : PD062153.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2021 09:37
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 15:42:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.980	19638778	214.8E6	23.455	24.725
28)	SA Decachlor...	8.256	9.038	30827252	202.4E6	25.054	21.437
Target Compounds							
2)	A alpha-BHC	3.924	4.368	14111290	162.4E6	11.173	12.073
3)	MA gamma-BHC...	4.209	4.653	14058532	160.4E6	11.841	12.860
6)	B beta-BHC	4.459	4.823	7121953	68760805	13.060	13.312
7)	B delta-BHC	0.000	5.015f	0	14061135	N.D.	1.063 #
8)	B Heptachlo...	0.000	5.861	0	3770825	N.D.	0.318 #
9)	A Endosulfan I	0.000	6.191f	0	388867	N.D.	0.036 #
10)	B gamma-Chl...	0.000	6.064f	0	1119775	N.D.	0.094 #
11)	B alpha-Chl...	0.000	6.173	0	850314	N.D.	0.075 #
12)	B 4,4'-DDE	0.000	6.317	0	2089180	N.D.	0.181 #
13)	MA Dieldrin	0.000	6.469	0	6994581	N.D.	0.606 #
14)	MA Endrin	6.049	6.683	62905348	562.2E6	61.221	56.807
15)	B Endosulfa...	0.000	6.898	0	6000546	N.D.	0.632 #
16)	A 4,4'-DDD	6.173	6.805	1370177	16071673	1.472	1.697
17)	MA 4,4'-DDT	6.415	7.103	123.5E6	1055.2E6	137.058	110.475
18)	B Endrin al...	0.000	7.016	0	8401032	N.D.	1.068 #
20)	A Methoxychlor	6.961	7.561	162.3E6	1235.9E6	343.414	274.161
21)	B Endrin ke...	7.198	7.708	3809069	22395449	2.985	2.208 #
24)	Chlordane-2	0.000	5.425f	0	302222	N.D.	0.788 #
25)	Chlordane-3	0.000	6.064f	0	1119775	N.D.	0.675 #
26)	Chlordane-4	0.000	6.173	0	850314	N.D.	0.443 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041421\
Data File : PD062153.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2021 09:37
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 15:42:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

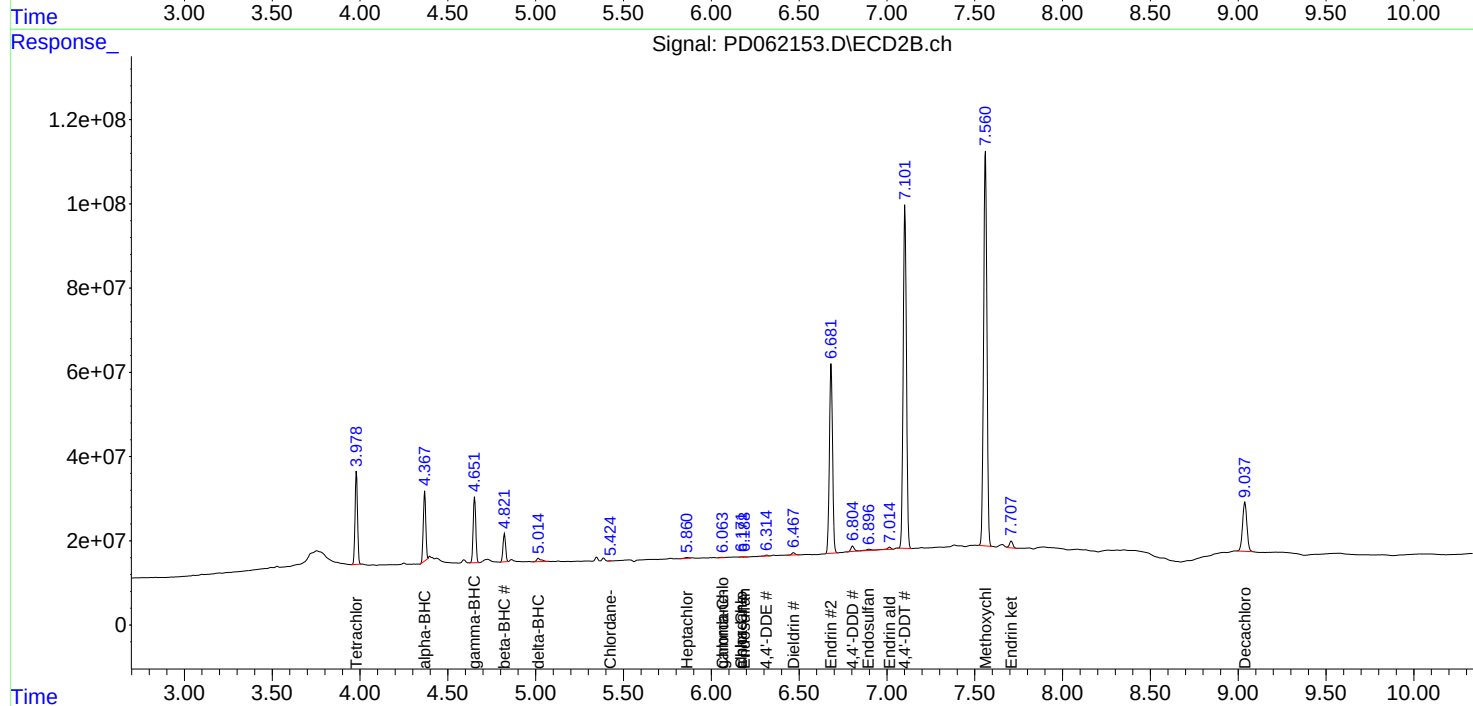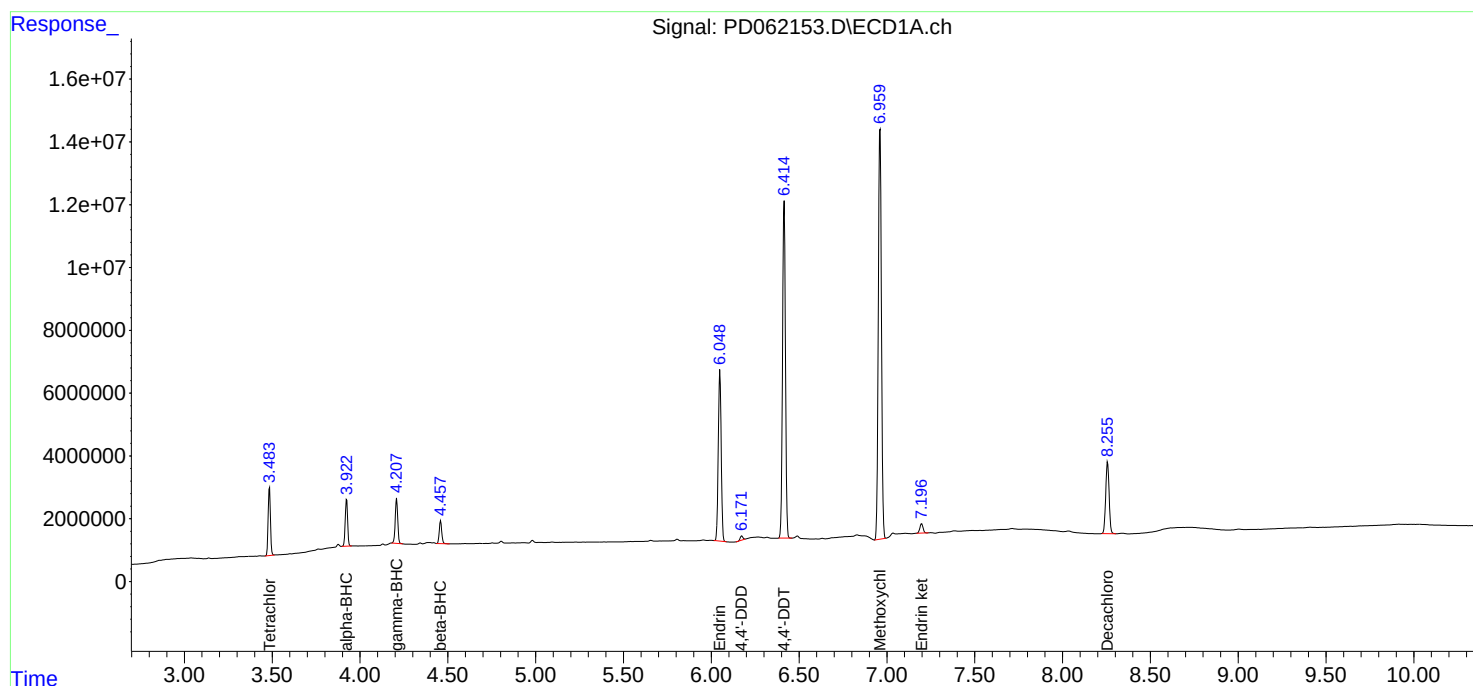


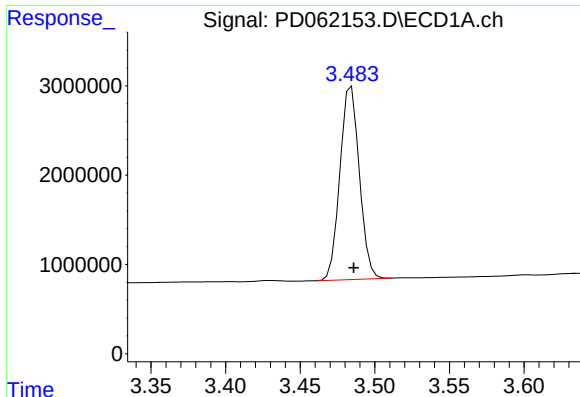

#1 Tetrachloro-m-xylene


R.T.: 3.484 min
Delta R.T.: -0.002 min
Response: 19638778
Conc: 23.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

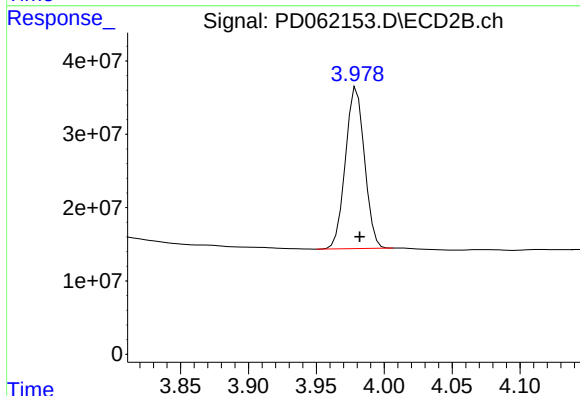


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 214830836
Conc: 24.72 ng/ml

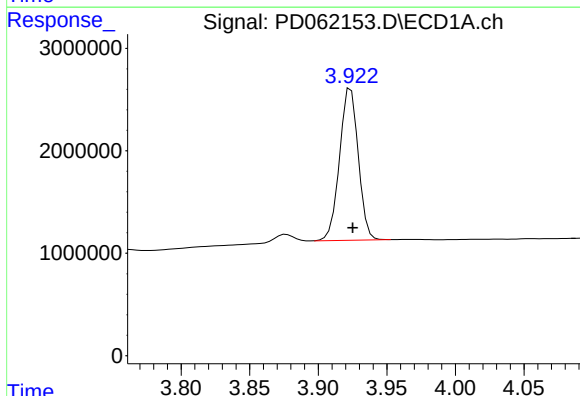


#2 alpha-BHC

R.T.: 3.924 min
Delta R.T.: -0.001 min
Response: 14111290
Conc: 11.17 ng/ml

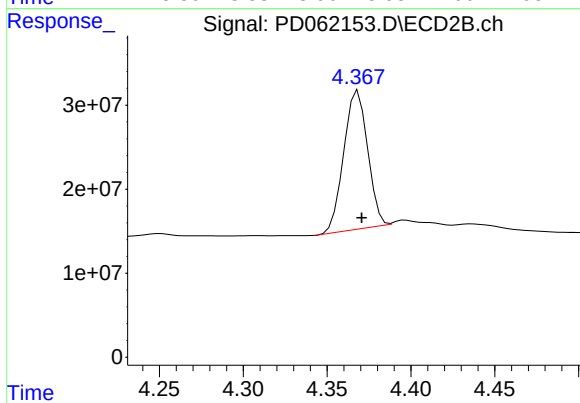

#2 alpha-BHC


R.T.: 4.368 min
Delta R.T.: -0.002 min
Response: 162387107
Conc: 12.07 ng/ml

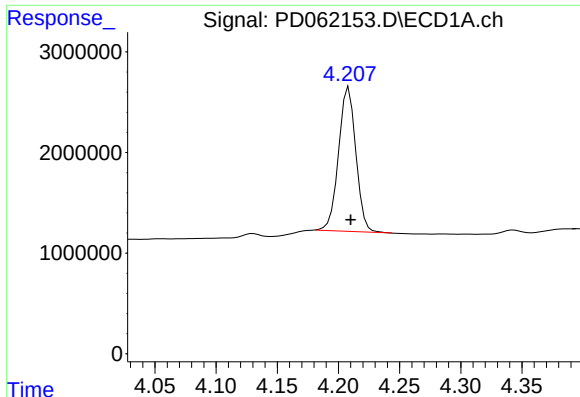

#3 gamma-BHC (Lindane)


R.T.: 4.209 min
Delta R.T.: -0.002 min
Response: 14058532
Conc: 11.84 ng/ml

Instrument :
ECD_D
ClientSampleId :

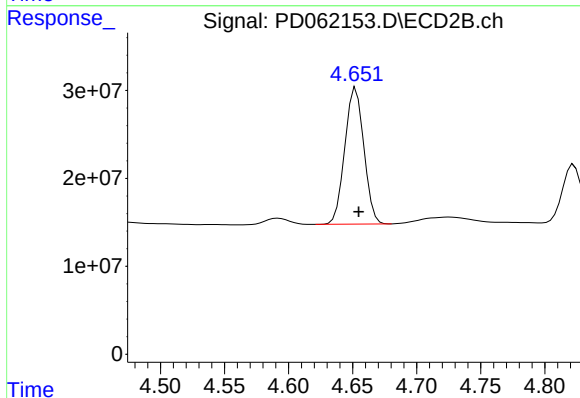


#3 gamma-BHC (Lindane)

R.T.: 4.653 min
Delta R.T.: -0.002 min
Response: 160407118
Conc: 12.86 ng/ml

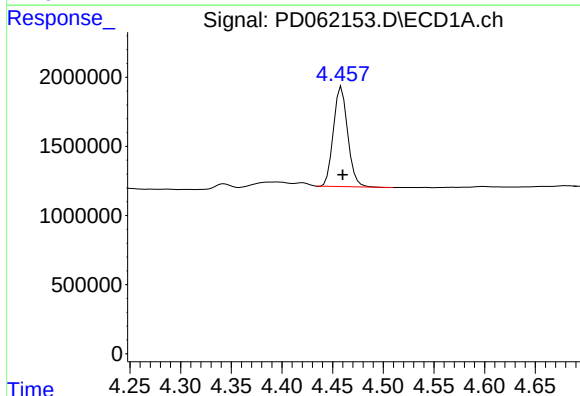


#6 beta-BHC

R.T.: 4.459 min
Delta R.T.: -0.001 min
Response: 7121953
Conc: 13.06 ng/ml

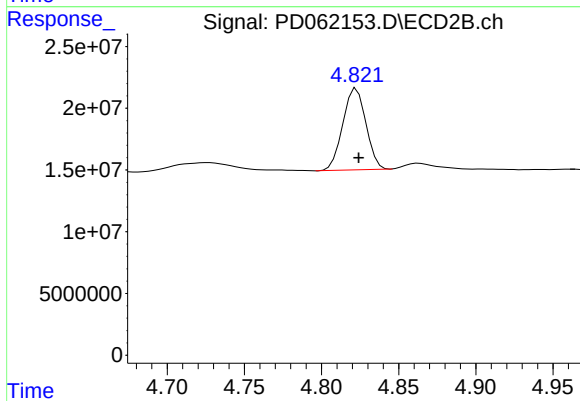

#6 beta-BHC


R.T.: 4.823 min
Delta R.T.: -0.002 min
Response: 68760805
Conc: 13.31 ng/ml

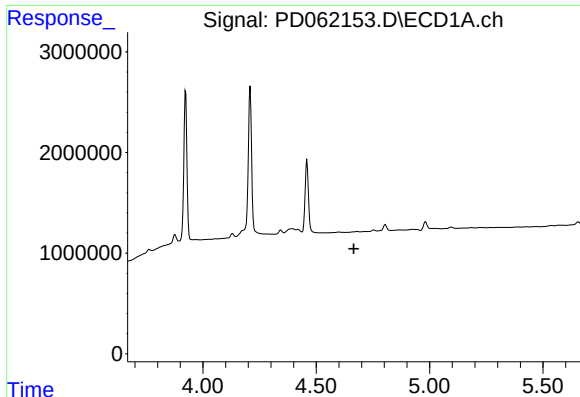

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.666 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

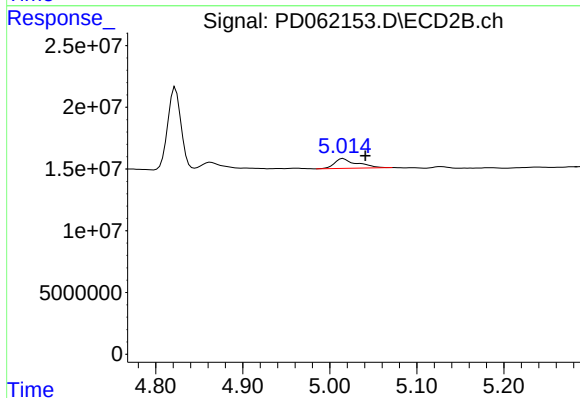


#7 delta-BHC

R.T.: 5.015 min
Delta R.T.: -0.026 min
Response: 14061135
Conc: 1.06 ng/ml

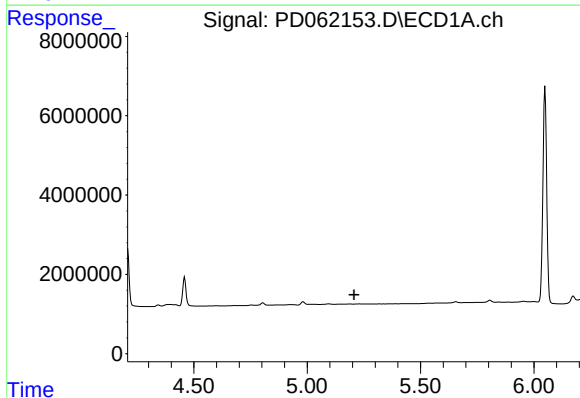


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.207 min
Response: 0
Conc: N.D.

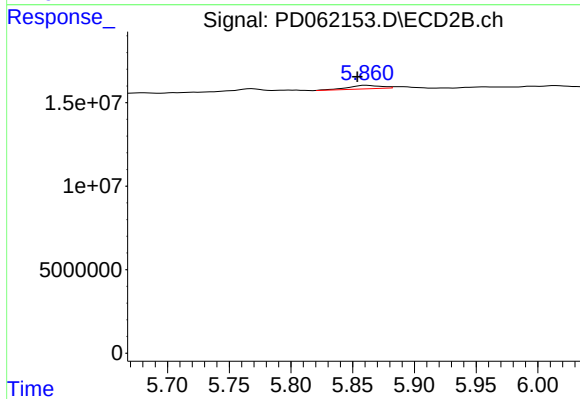

#8 Heptachlor epoxide


R.T.: 5.861 min
Delta R.T.: 0.007 min
Response: 3770825
Conc: 0.32 ng/ml

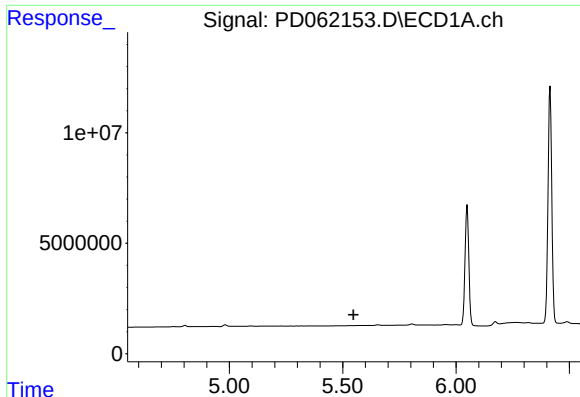

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.548 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

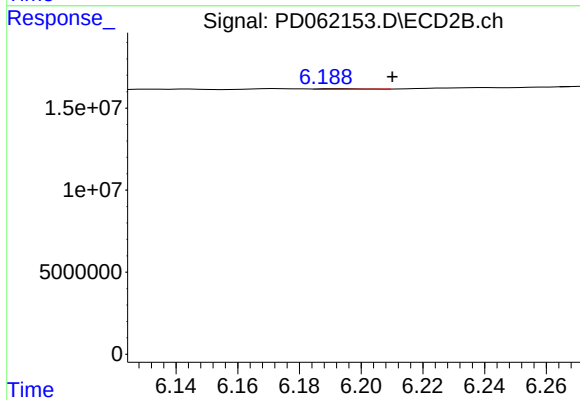


#9 Endosulfan I

R.T.: 6.191 min
Delta R.T.: -0.019 min
Response: 388867
Conc: 0.04 ng/ml

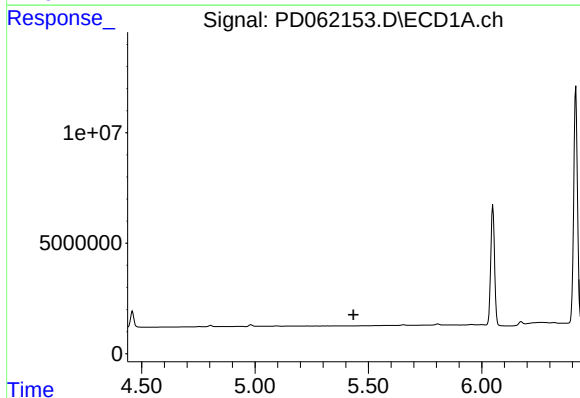


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.435 min
Response: 0
Conc: N.D.

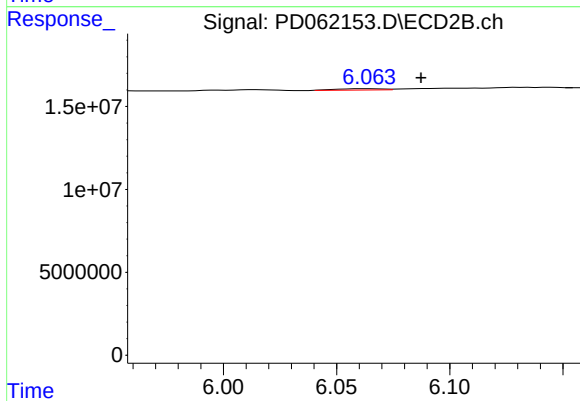

#10 gamma-Chlordane


R.T.: 6.064 min
Delta R.T.: -0.023 min
Response: 1119775
Conc: 0.09 ng/ml

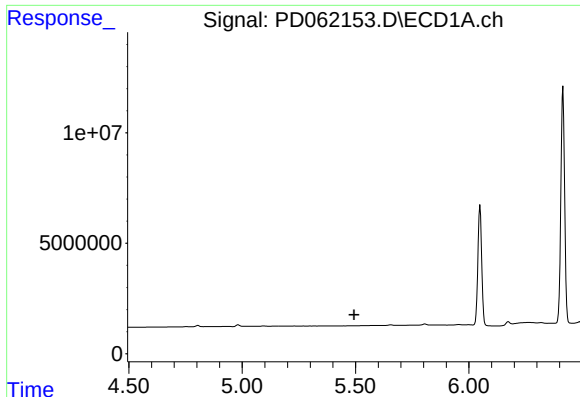

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.494 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

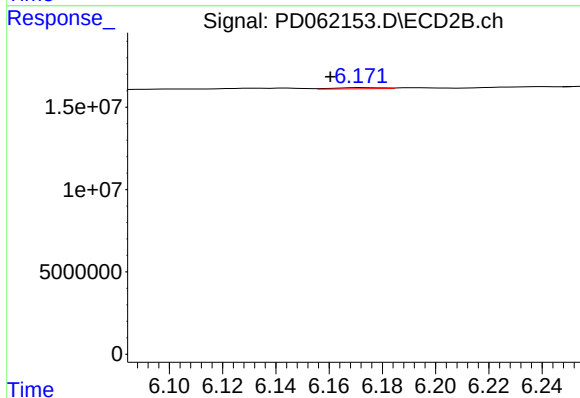


#11 alpha-Chlordane

R.T.: 6.173 min
Delta R.T.: 0.012 min
Response: 850314
Conc: 0.07 ng/ml

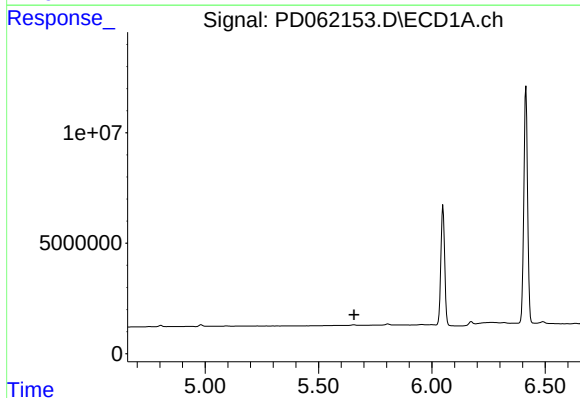


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.657 min
Response: 0
Conc: N.D.

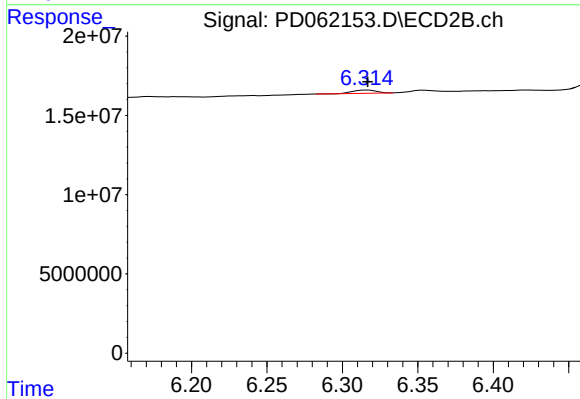

#12 4,4'-DDE


R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 2089180
Conc: 0.18 ng/ml

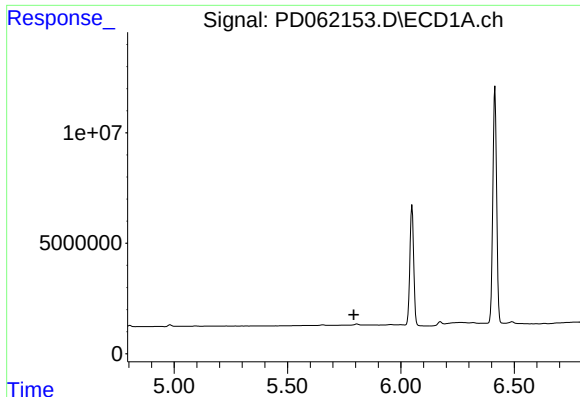

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.792 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

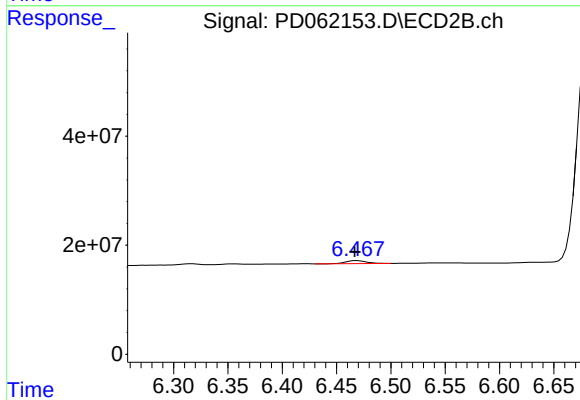


#13 Dieldrin

R.T.: 6.469 min
Delta R.T.: 0.002 min
Response: 6994581
Conc: 0.61 ng/ml

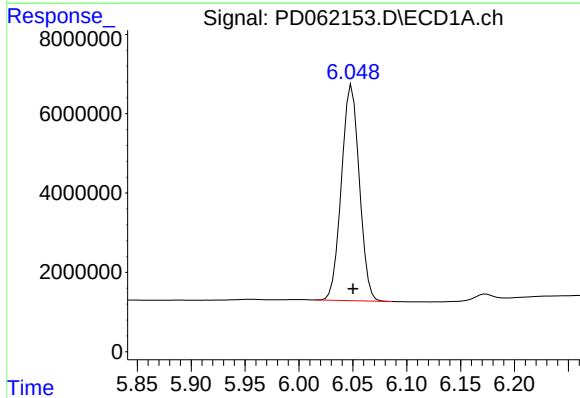


#14 Endrin

R.T.: 6.049 min
Delta R.T.: -0.001 min
Response: 62905348
Conc: 61.22 ng/ml

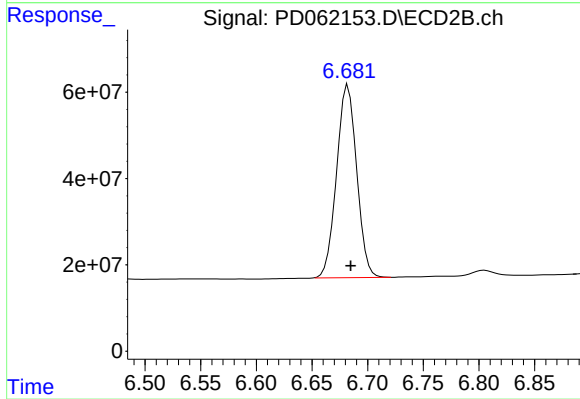

#14 Endrin


R.T.: 6.683 min
Delta R.T.: -0.002 min
Response: 562177189
Conc: 56.81 ng/ml

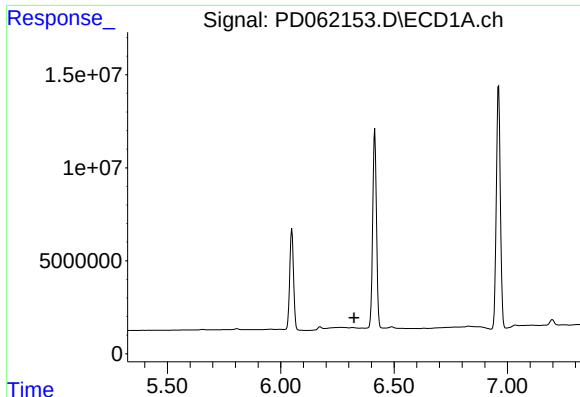

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.323 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

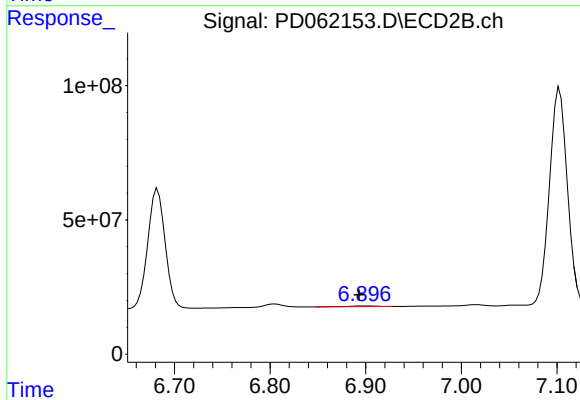


#15 Endosulfan II

R.T.: 6.898 min
Delta R.T.: 0.005 min
Response: 6000546
Conc: 0.63 ng/ml

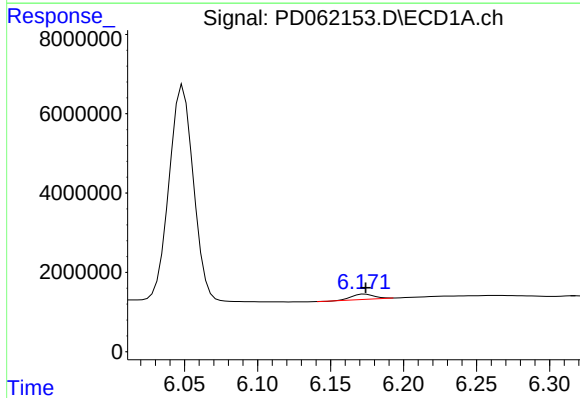


#16 4,4'-DDD

R.T.: 6.173 min
Delta R.T.: 0.000 min
Response: 1370177
Conc: 1.47 ng/ml

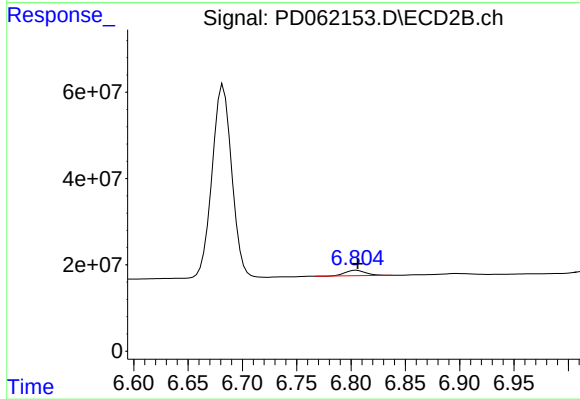

#16 4,4'-DDD


R.T.: 6.805 min
Delta R.T.: -0.001 min
Response: 16071673
Conc: 1.70 ng/ml

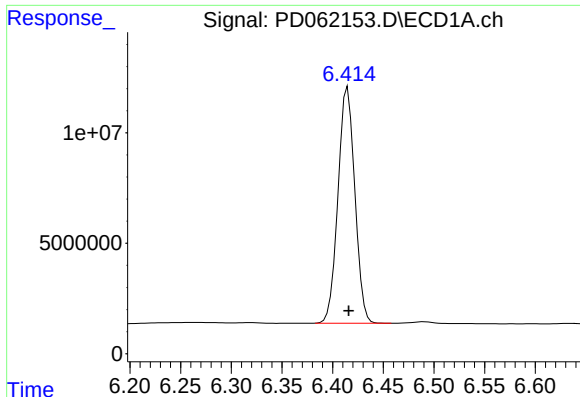

#17 4,4'-DDT


R.T.: 6.415 min
Delta R.T.: 0.000 min
Response: 123451891
Conc: 137.06 ng/ml

Instrument :
ECD_D
ClientSampleId :

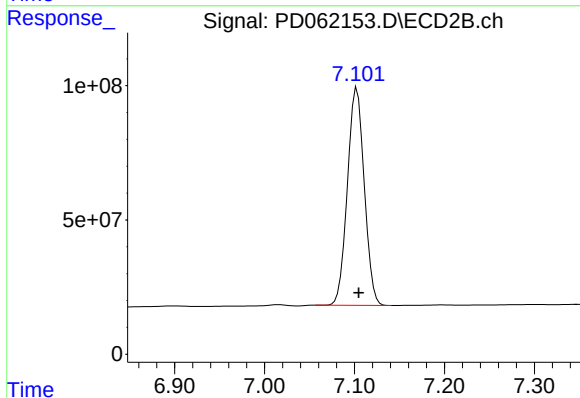


#17 4,4'-DDT

R.T.: 7.103 min
Delta R.T.: -0.002 min
Response: 1055214053
Conc: 110.47 ng/ml

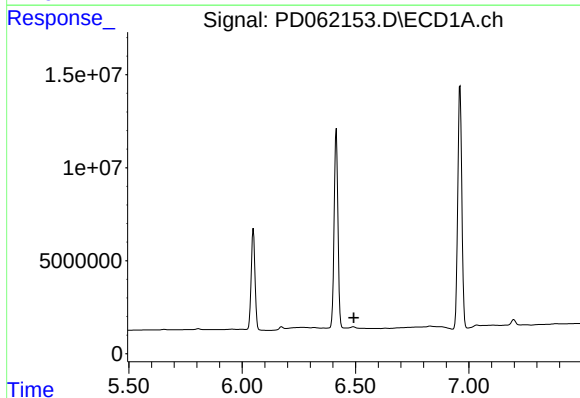


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.492 min
Response: 0
Conc: N.D.

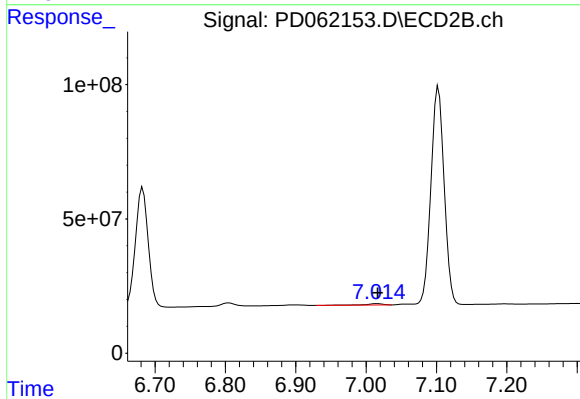

#18 Endrin aldehyde


R.T.: 7.016 min
Delta R.T.: -0.001 min
Response: 8401032
Conc: 1.07 ng/ml

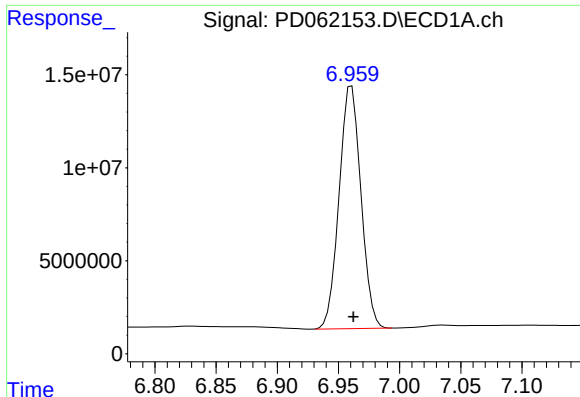

#20 Methoxychlor


R.T.: 6.961 min
Delta R.T.: -0.002 min
Response: 162263457
Conc: 343.41 ng/ml

Instrument :
ECD_D
ClientSampleId :

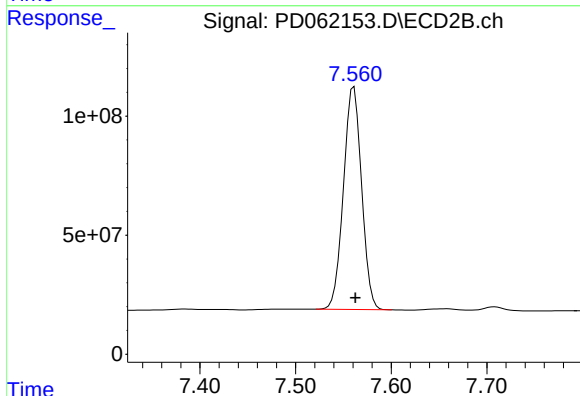


#20 Methoxychlor

R.T.: 7.561 min
Delta R.T.: -0.001 min
Response: 1235895554
Conc: 274.16 ng/ml

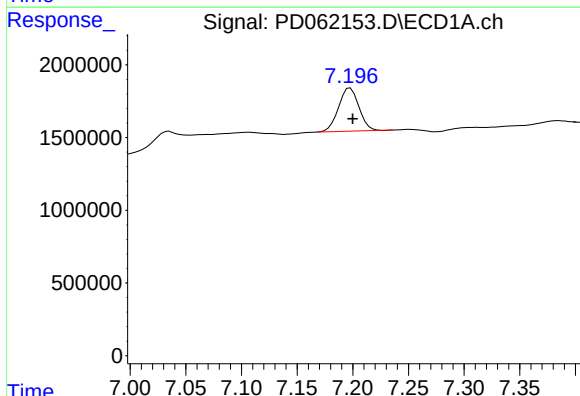


#21 Endrin ketone

R.T.: 7.198 min
Delta R.T.: -0.002 min
Response: 3809069
Conc: 2.98 ng/ml

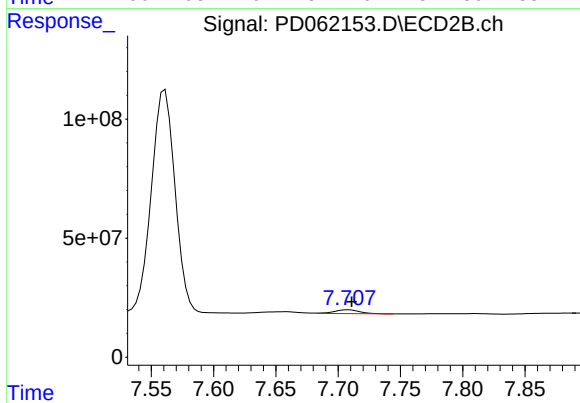

#21 Endrin ketone


R.T.: 7.708 min
Delta R.T.: -0.003 min
Response: 22395449
Conc: 2.21 ng/ml

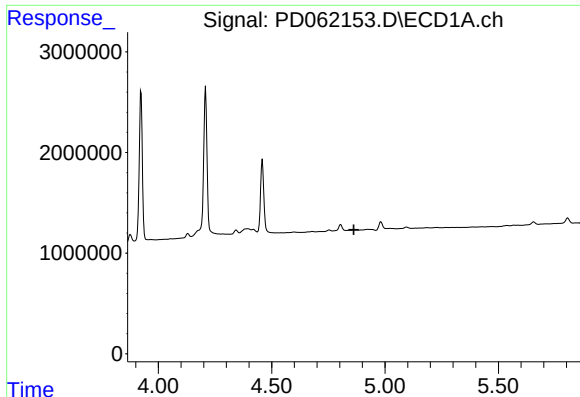

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.862 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

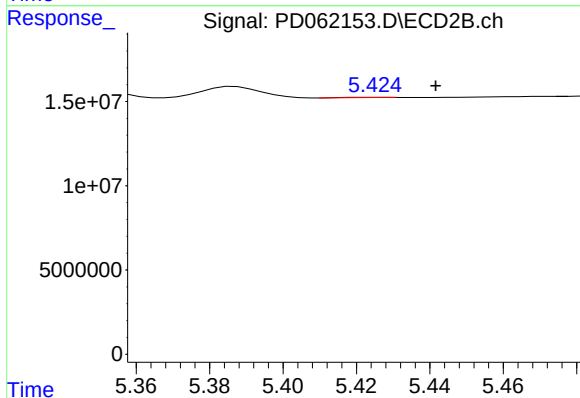


#24 Chlordane-2

R.T.: 5.425 min
Delta R.T.: -0.016 min
Response: 302222
Conc: 0.79 ng/ml

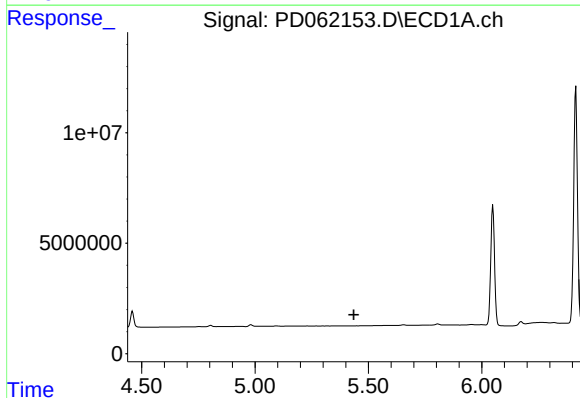

#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.435 min
Response: 0
Conc: N.D.

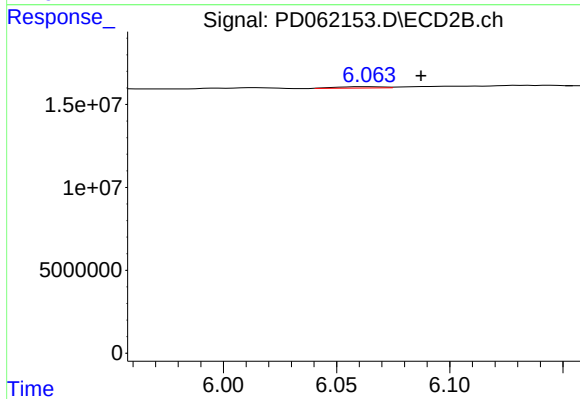

#25 Chlordane-3

R.T.: 6.064 min
Delta R.T.: -0.023 min
Response: 1119775
Conc: 0.68 ng/ml

