

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041421\
 Data File : PD062157.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2021 11:24
 Operator : AR\AJ
 Sample : M1998-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-5A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 15:43:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.980	10878962	106.2E6	12.993	12.225
28)	SA Decachlor...	8.256	9.038	15770029	101.0E6	12.817	10.699
Target Compounds							
12)	B 4,4'-DDE	5.655	6.315	78073925	733.0E6	69.481	63.604



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041421\
Data File : PD062157.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2021 11:24
Operator : AR\AJ
Sample : M1998-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SB-5A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 15:43:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

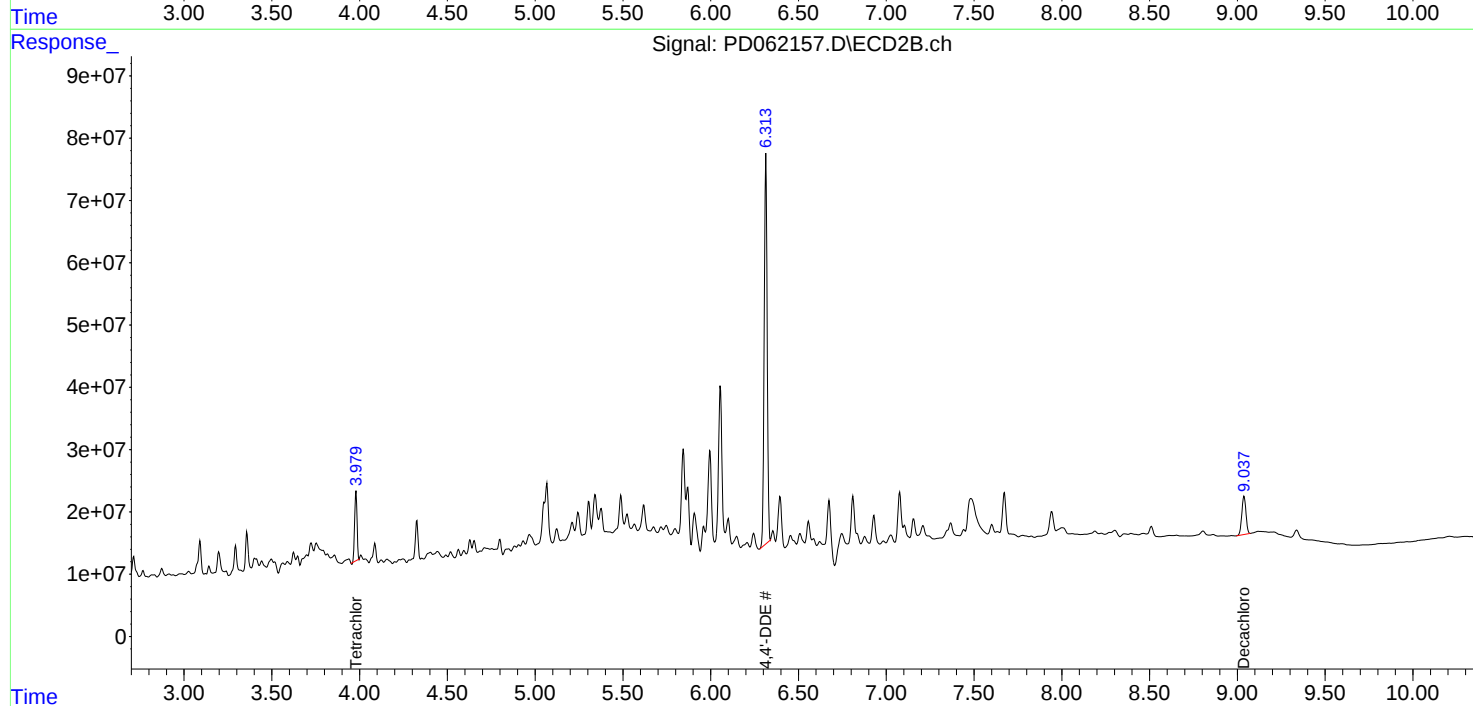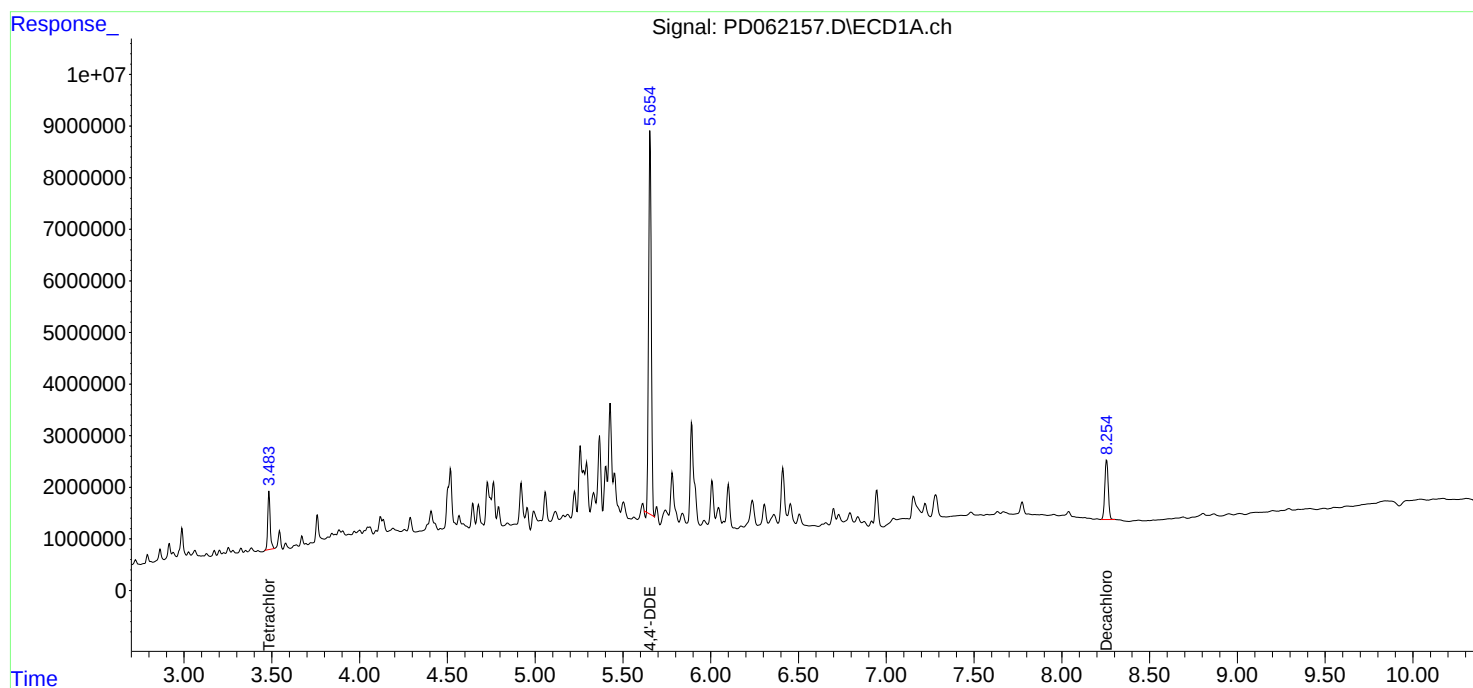


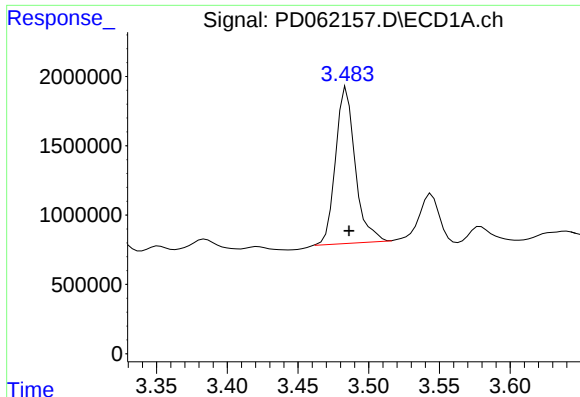

#1 Tetrachloro-m-xylene


R.T.: 3.484 min
Delta R.T.: -0.002 min
Response: 10878962
Conc: 12.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-5A

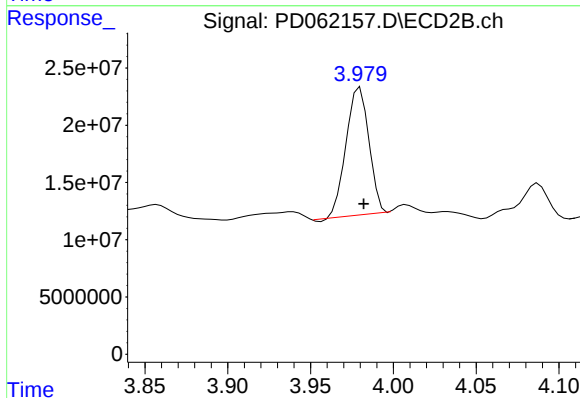


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 106223037
Conc: 12.23 ng/ml

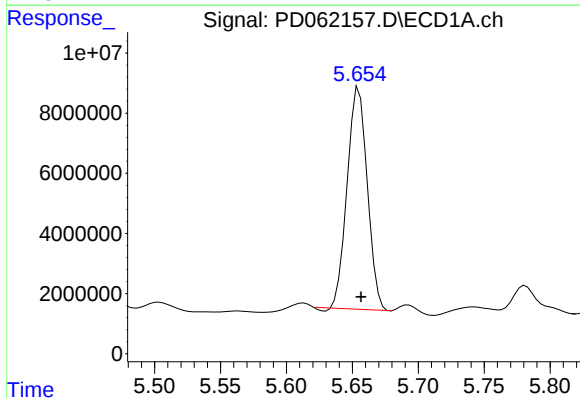


#12 4,4'-DDE

R.T.: 5.655 min
Delta R.T.: -0.002 min
Response: 78073925
Conc: 69.48 ng/ml

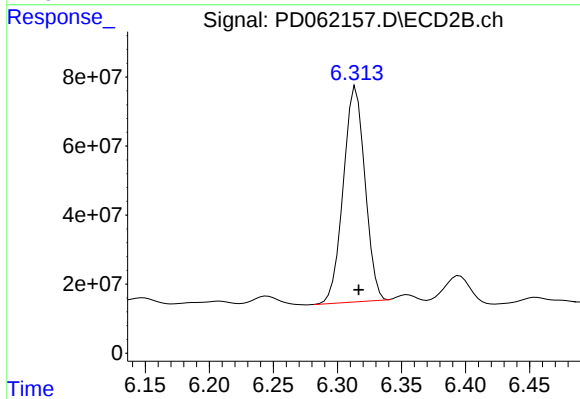

#12 4,4'-DDE


R.T.: 6.315 min
Delta R.T.: -0.002 min
Response: 732976634
Conc: 63.60 ng/ml

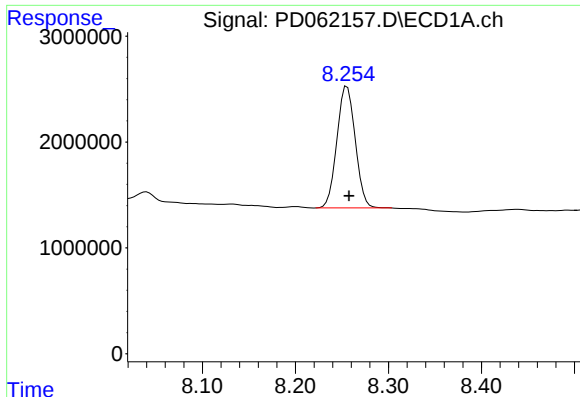

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.002 min
Response: 15770029
Conc: 12.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-5A

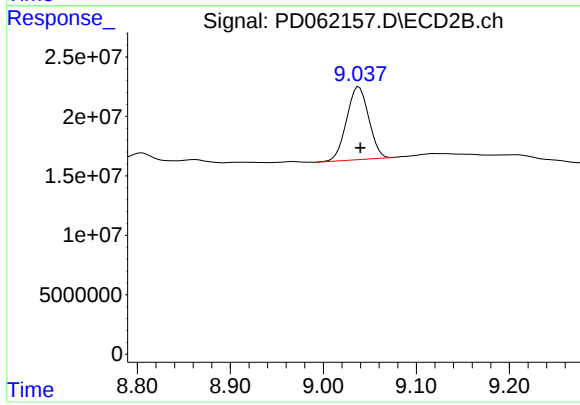

#28 Decachlorobiphenyl

R.T.: 9.038 min
Delta R.T.: -0.002 min
Response: 101005981
Conc: 10.70 ng/ml