

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041421\
 Data File : PD062160.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Apr 2021 13:05
 Operator : AR\AJ
 Sample : M1998-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-4B

Manual Integrations
 APPROVED

Ankita
 4/15/2021 11:16:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 15:44:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 30 04:47:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.487	3.980	11127015	122.1E6	13.289	14.051
28) SA Decachlor...	8.259	9.040	13013019	85934877	10.576	9.103
Target Compounds						
12) B 4,4'-DDE	5.657	6.315	24068425	260.4E6	21.419m	22.597
17) MA 4,4'-DDT	6.418	7.105	39844815	334.6E6	44.236	35.026

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD041421\
Data File : PD062160.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Apr 2021 13:05
Operator : AR\AJ
Sample : M1998-06
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
SB-4B


Manual Integrations
APPROVED

Ankita
4/15/2021 11:16:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 15:44:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD032921.M
Quant Title : GC Extractables
QLast Update : Tue Mar 30 04:47:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

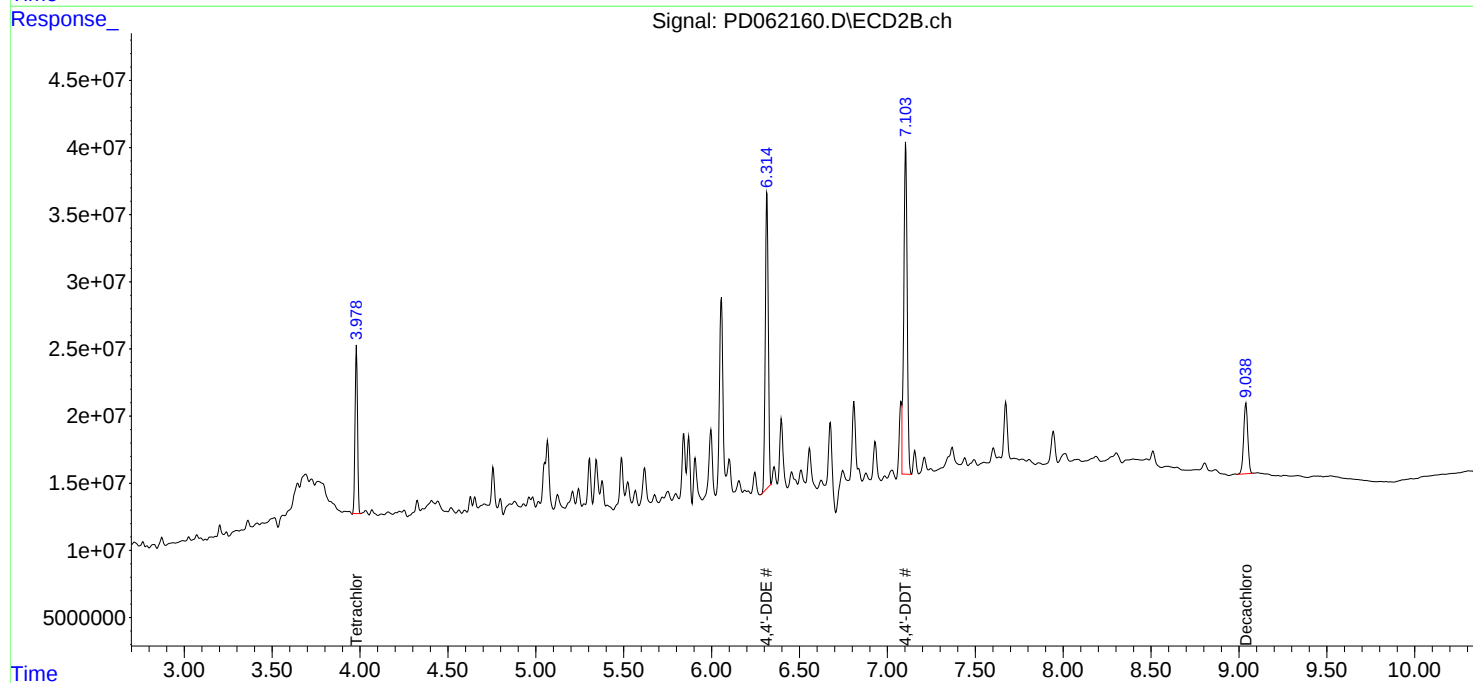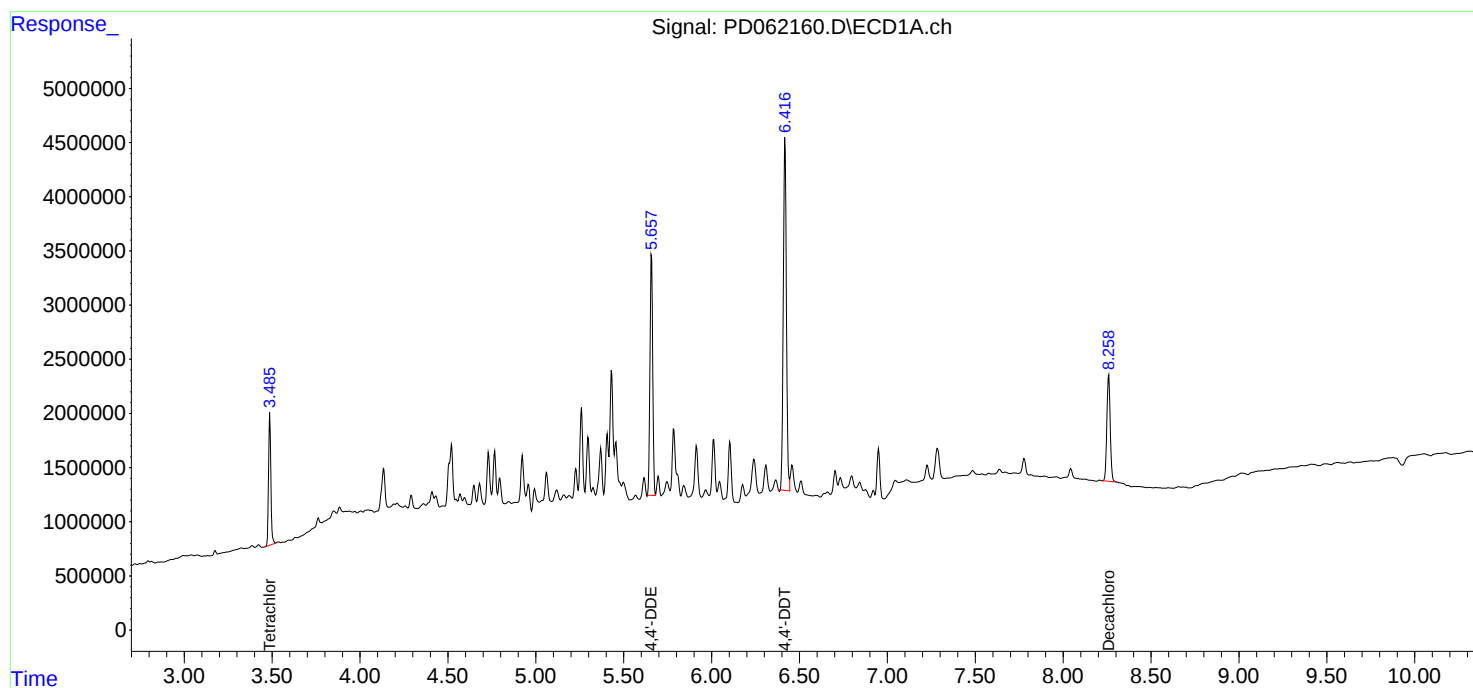

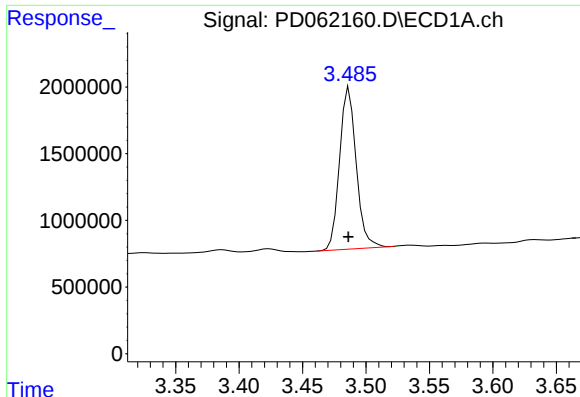


#1 Tetrachloro-m-xylene

R.T.: 3.487 min
Delta R.T.: 0.000 min
Response: 11127015
Conc: 13.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-4B


Manual Integrations
APPROVED

Ankita
4/15/2021 11:16:57 AM

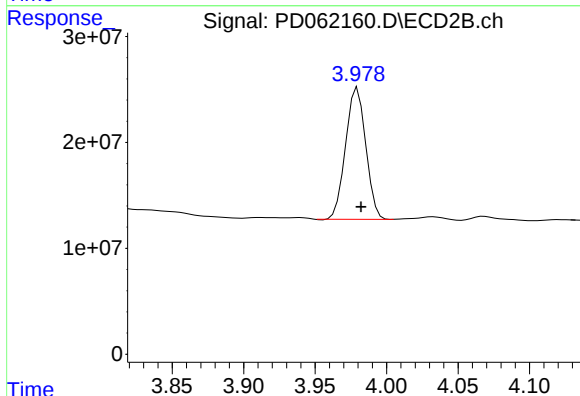


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 122091274
Conc: 14.05 ng/ml

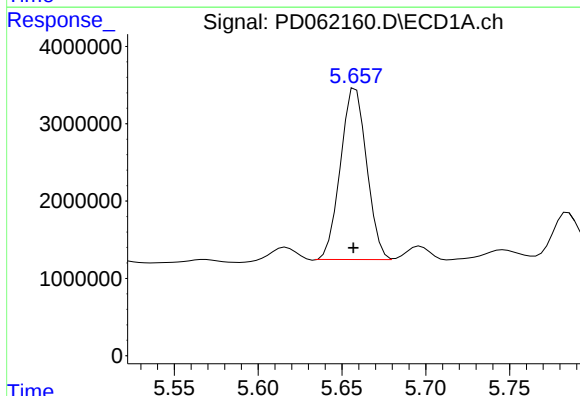


#12 4,4'-DDE

R.T.: 5.657 min
Delta R.T.: 0.000 min
Response: 24068425
Conc: 21.42 ng/ml m

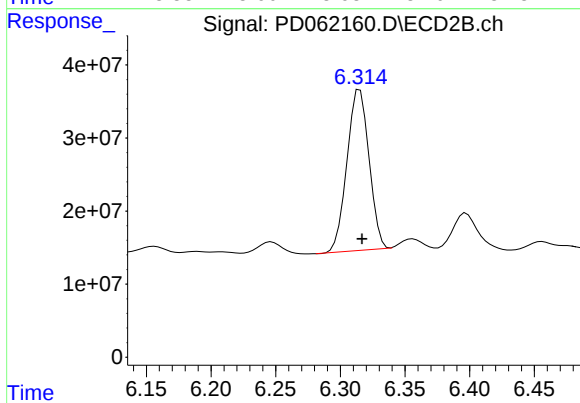

#12 4,4'-DDE

R.T.: 6.315 min
Delta R.T.: -0.002 min
Response: 260407065
Conc: 22.60 ng/ml

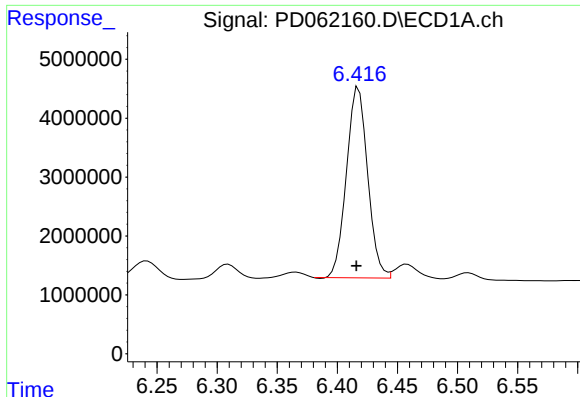


#17 4,4'-DDT

R.T.: 6.418 min
Delta R.T.: 0.002 min
Response: 39844815
Conc: 44.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-4B


Manual Integrations
APPROVED

Ankita
4/15/2021 11:16:57 AM

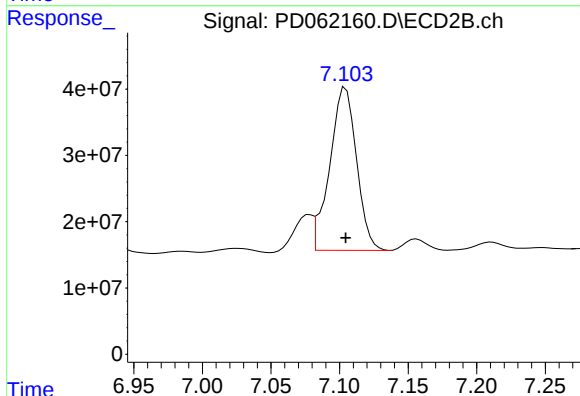


#17 4,4'-DDT

R.T.: 7.105 min
Delta R.T.: 0.000 min
Response: 334556028
Conc: 35.03 ng/ml

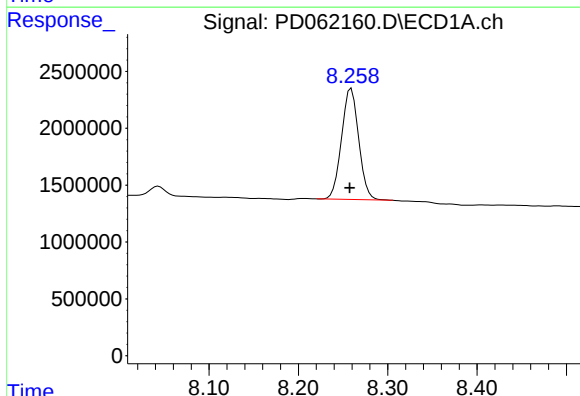

#28 Decachlorobiphenyl

R.T.: 8.259 min
Delta R.T.: 0.002 min
Response: 13013019
Conc: 10.58 ng/ml

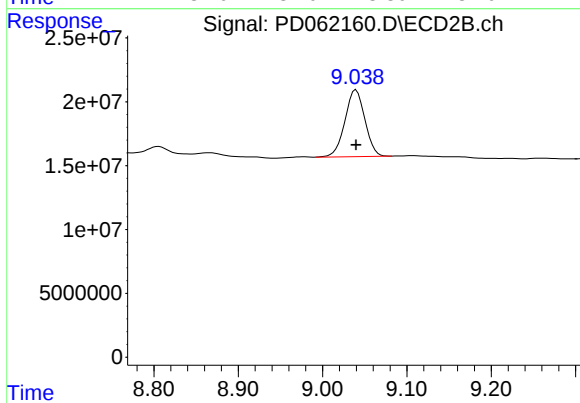

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.000 min
Response: 85934877
Conc: 9.10 ng/ml