

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042325\
 Data File : PD088251.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2025 16:00
 Operator : AR\AJ
 Sample : Q1858-02MSD
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COMP-2MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 01:34:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041825.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 19 06:32:27 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.552	2.883	34755500	259.5E6	17.400	17.746
28)	SA Decachlor...	9.074	8.076	50893408	239.9E6	15.384	12.980
Target Compounds							
2)	A alpha-BHC	4.001	3.396	196.5E6	986.3E6	45.570	43.142
3)	MA gamma-BHC...	4.332	3.732	188.4E6	876.8E6	44.981	40.707
4)	MA Heptachlor	4.931	4.086	158.8E6	800.7E6	39.322	37.417
5)	MB Aldrin	5.273	4.372	180.9E6	867.2E6	45.792	41.685
6)	B beta-BHC	4.516	4.028	65918350	420.8E6	40.606	45.468
7)	B delta-BHC	4.765	4.265	190.7E6	895.3E6	46.232	42.107
8)	B Heptachlo...	5.692	4.876	159.5E6	783.3E6	44.627	41.458
9)	A Endosulfan I	6.076	5.251	153.5E6	696.4E6	45.442	38.662
10)	B gamma-Chl...	5.947	5.129	162.4E6	875.7E6	44.831	43.148
11)	B alpha-Chl...	6.028	5.194	162.3E6	827.2E6	44.952	42.200
12)	B 4,4'-DDE	6.197	5.379	132.9E6	782.6E6	40.301	39.739
13)	MA Dieldrin	6.348	5.516	160.8E6	826.7E6	45.049	41.474
14)	MA Endrin	6.575	5.792	128.1E6	733.8E6	42.942	40.313
15)	B Endosulfa...	6.786	6.084	131.0E6	870.1E6	41.889	49.660
16)	A 4,4'-DDD	6.706	5.933	114.2E6	650.2E6	45.406	39.682
17)	MA 4,4'-DDT	7.021	6.187	103.5E6	670.8E6	37.278	39.420
18)	B Endrin al...	6.915	6.262	101.1E6	574.3E6	43.794	43.176
19)	B Endosulfa...	7.150	6.485	121.5E6	638.0E6	42.249	37.240
20)	A Methoxychlor	7.493	6.757	45505101	293.5E6	30.346	32.182
21)	B Endrin ke...	7.630	6.994	118.9E6	622.1E6	38.536	33.258
22)	Mirex	8.114	7.188	77837651	502.1E6	33.146	33.875
23)	Chlordane-1	4.688f	3.905	3899987	43339662	23.473	54.060 #
24)	Chlordane-2	5.224	4.508	100258	3795117	0.602	4.598 #
25)	Chlordane-3	5.947	5.129	162.4E6	875.7E6	240.731	346.271 #
26)	Chlordane-4	6.028	5.194	162.3E6	827.2E6	199.011	386.889 #
27)	Chlordane-5	6.869	6.084	670898	870.1E6	4.938	901.196 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042325\
Data File : PD088251.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2025 16:00
Operator : AR\AJ
Sample : Q1858-02MSD
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
COMP-2MSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 01:34:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041825.M
Quant Title : GC Extractables
QLast Update : Sat Apr 19 06:32:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

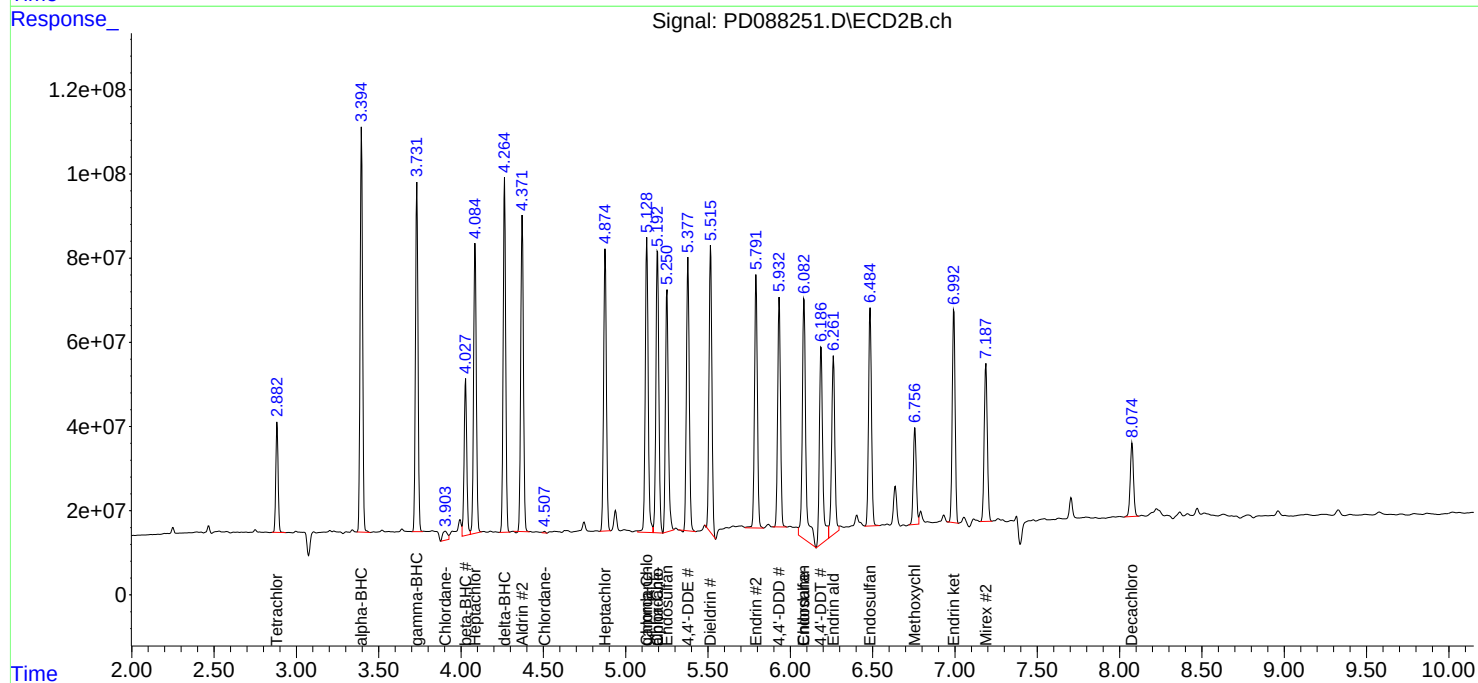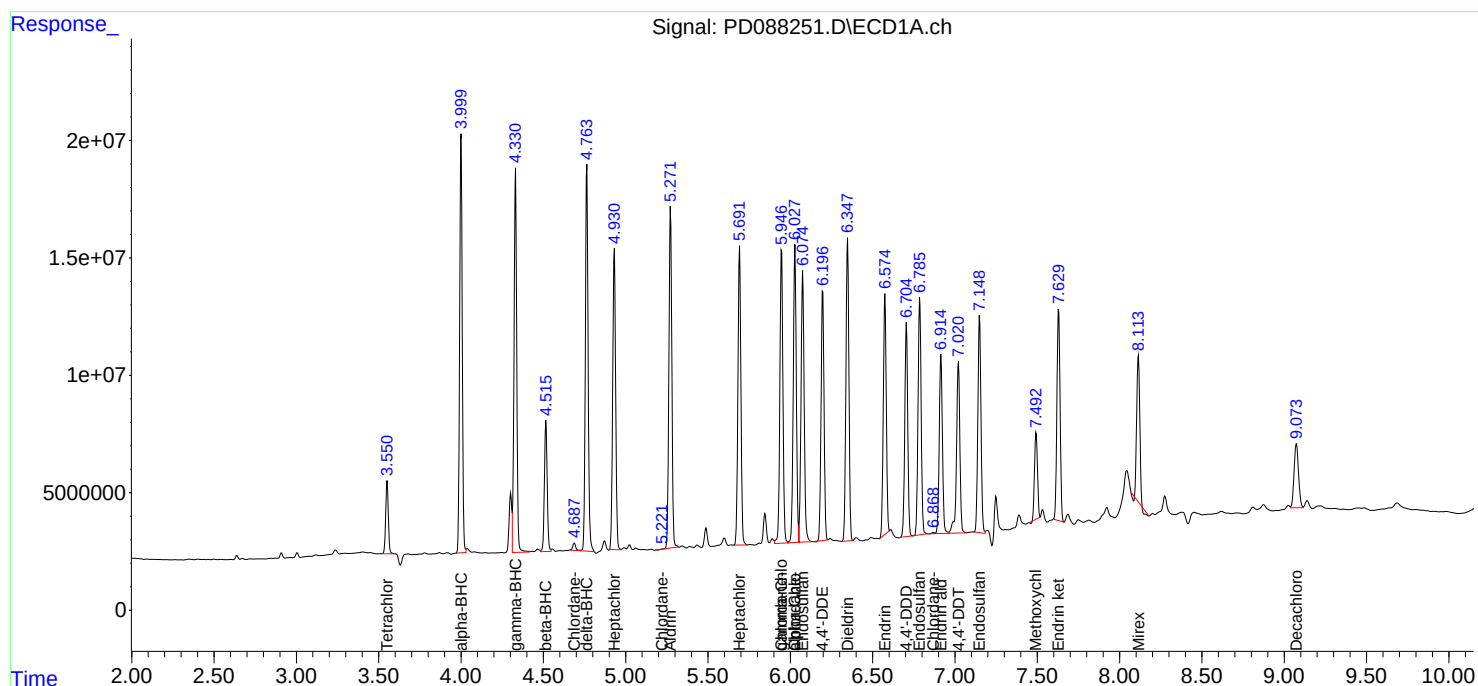


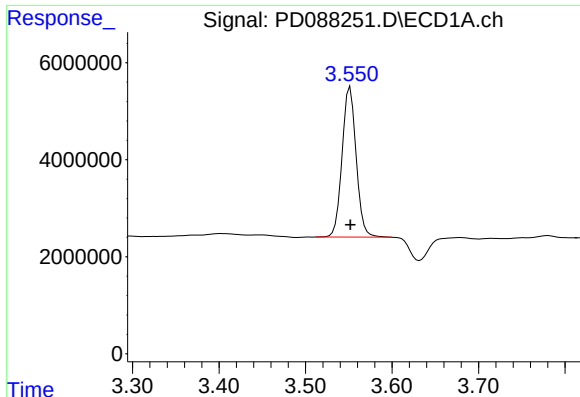

#1 Tetrachloro-m-xylene


R.T.: 3.552 min
Delta R.T.: 0.000 min
Response: 34755500
Conc: 17.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2MSD

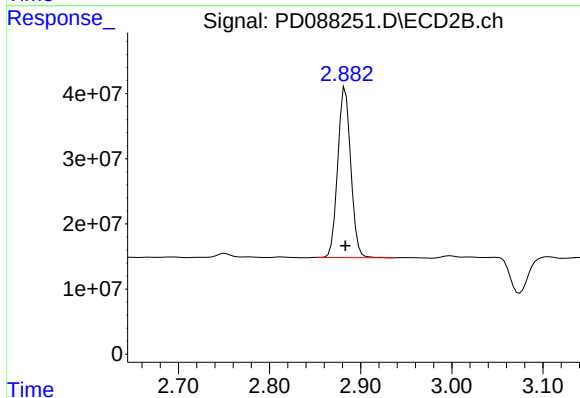


#1 Tetrachloro-m-xylene

R.T.: 2.883 min
Delta R.T.: 0.000 min
Response: 259477904
Conc: 17.75 ng/ml

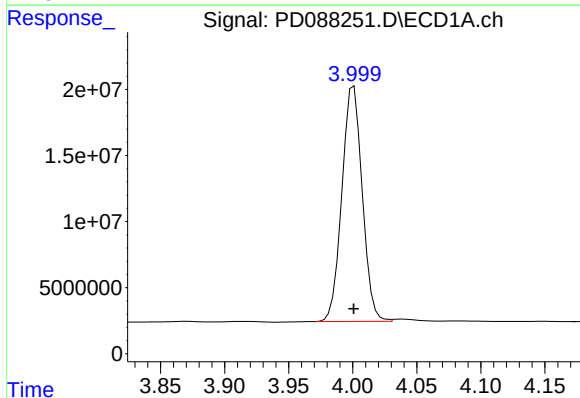


#2 alpha-BHC

R.T.: 4.001 min
Delta R.T.: 0.000 min
Response: 196496810
Conc: 45.57 ng/ml

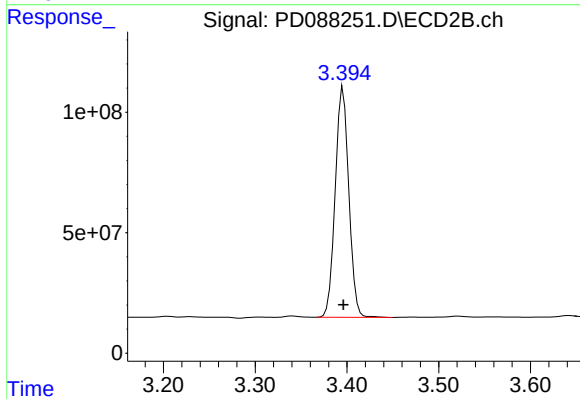

#2 alpha-BHC


R.T.: 3.396 min
Delta R.T.: 0.000 min
Response: 986296102
Conc: 43.14 ng/ml

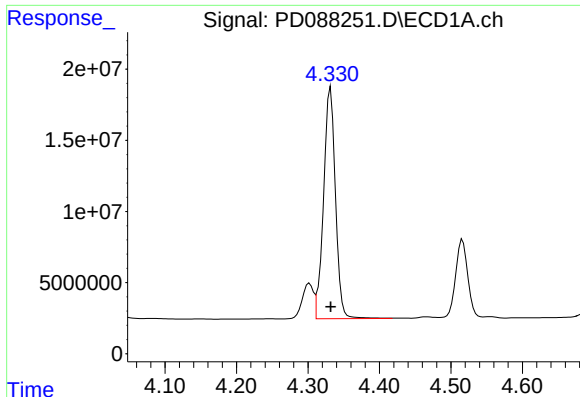

#3 gamma-BHC (Lindane)


R.T.: 4.332 min
Delta R.T.: 0.000 min
Response: 188359668
Conc: 44.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2MSD

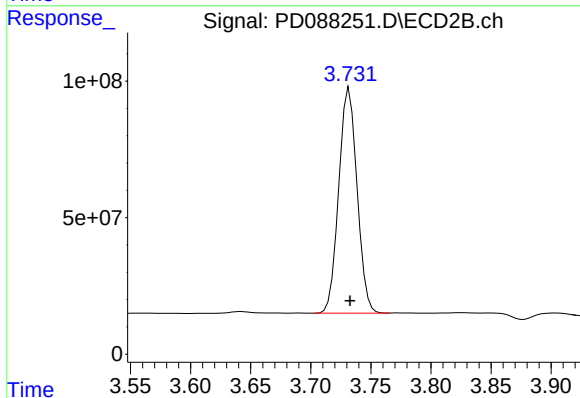


#3 gamma-BHC (Lindane)

R.T.: 3.732 min
Delta R.T.: 0.000 min
Response: 876772496
Conc: 40.71 ng/ml

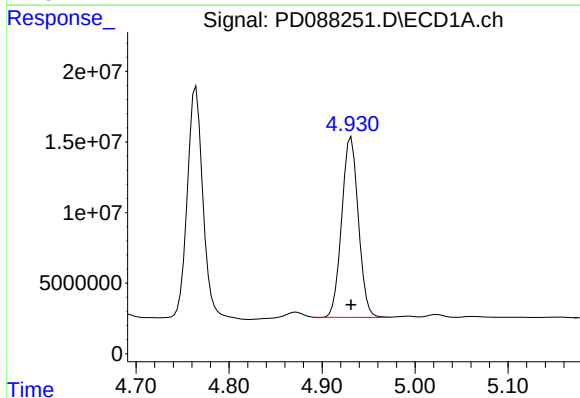


#4 Heptachlor

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 158818617
Conc: 39.32 ng/ml

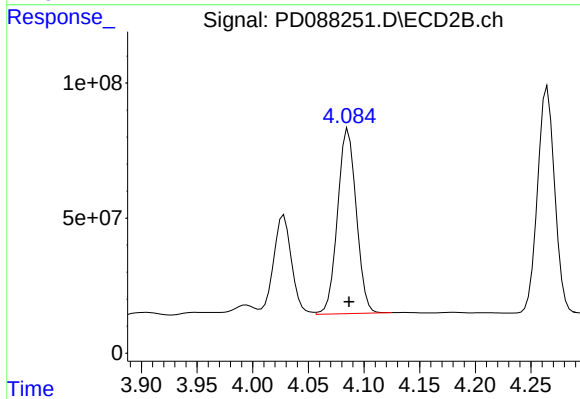

#4 Heptachlor


R.T.: 4.086 min
Delta R.T.: 0.000 min
Response: 800650164
Conc: 37.42 ng/ml

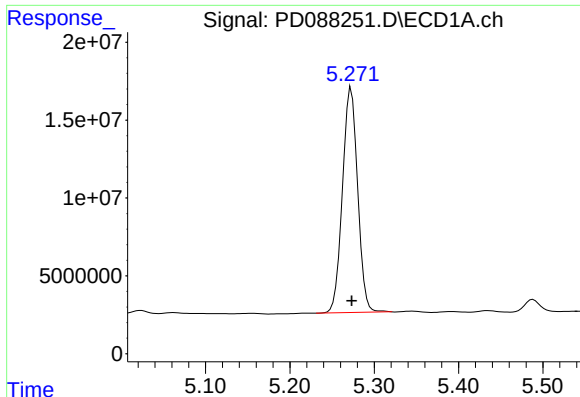

#5 Aldrin


R.T.: 5.273 min
Delta R.T.: 0.000 min
Response: 180860790
Conc: 45.79 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2MSD

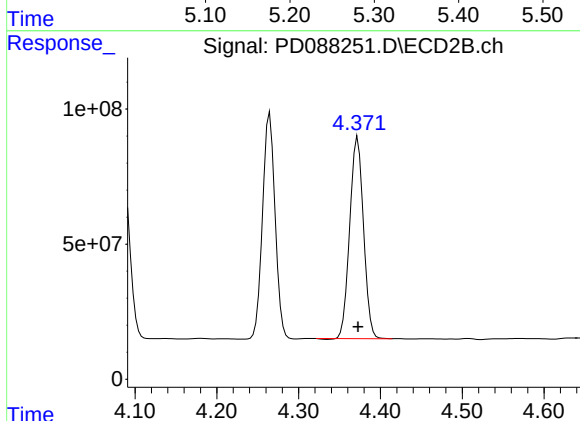


#5 Aldrin

R.T.: 4.372 min
Delta R.T.: 0.000 min
Response: 867165556
Conc: 41.69 ng/ml

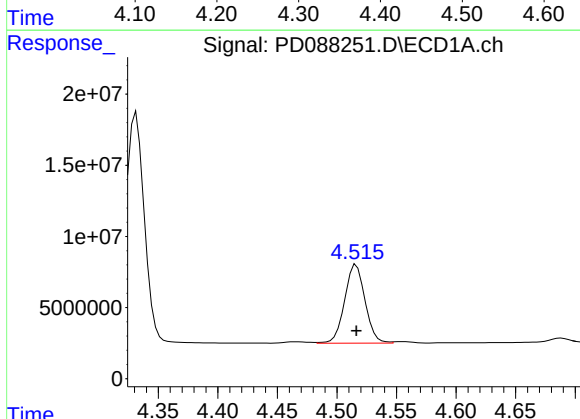


#6 beta-BHC

R.T.: 4.516 min
Delta R.T.: 0.000 min
Response: 65918350
Conc: 40.61 ng/ml

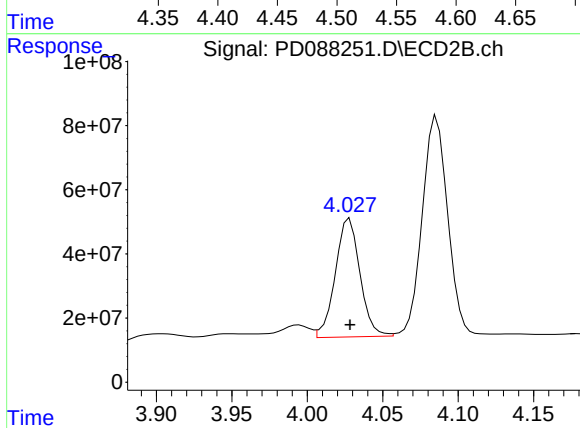

#6 beta-BHC


R.T.: 4.028 min
Delta R.T.: 0.000 min
Response: 420770194
Conc: 45.47 ng/ml

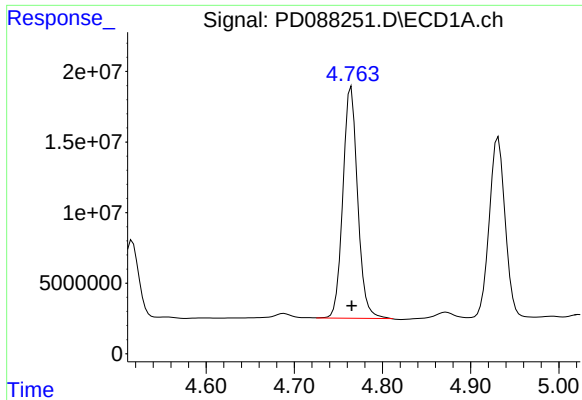

#7 delta-BHC


R.T.: 4.765 min
Delta R.T.: 0.000 min
Response: 190705329
Conc: 46.23 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2MSD

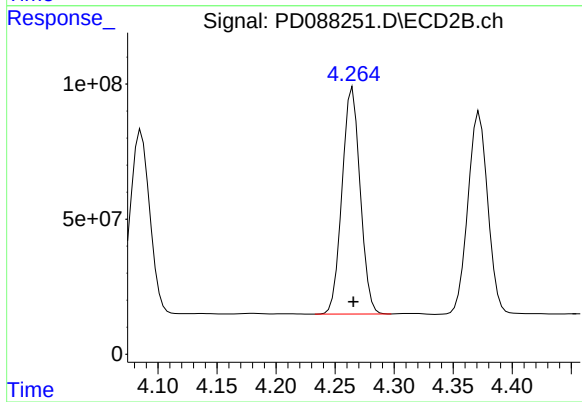


#7 delta-BHC

R.T.: 4.265 min
Delta R.T.: 0.000 min
Response: 895263477
Conc: 42.11 ng/ml

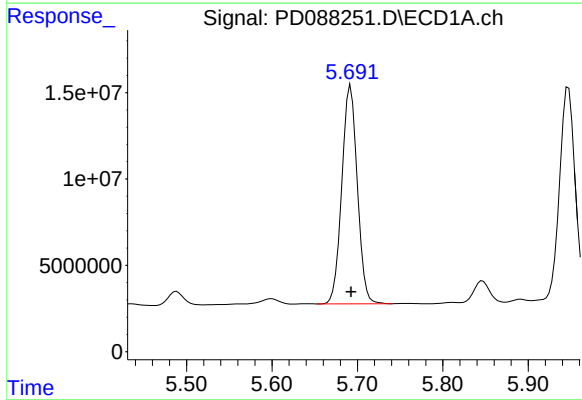


#8 Heptachlor epoxide

R.T.: 5.692 min
Delta R.T.: 0.000 min
Response: 159493414
Conc: 44.63 ng/ml

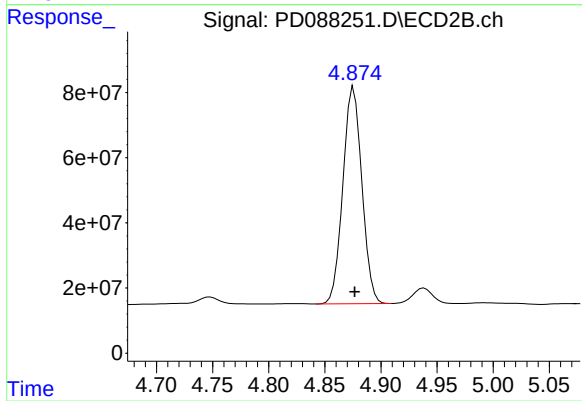

#8 Heptachlor epoxide


R.T.: 4.876 min
Delta R.T.: 0.000 min
Response: 783317476
Conc: 41.46 ng/ml

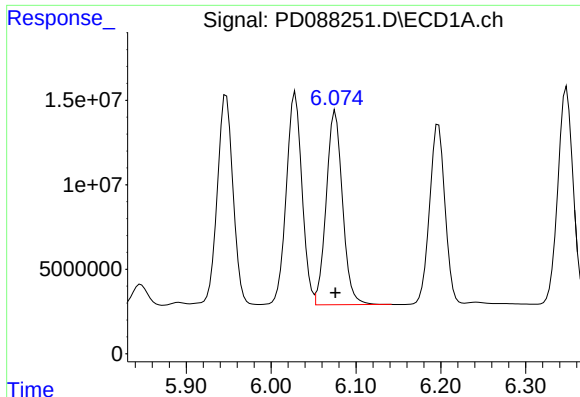

#9 Endosulfan I


R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 153464801
Conc: 45.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2MSD

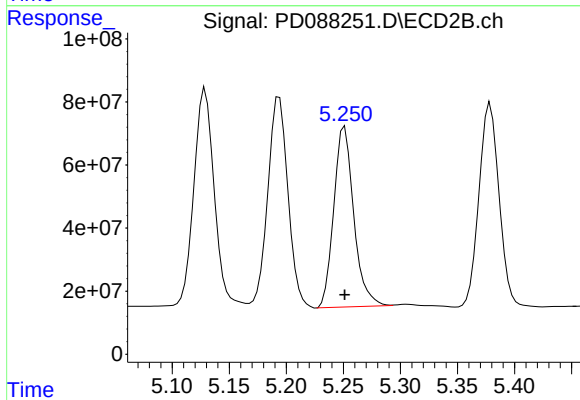


#9 Endosulfan I

R.T.: 5.251 min
Delta R.T.: 0.000 min
Response: 696401029
Conc: 38.66 ng/ml

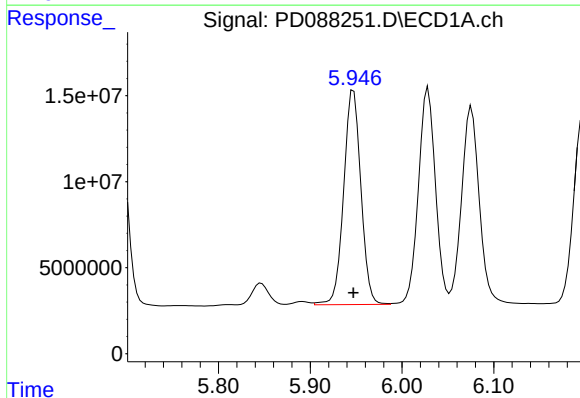


#10 gamma-Chlordane

R.T.: 5.947 min
Delta R.T.: 0.000 min
Response: 162380396
Conc: 44.83 ng/ml

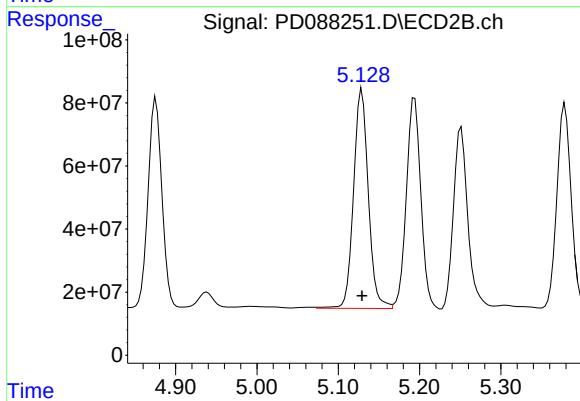

#10 gamma-Chlordane


R.T.: 5.129 min
Delta R.T.: 0.000 min
Response: 875735248
Conc: 43.15 ng/ml

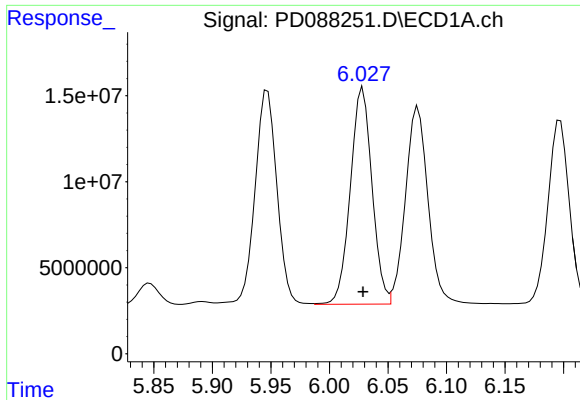

#11 alpha-Chlordane


R.T.: 6.028 min
Delta R.T.: 0.000 min
Response: 162259147
Conc: 44.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2MSD

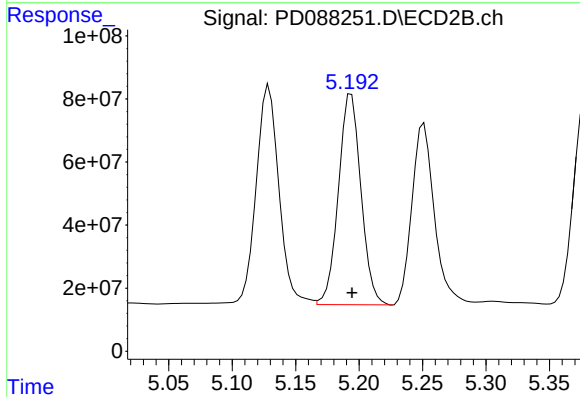


#11 alpha-Chlordane

R.T.: 5.194 min
Delta R.T.: 0.000 min
Response: 827228620
Conc: 42.20 ng/ml

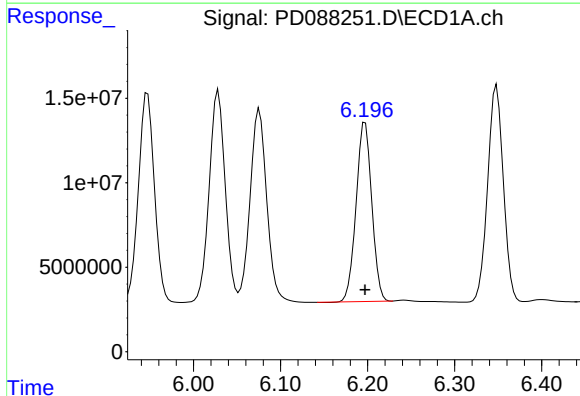


#12 4,4'-DDE

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 132923737
Conc: 40.30 ng/ml

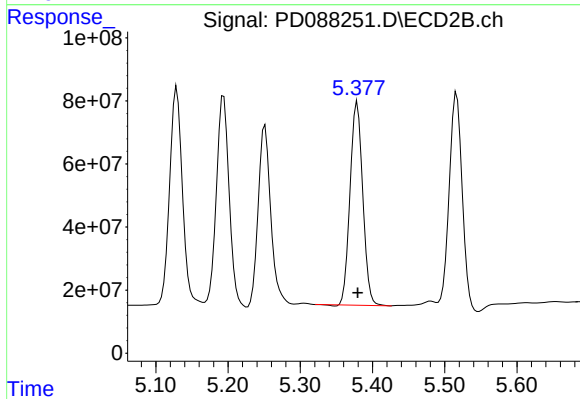

#12 4,4'-DDE


R.T.: 5.379 min
Delta R.T.: 0.000 min
Response: 782626872
Conc: 39.74 ng/ml

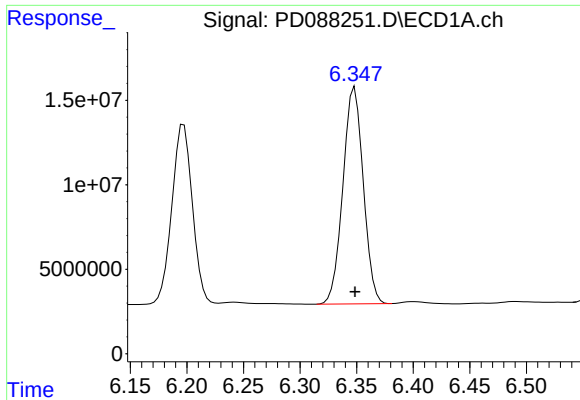

#13 Dieldrin


R.T.: 6.348 min
Delta R.T.: 0.000 min
Response: 160758873
Conc: 45.05 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2MSD

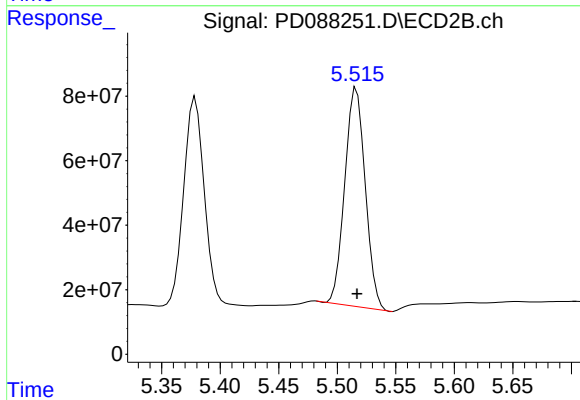


#13 Dieldrin

R.T.: 5.516 min
Delta R.T.: 0.000 min
Response: 826696744
Conc: 41.47 ng/ml

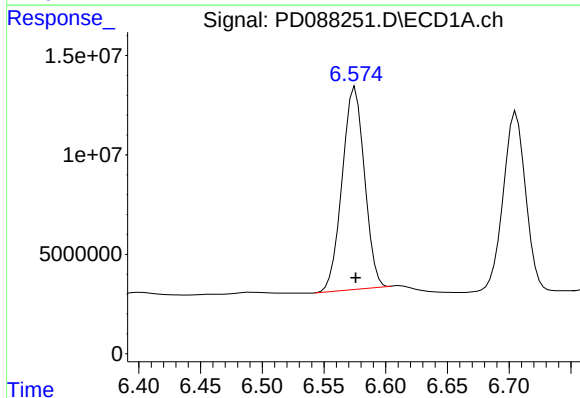


#14 Endrin

R.T.: 6.575 min
Delta R.T.: 0.000 min
Response: 128078507
Conc: 42.94 ng/ml

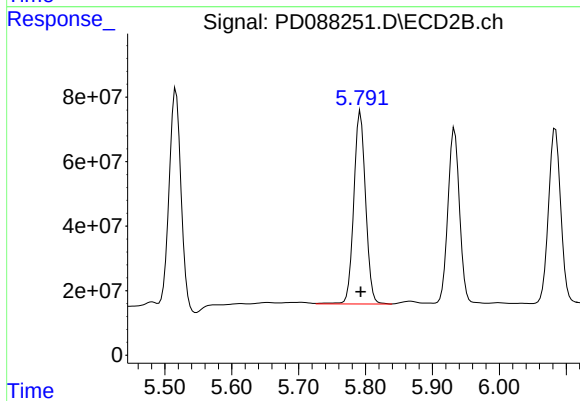

#14 Endrin


R.T.: 5.792 min
Delta R.T.: 0.000 min
Response: 733792077
Conc: 40.31 ng/ml

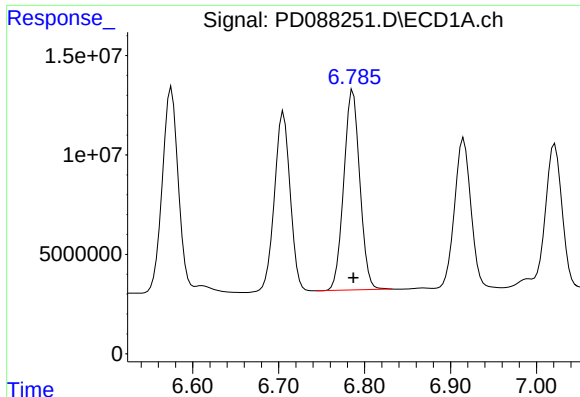

#15 Endosulfan II


R.T.: 6.786 min
Delta R.T.: 0.000 min
Response: 130954168
Conc: 41.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2MSD

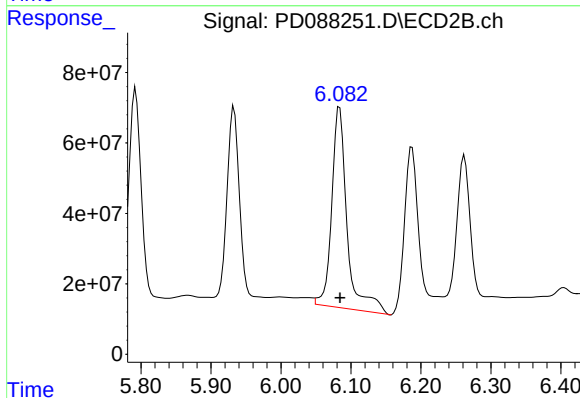


#15 Endosulfan II

R.T.: 6.084 min
Delta R.T.: 0.000 min
Response: 870127374
Conc: 49.66 ng/ml

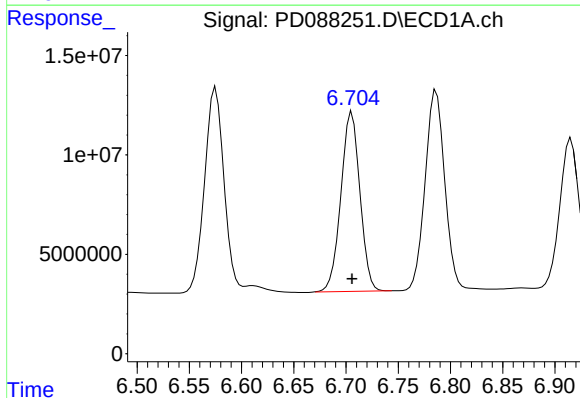


#16 4,4'-DDD

R.T.: 6.706 min
Delta R.T.: 0.000 min
Response: 114195151
Conc: 45.41 ng/ml

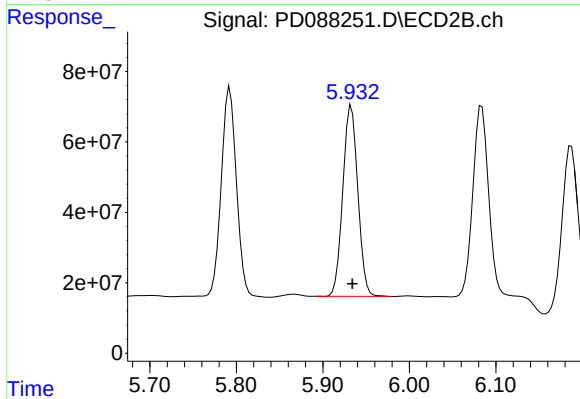

#16 4,4'-DDD


R.T.: 5.933 min
Delta R.T.: -0.001 min
Response: 650244172
Conc: 39.68 ng/ml

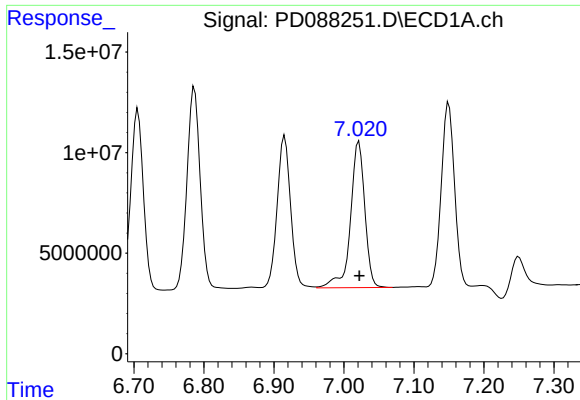

#17 4,4'-DDT


R.T.: 7.021 min
Delta R.T.: 0.000 min
Response: 103540636
Conc: 37.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2MSD

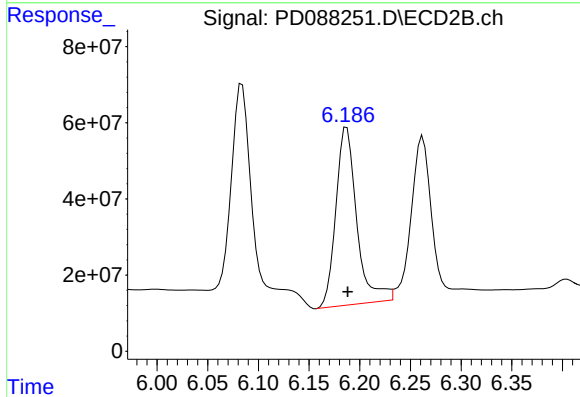


#17 4,4'-DDT

R.T.: 6.187 min
Delta R.T.: 0.000 min
Response: 670798809
Conc: 39.42 ng/ml

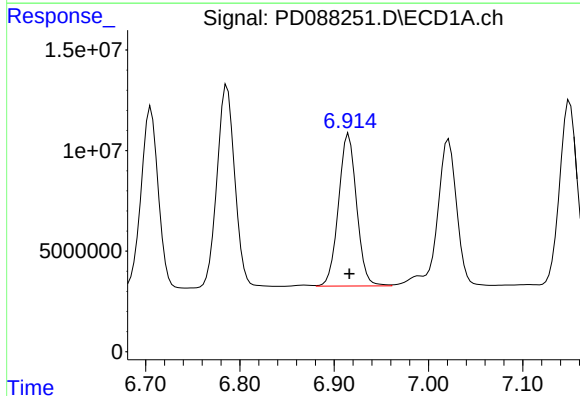


#18 Endrin aldehyde

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 101076625
Conc: 43.79 ng/ml

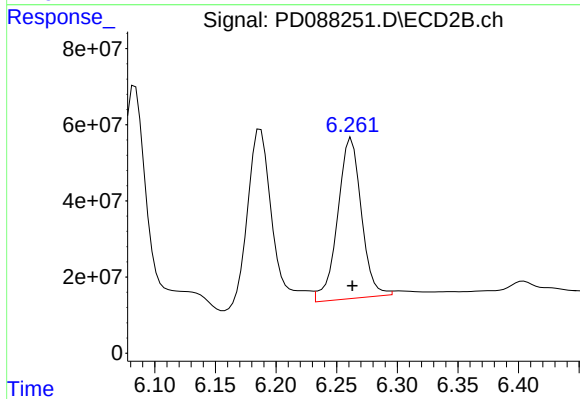

#18 Endrin aldehyde


R.T.: 6.262 min
Delta R.T.: 0.000 min
Response: 574289081
Conc: 43.18 ng/ml

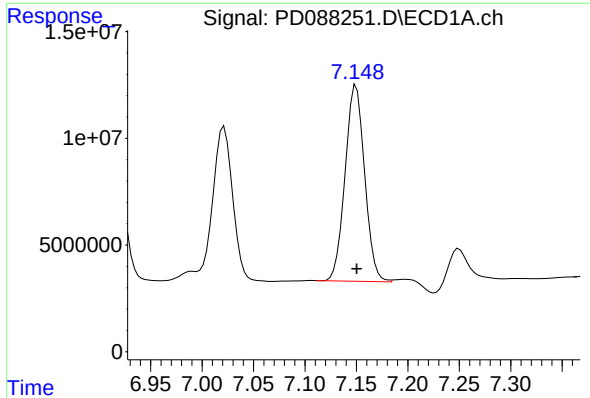

#19 Endosulfan Sulfate


R.T.: 7.150 min
Delta R.T.: 0.000 min
Response: 121501984
Conc: 42.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2MSD

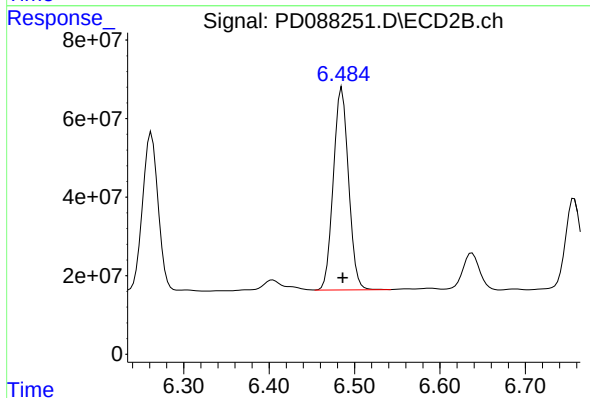


#19 Endosulfan Sulfate

R.T.: 6.485 min
Delta R.T.: 0.000 min
Response: 638038365
Conc: 37.24 ng/ml

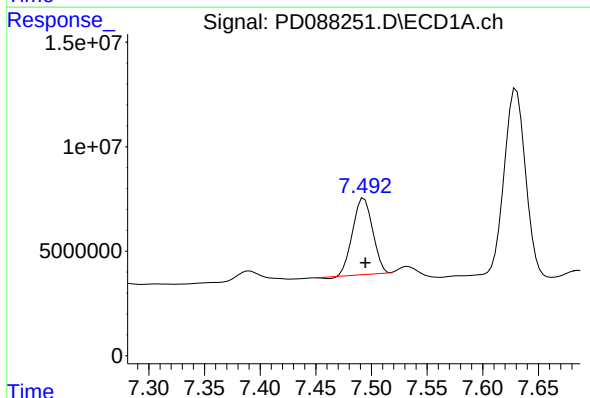


#20 Methoxychlor

R.T.: 7.493 min
Delta R.T.: -0.001 min
Response: 45505101
Conc: 30.35 ng/ml

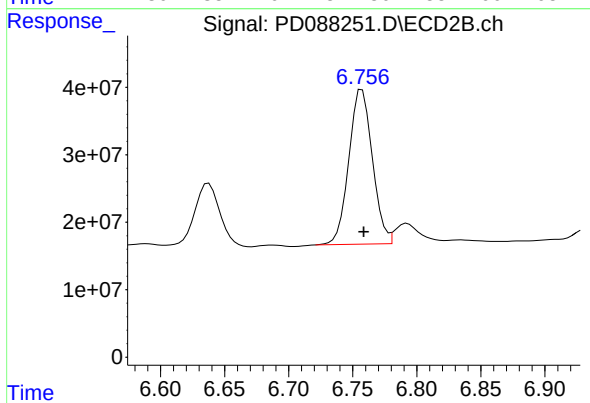

#20 Methoxychlor


R.T.: 6.757 min
Delta R.T.: -0.001 min
Response: 293532050
Conc: 32.18 ng/ml

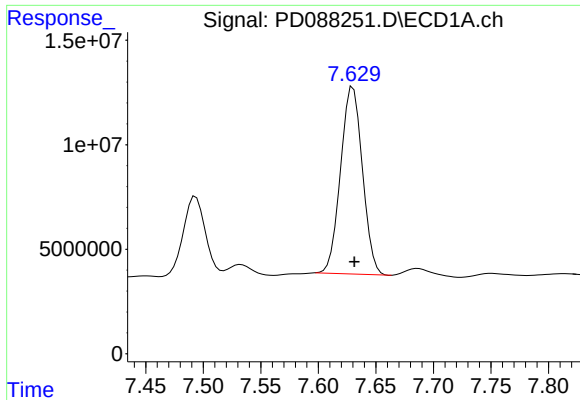

#21 Endrin ketone


R.T.: 7.630 min
Delta R.T.: -0.001 min
Response: 118944753
Conc: 38.54 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2MSD

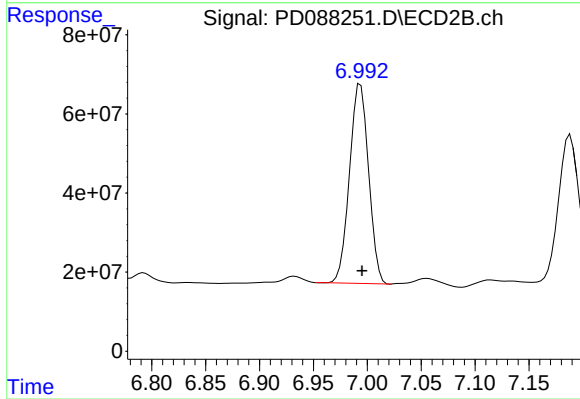


#21 Endrin ketone

R.T.: 6.994 min
Delta R.T.: -0.001 min
Response: 622061027
Conc: 33.26 ng/ml

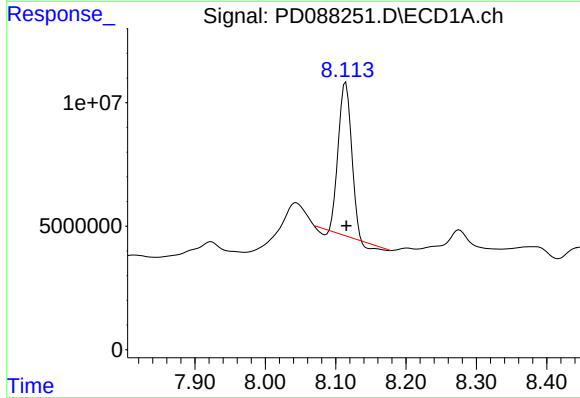


#22 Mirex

R.T.: 8.114 min
Delta R.T.: 0.000 min
Response: 77837651
Conc: 33.15 ng/ml

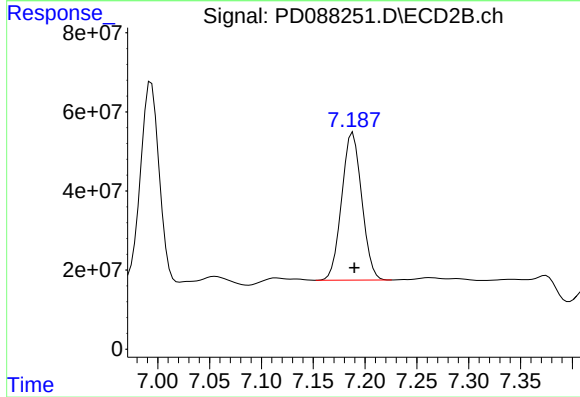

#22 Mirex


R.T.: 7.188 min
Delta R.T.: -0.001 min
Response: 502063025
Conc: 33.88 ng/ml

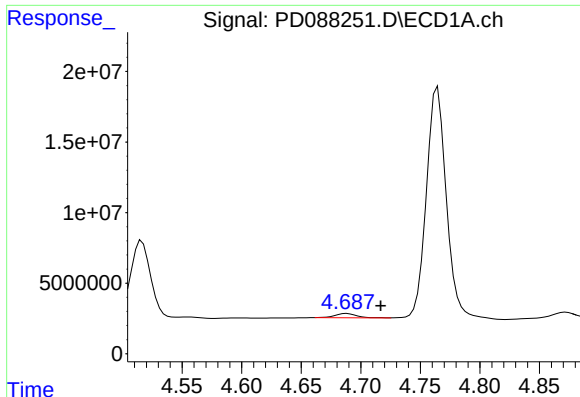

#23 Chlordane-1


R.T.: 4.688 min
Delta R.T.: -0.028 min
Response: 3899987
Conc: 23.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2MSD

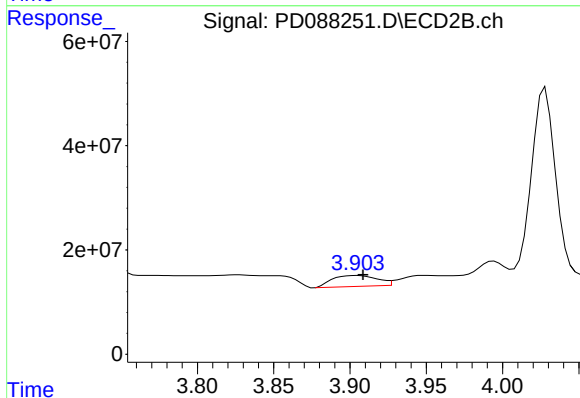


#23 Chlordane-1

R.T.: 3.905 min
Delta R.T.: -0.004 min
Response: 43339662
Conc: 54.06 ng/ml

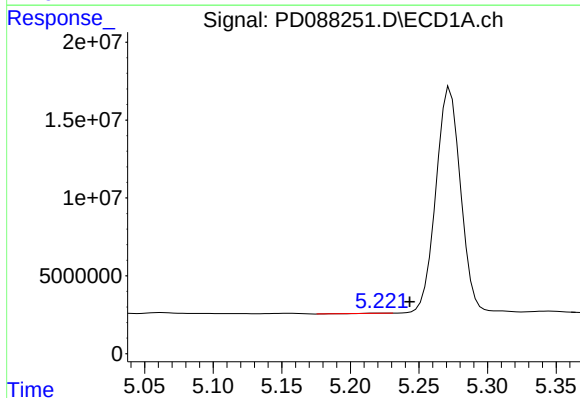


#24 Chlordane-2

R.T.: 5.224 min
Delta R.T.: -0.019 min
Response: 100258
Conc: 0.60 ng/ml

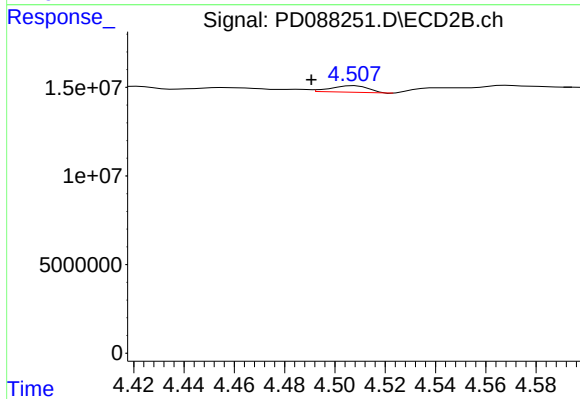

#24 Chlordane-2


R.T.: 4.508 min
Delta R.T.: 0.017 min
Response: 3795117
Conc: 4.60 ng/ml

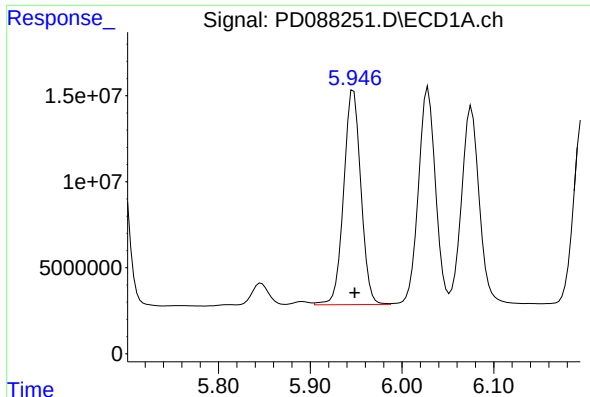

#25 Chlordane-3


R.T.: 5.947 min
Delta R.T.: -0.001 min
Response: 162380396
Conc: 240.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2MSD

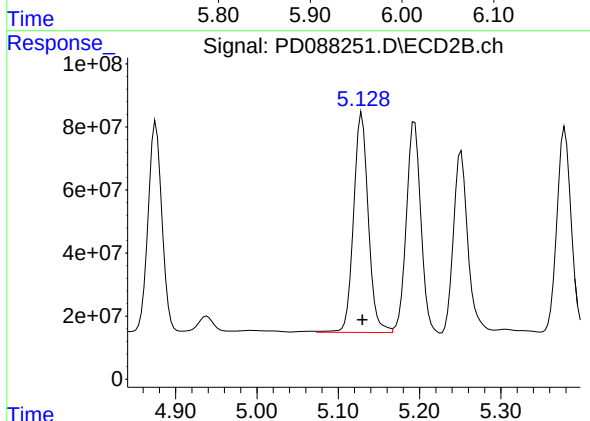


#25 Chlordane-3

R.T.: 5.129 min
Delta R.T.: 0.000 min
Response: 875735248
Conc: 346.27 ng/ml

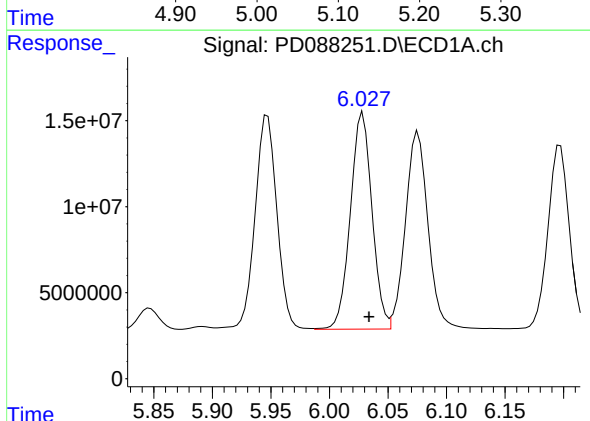


#26 Chlordane-4

R.T.: 6.028 min
Delta R.T.: -0.005 min
Response: 162259147
Conc: 199.01 ng/ml

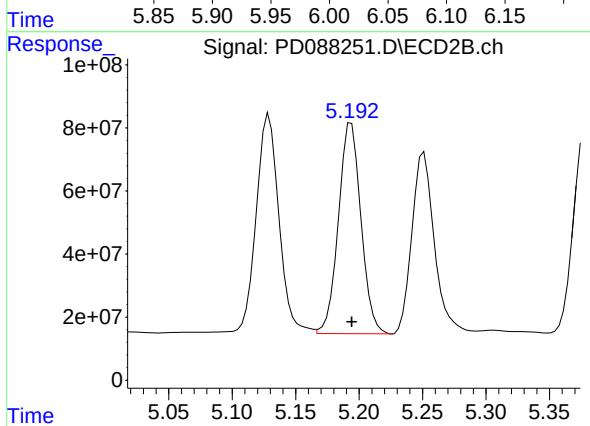

#26 Chlordane-4


R.T.: 5.194 min
Delta R.T.: 0.000 min
Response: 827228620
Conc: 386.89 ng/ml

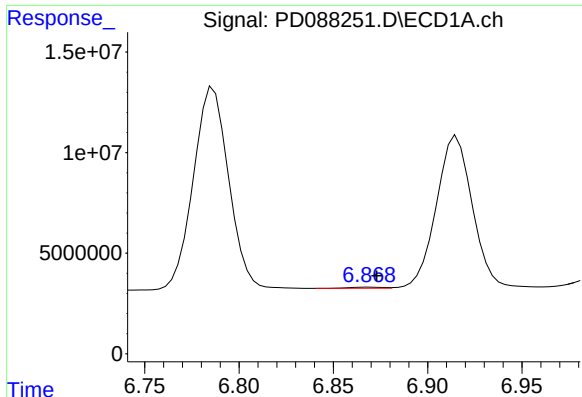

#27 Chlordane-5


R.T.: 6.869 min
Delta R.T.: -0.004 min
Response: 670898
Conc: 4.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2MSD

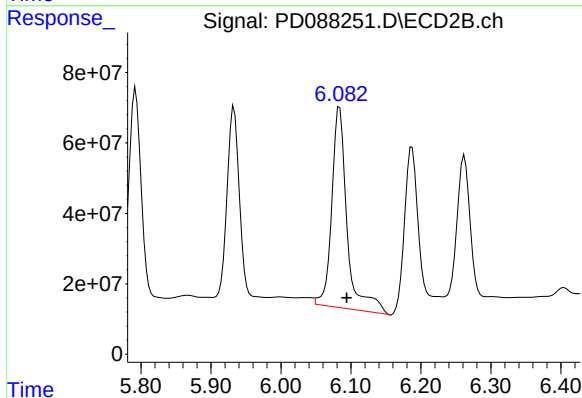


#27 Chlordane-5

R.T.: 6.084 min
Delta R.T.: -0.010 min
Response: 870127374
Conc: 901.20 ng/ml

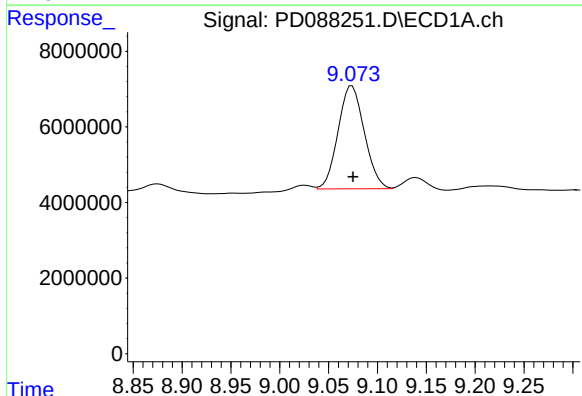

#28 Decachlorobiphenyl

R.T.: 9.074 min
Delta R.T.: 0.000 min
Response: 50893408
Conc: 15.38 ng/ml

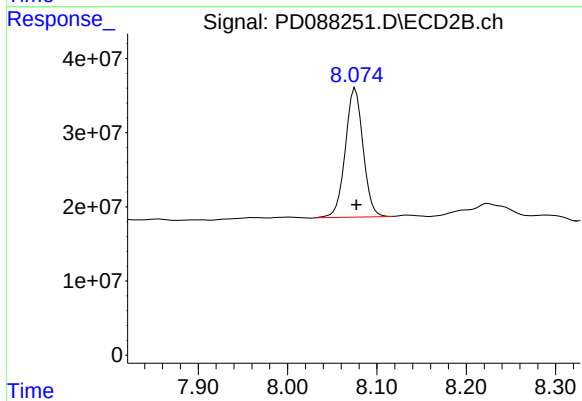

#28 Decachlorobiphenyl

R.T.: 8.076 min
Delta R.T.: -0.001 min
Response: 239859071
Conc: 12.98 ng/ml