

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042721\
 Data File : PD062481.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2021 12:13
 Operator : AR\AJ
 Sample : PB135914BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 12:54:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.489	3.981	15306068	209.5E6	18.792	19.893
28)	SA Decachlor...	8.261	9.043	23628565	188.2E6	19.479	22.185
Target Compounds							
3)	MA gamma-BHC...	0.000	4.652	0	1745707	N.D.	0.111 #
8)	B Heptachlo...	0.000	5.862	0	10508367	N.D.	0.765 #
9)	A Endosulfan I	0.000	6.195f	0	2039858	N.D.	0.156 #
15)	B Endosulfa...	0.000	6.906	0	11214963	N.D.	0.975 #
17)	MA 4,4'-DDT	0.000	7.108	0	1827117	N.D.	0.183 #
19)	B Endosulfa...	0.000	7.238	0	743793	N.D.	0.069 #
21)	B Endrin ke...	0.000	7.734f	0	2326539	N.D.	0.232 #
27)	Chlordane-5	0.000	6.963	0	252832	N.D.	0.615 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042721\
Data File : PD062481.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2021 12:13
Operator : AR\AJ
Sample : PB135914BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 12:54:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

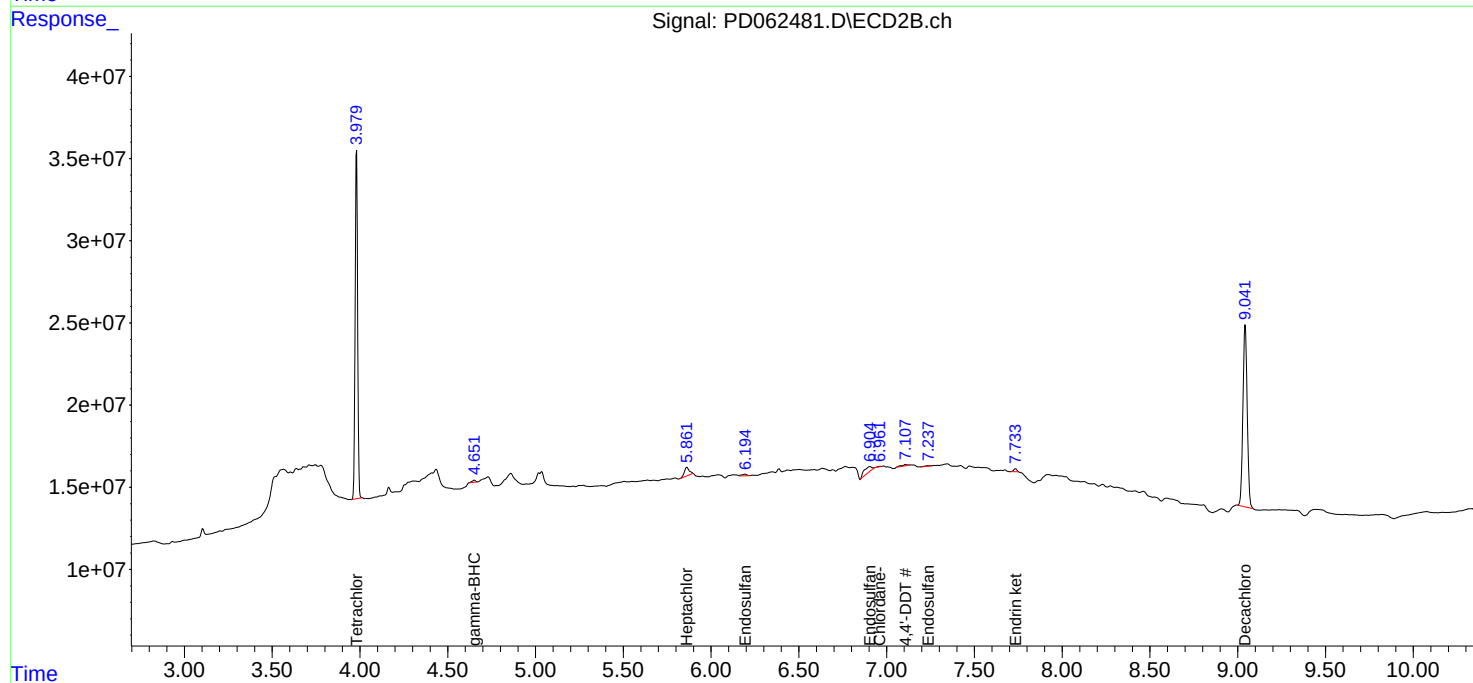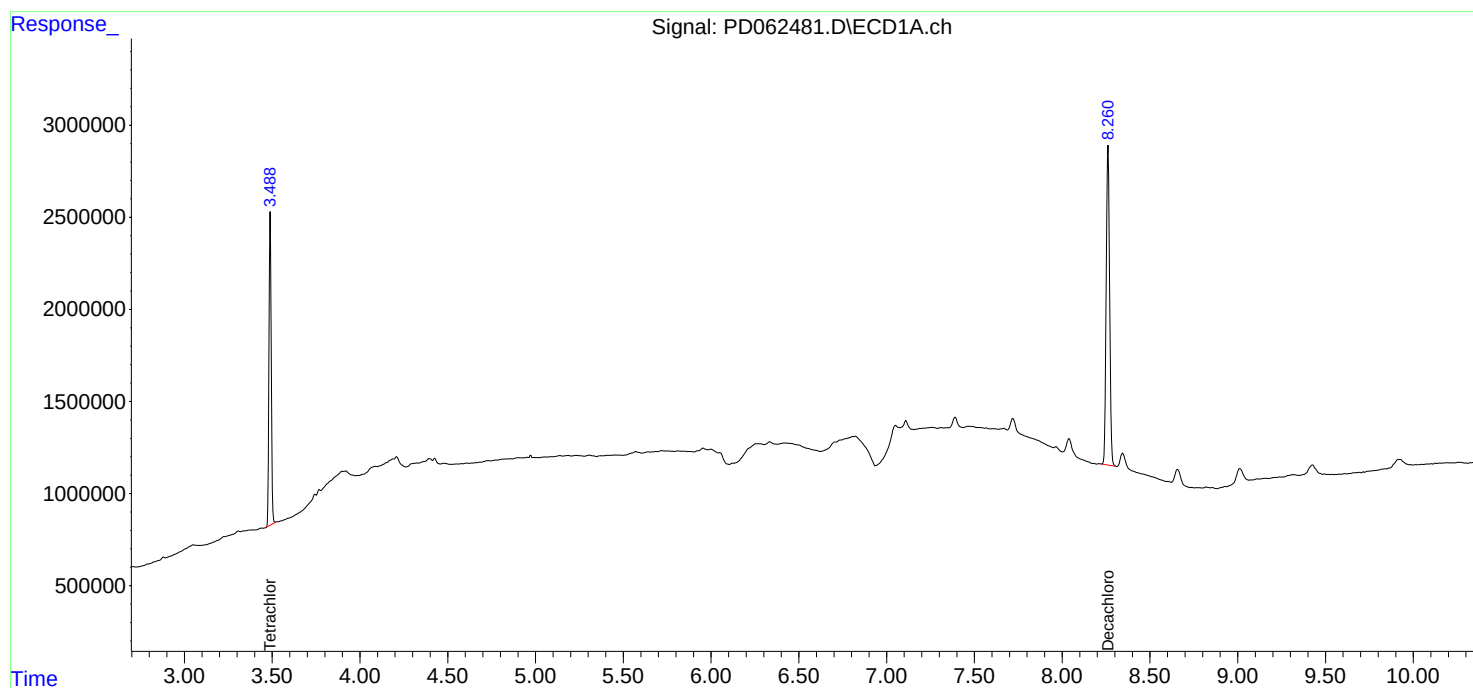


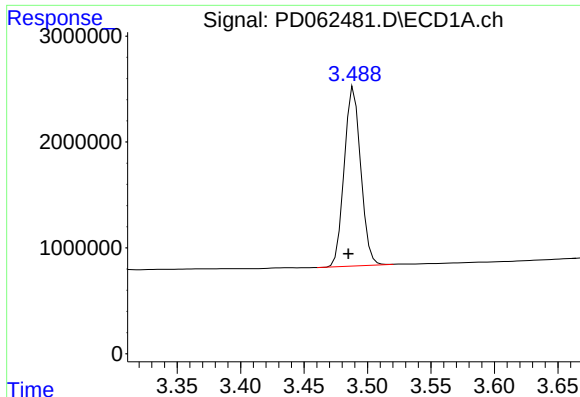

#1 Tetrachloro-m-xylene


R.T.: 3.489 min
Delta R.T.: 0.004 min
Response: 15306068
Conc: 18.79 ng/ml

Instrument :
ECD_D
ClientSampleId :

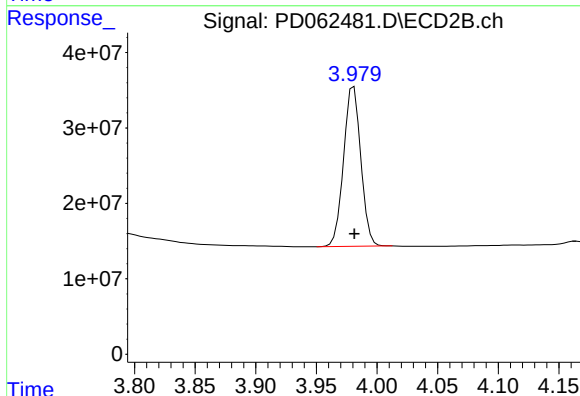


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 209498297
Conc: 19.89 ng/ml

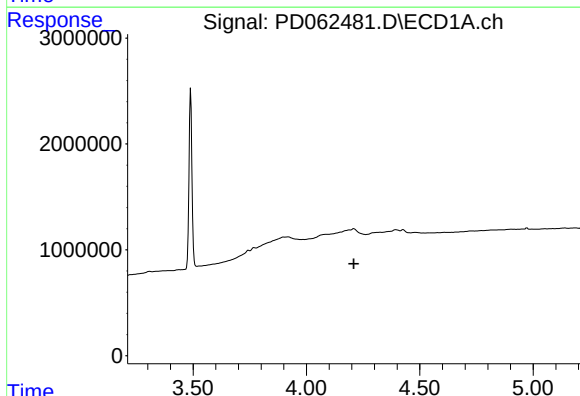


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.209 min
Response: 0
Conc: N.D.

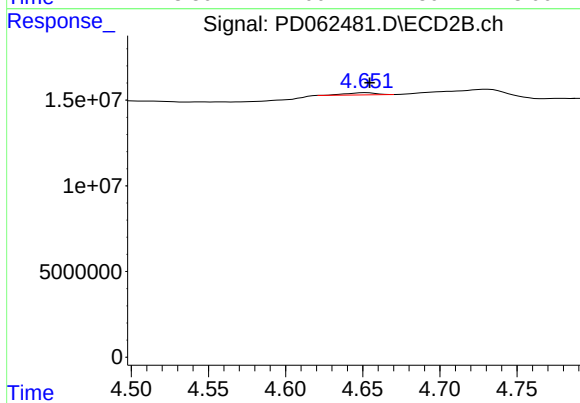

#3 gamma-BHC (Lindane)


R.T.: 4.652 min
Delta R.T.: -0.002 min
Response: 1745707
Conc: 0.11 ng/ml

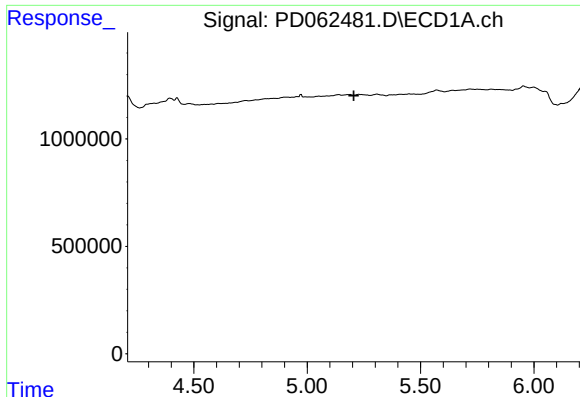

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.206 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

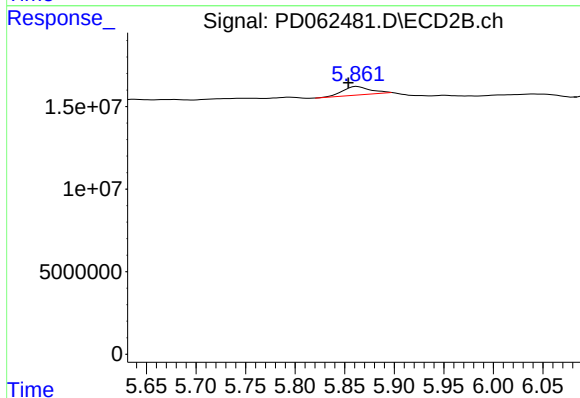


#8 Heptachlor epoxide

R.T.: 5.862 min
Delta R.T.: 0.009 min
Response: 10508367
Conc: 0.76 ng/ml

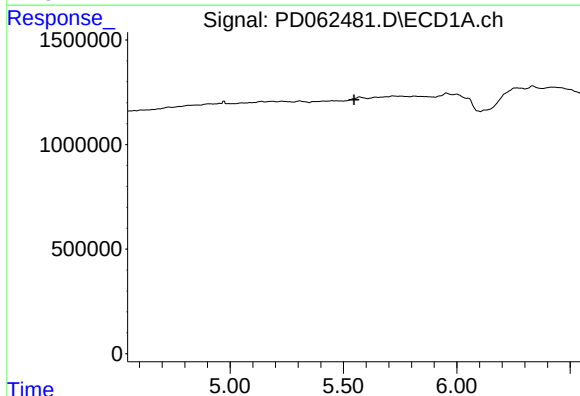


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.547 min
Response: 0
Conc: N.D.

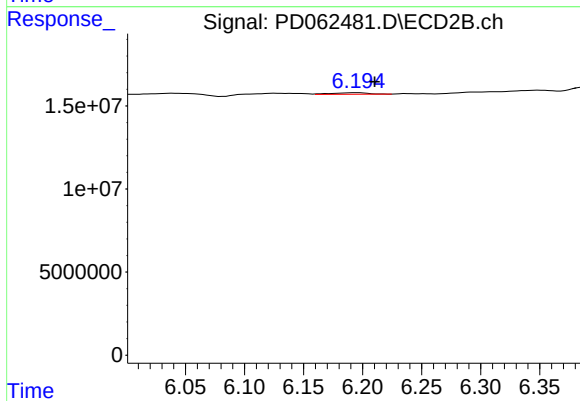

#9 Endosulfan I


R.T.: 6.195 min
Delta R.T.: -0.015 min
Response: 2039858
Conc: 0.16 ng/ml

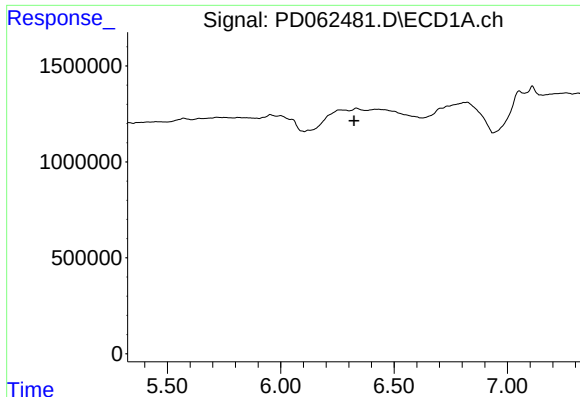

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.323 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

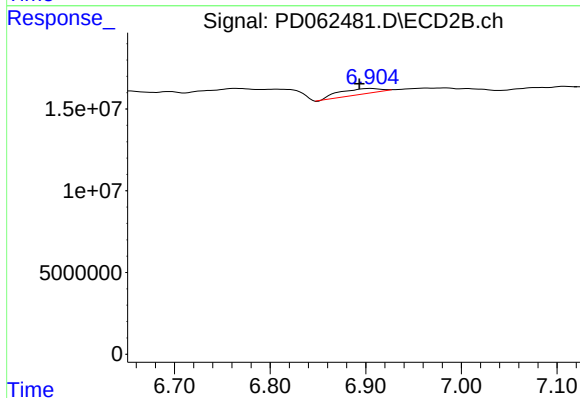


#15 Endosulfan II

R.T.: 6.906 min
Delta R.T.: 0.012 min
Response: 11214963
Conc: 0.97 ng/ml

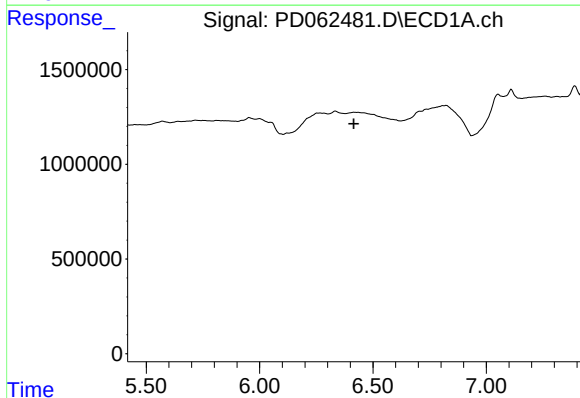


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.415 min
Response: 0
Conc: N.D.

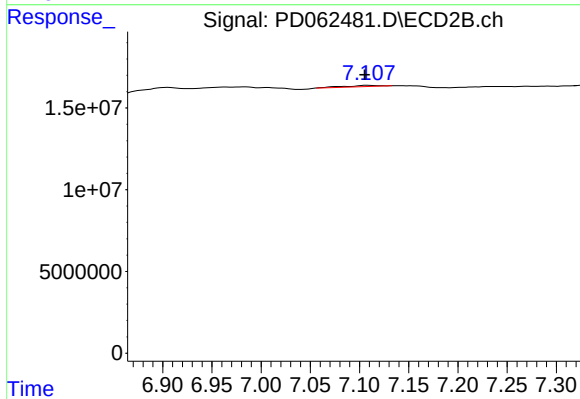

#17 4,4'-DDT


R.T.: 7.108 min
Delta R.T.: 0.003 min
Response: 1827117
Conc: 0.18 ng/ml

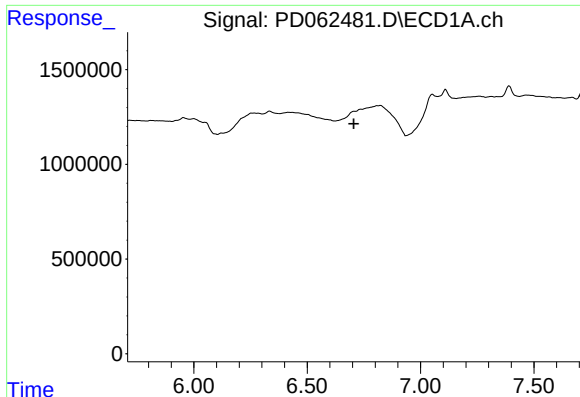

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 6.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

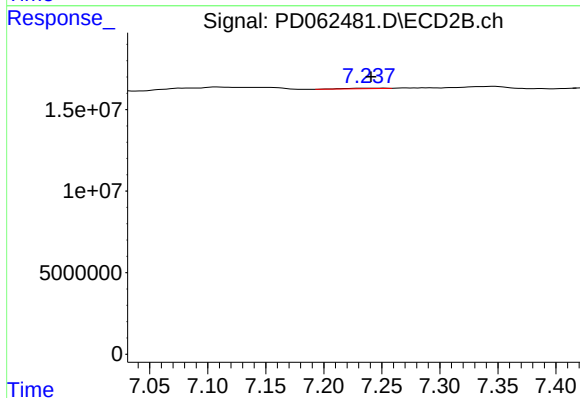


#19 Endosulfan Sulfate

R.T.: 7.238 min
Delta R.T.: -0.003 min
Response: 743793
Conc: 0.07 ng/ml

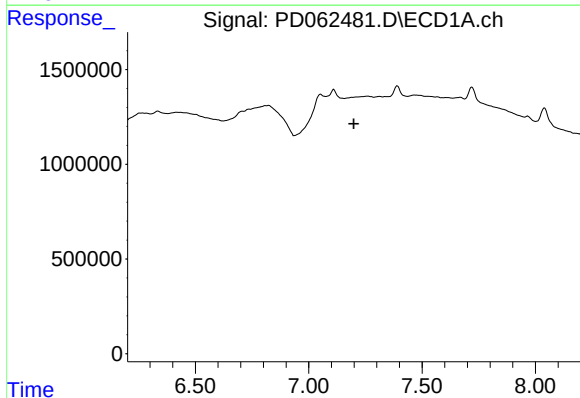


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

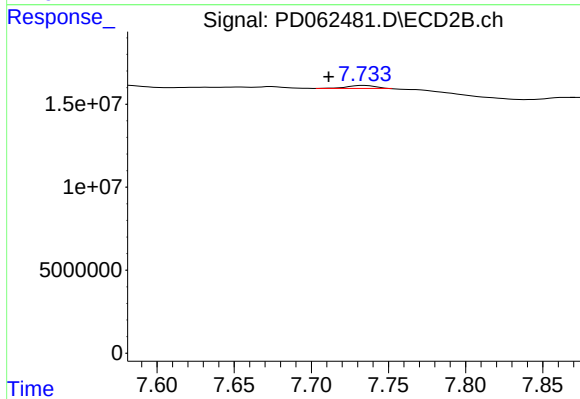

#21 Endrin ketone


R.T.: 7.734 min
Delta R.T.: 0.023 min
Response: 2326539
Conc: 0.23 ng/ml

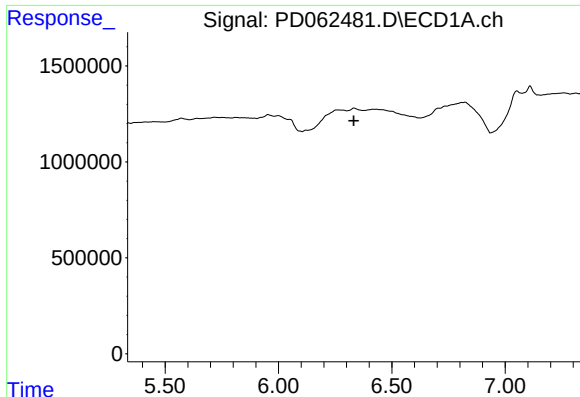

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.333 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

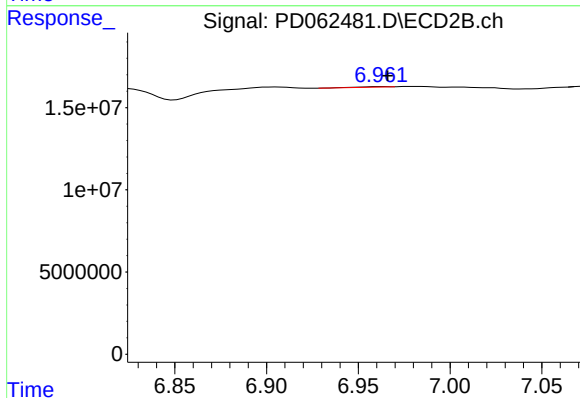


#27 Chlordane-5

R.T.: 6.963 min
Delta R.T.: -0.003 min
Response: 252832
Conc: 0.61 ng/ml

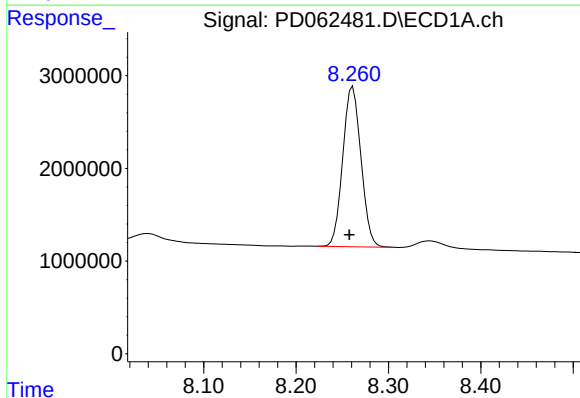

#28 Decachlorobiphenyl

R.T.: 8.261 min
Delta R.T.: 0.004 min
Response: 23628565
Conc: 19.48 ng/ml

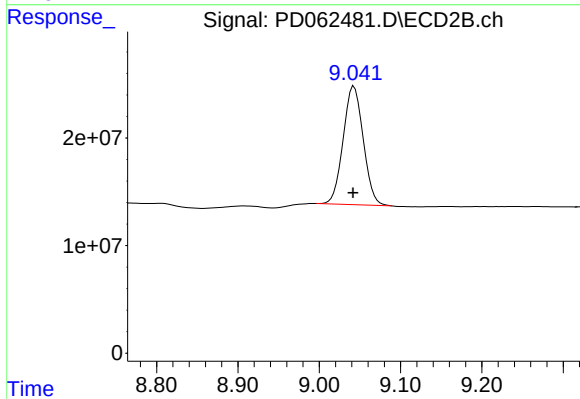

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.000 min
Response: 188235443
Conc: 22.18 ng/ml