

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042721\
 Data File : PD062478.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2021 11:25
 Operator : AR\AJ
 Sample : M2106-03RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 SB-22-14.5-15.0RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 12:53:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.484	3.980	11087147	152.2E6	13.612	14.455
28)	SA Decachlor...	8.256	9.040	35726378	290.8E6	29.452	34.270
Target Compounds							
12)	B 4,4'-DDE	5.654	6.316	2981510	41632240	2.456	2.949



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042721\
Data File : PD062478.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2021 11:25
Operator : AR\AJ
Sample : M2106-03RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
SB-22-14.5-15.0RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 12:53:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

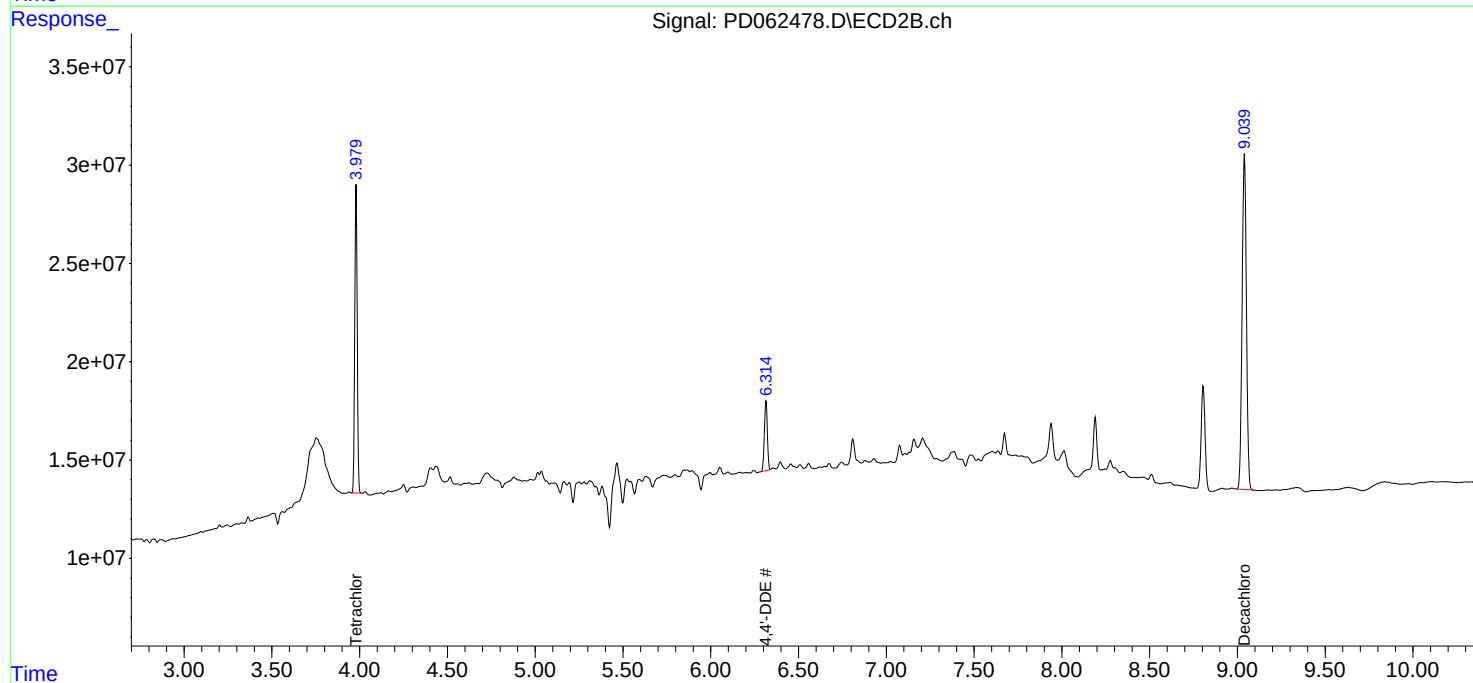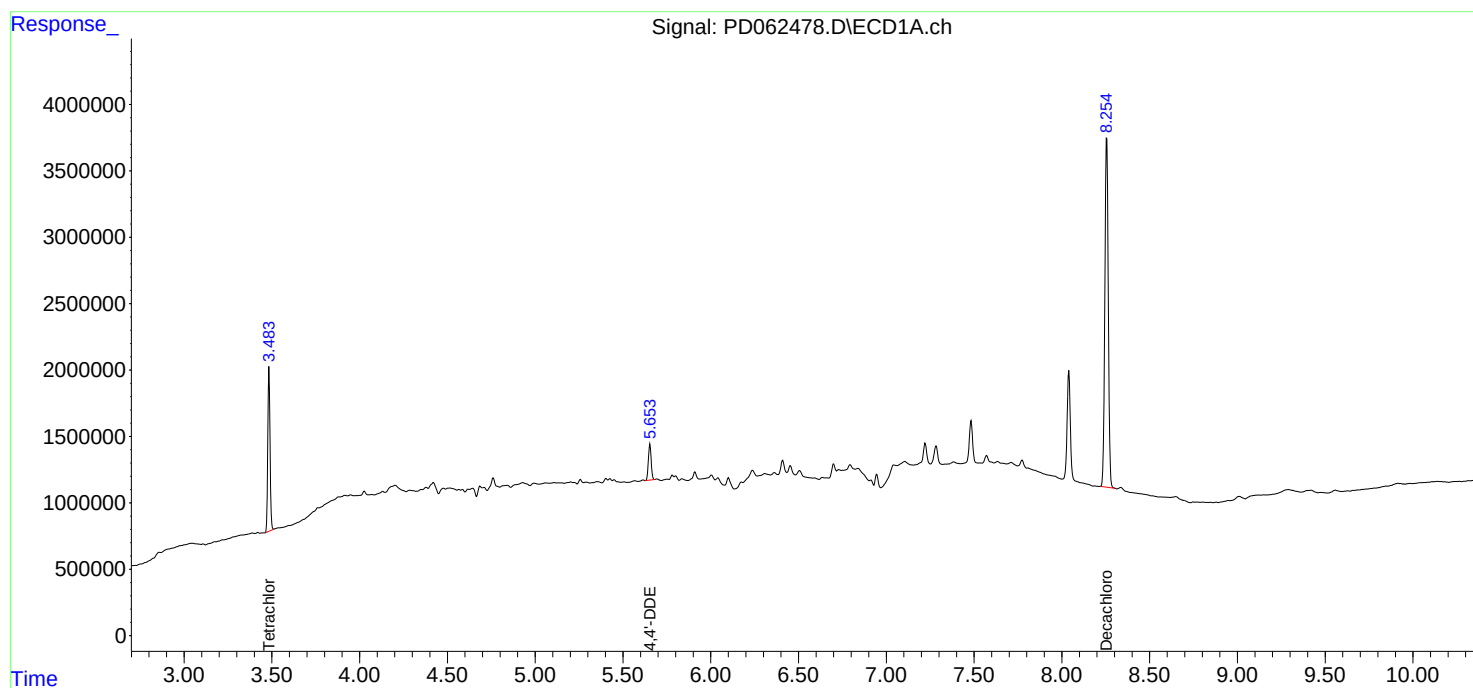


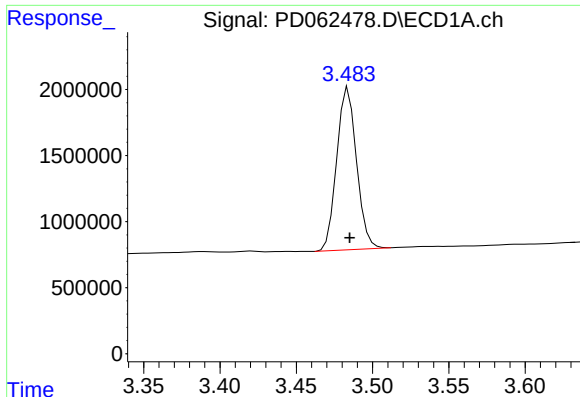

#1 Tetrachloro-m-xylene


R.T.: 3.484 min
Delta R.T.: 0.000 min
Response: 11087147
Conc: 13.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-22-14.5-15.0RE

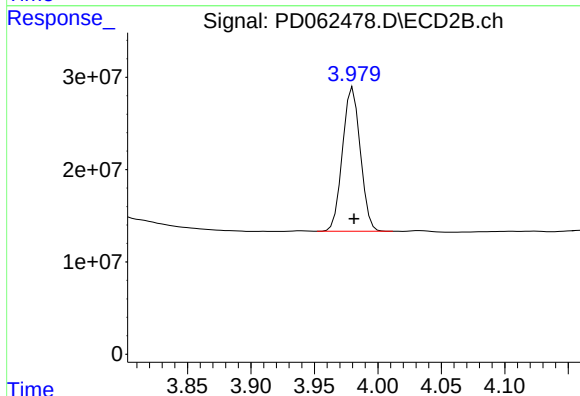


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: 0.000 min
Response: 152232173
Conc: 14.46 ng/ml

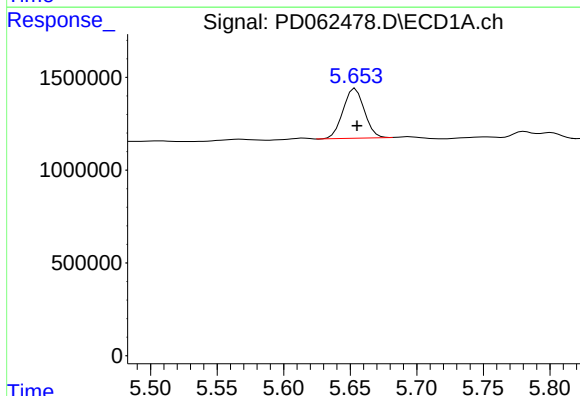


#12 4,4'-DDE

R.T.: 5.654 min
Delta R.T.: -0.001 min
Response: 2981510
Conc: 2.46 ng/ml

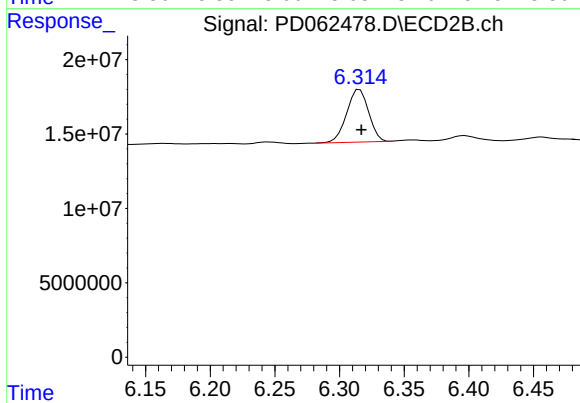

#12 4,4'-DDE


R.T.: 6.316 min
Delta R.T.: -0.001 min
Response: 41632240
Conc: 2.95 ng/ml

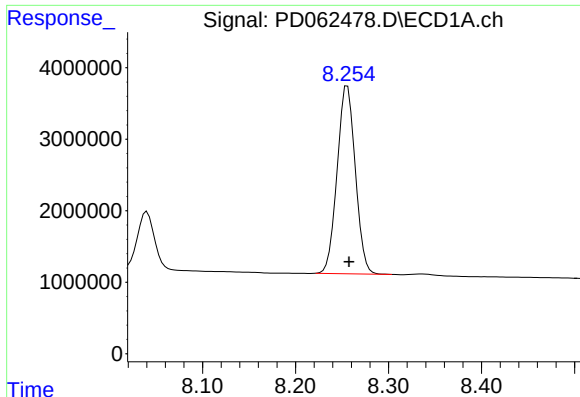

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.002 min
Response: 35726378
Conc: 29.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
SB-22-14.5-15.0RE

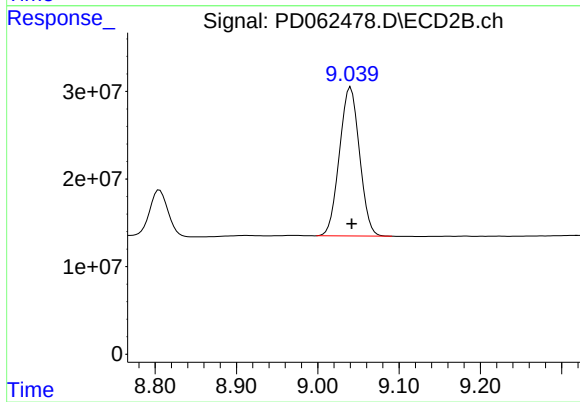

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: -0.001 min
Response: 290781889
Conc: 34.27 ng/ml