

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042721\
 Data File : PD062483.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2021 12:41
 Operator : AR\AJ
 Sample : M2169-06DL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 CF-6DL

Manual Integrations
 APPROVED

Ankita
 4/28/2021 10:35:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 12:54:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 23:19:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.484	3.981	3486287	46693814	4.280	4.434
28) SA Decachlor...	8.256	9.040	5732524	43377504	4.726	5.112
Target Compounds						
12) B 4,4'-DDE	5.654	6.316	72254487	823.2E6	59.523	58.303
13) MA Dieldrin	5.788	6.466	983297	11964219	0.771m	0.851
16) A 4,4'-DDD	6.172	6.806	2479358	36202695	2.477	3.249 #
17) MA 4,4'-DDT	6.414	7.104	85743492	900.8E6	83.965	90.330

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042721\
Data File : PD062483.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2021 12:41
Operator : AR\AJ
Sample : M2169-06DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
CF-6DL


Manual Integrations
APPROVED

Ankita
4/28/2021 10:35:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 12:54:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD042321.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 23:19:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

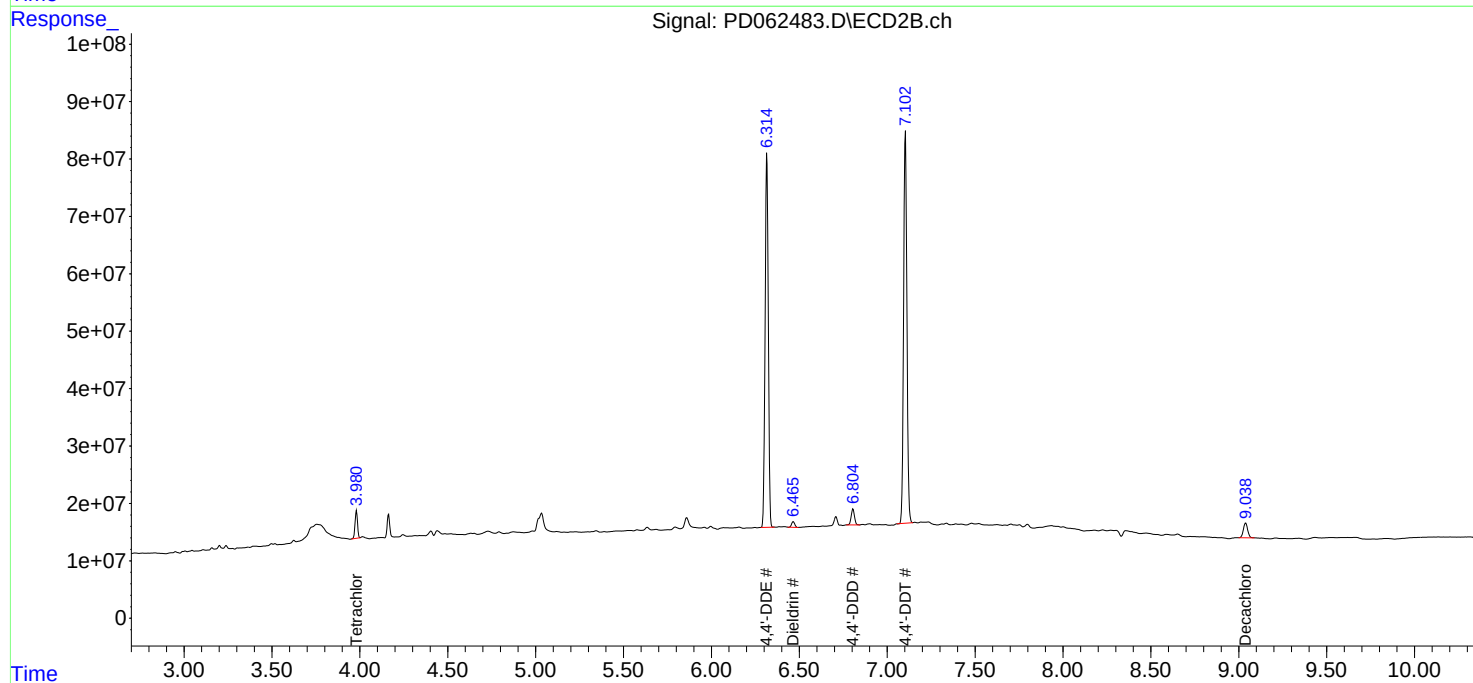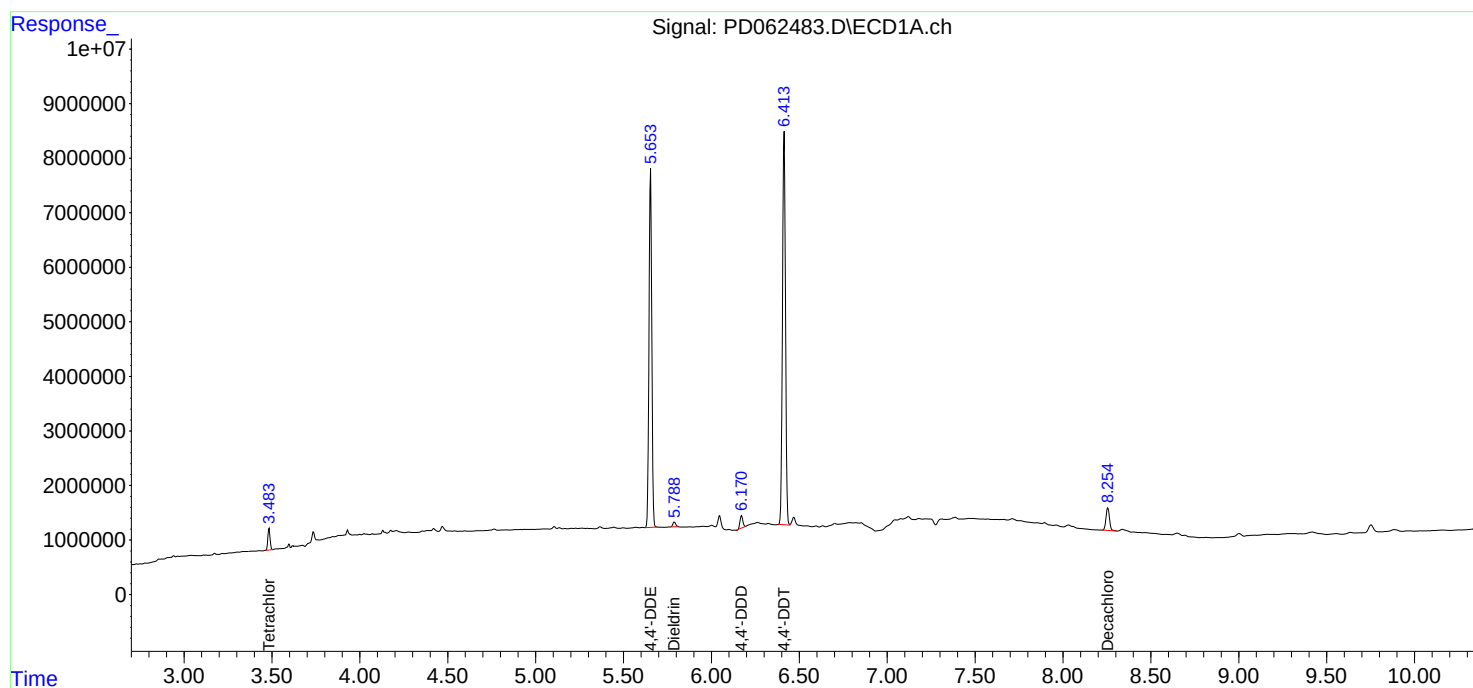

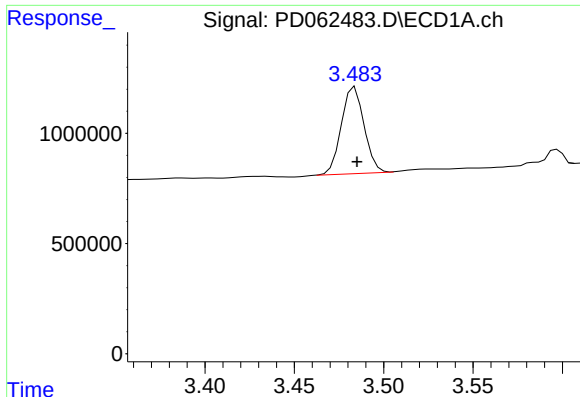


#1 Tetrachloro-m-xylene

R.T.: 3.484 min
Delta R.T.: -0.001 min
Response: 3486287
Conc: 4.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
CF-6DL


Manual Integrations
APPROVED

Ankita
4/28/2021 10:35:48 AM

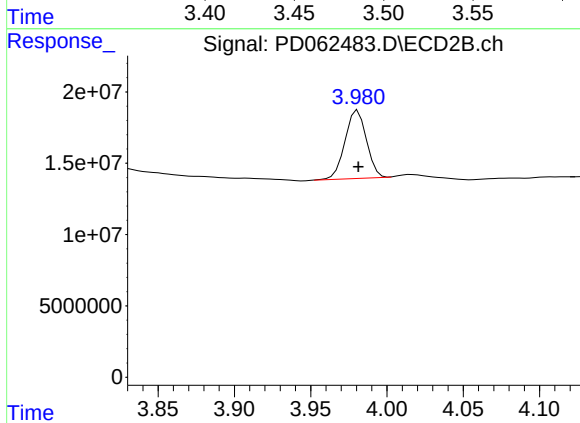


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 46693814
Conc: 4.43 ng/ml

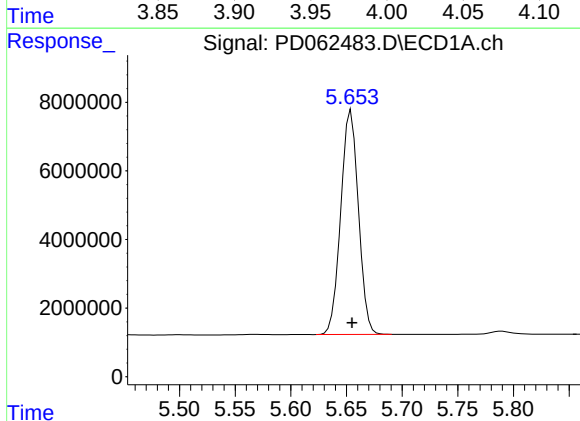


#12 4,4'-DDE

R.T.: 5.654 min
Delta R.T.: 0.000 min
Response: 72254487
Conc: 59.52 ng/ml

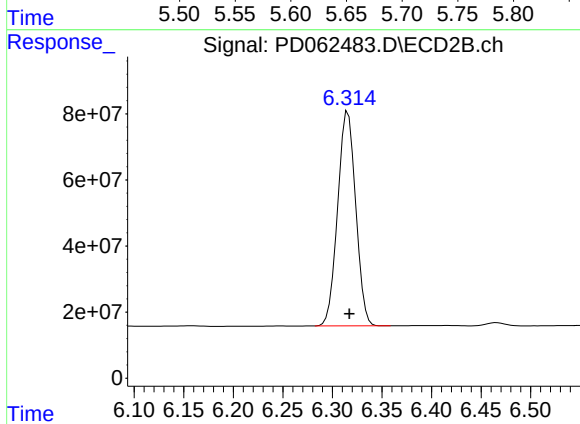

#12 4,4'-DDE

R.T.: 6.316 min
Delta R.T.: -0.001 min
Response: 823223355
Conc: 58.30 ng/ml

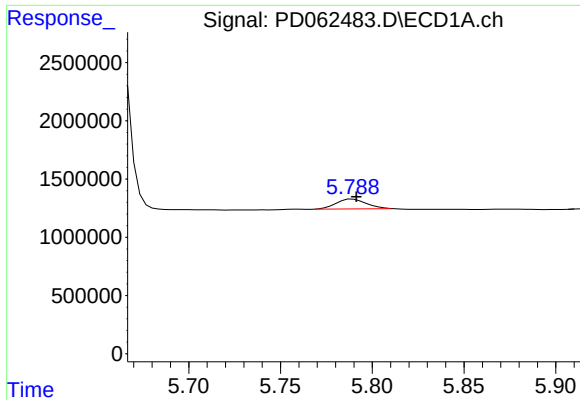


#13 Dieldrin

R.T.: 5.788 min
Delta R.T.: -0.003 min
Response: 983297
Conc: 0.77 ng/ml m

Instrument :
ECD_D
ClientSampleId :
CF-6DL


Manual Integrations
APPROVED

Ankita
4/28/2021 10:35:48 AM

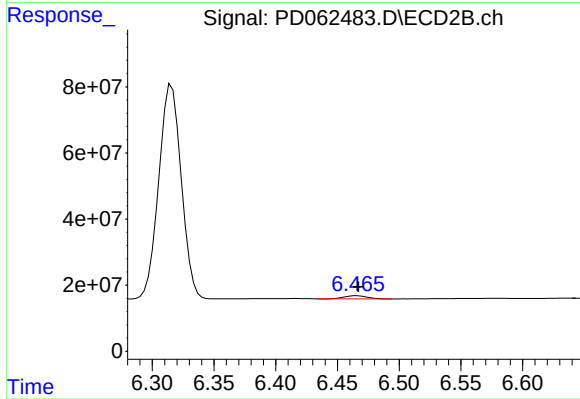


#13 Dieldrin

R.T.: 6.466 min
Delta R.T.: 0.000 min
Response: 11964219
Conc: 0.85 ng/ml

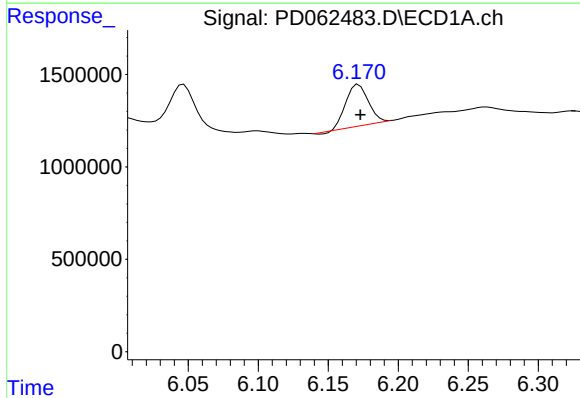


#16 4,4'-DDD

R.T.: 6.172 min
Delta R.T.: -0.001 min
Response: 2479358
Conc: 2.48 ng/ml

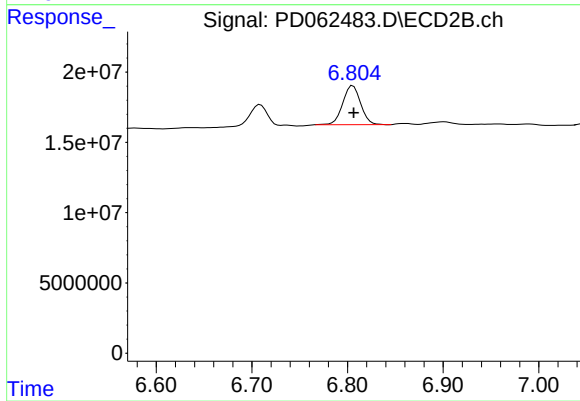

#16 4,4'-DDD

R.T.: 6.806 min
Delta R.T.: 0.000 min
Response: 36202695
Conc: 3.25 ng/ml

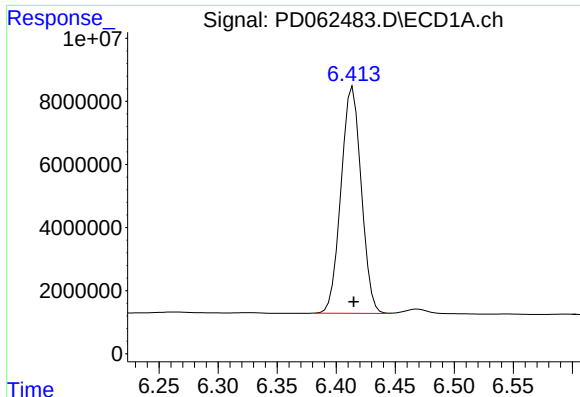


#17 4,4'-DDT

R.T.: 6.414 min
Delta R.T.: 0.000 min
Response: 85743492
Conc: 83.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
CF-6DL


Manual Integrations
APPROVED

Ankita
4/28/2021 10:35:48 AM

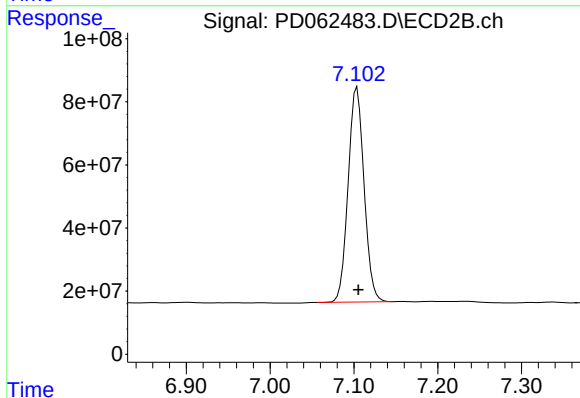


#17 4,4'-DDT

R.T.: 7.104 min
Delta R.T.: -0.002 min
Response: 900790048
Conc: 90.33 ng/ml

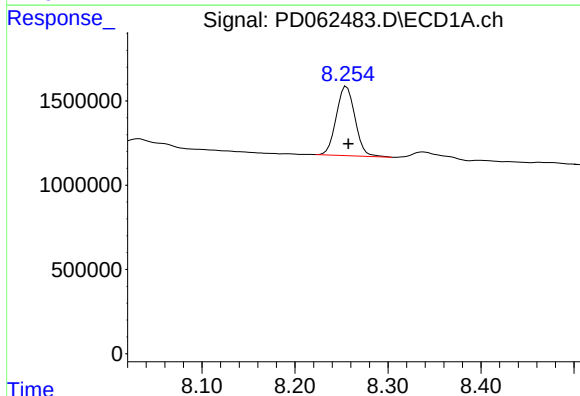

#28 Decachlorobiphenyl

R.T.: 8.256 min
Delta R.T.: -0.002 min
Response: 5732524
Conc: 4.73 ng/ml

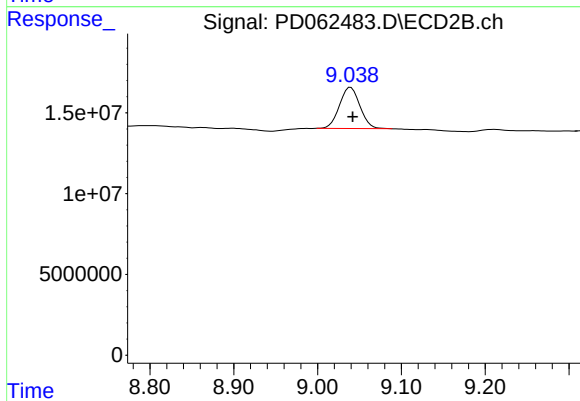

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: -0.002 min
Response: 43377504
Conc: 5.11 ng/ml