

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042722\
 Data File : PD069263.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2022 12:40
 Operator : AR\AJ
 Sample : PB144345BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS345

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/28/2022
 Supervised By : mohammad ahmed 04/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 21:33:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.450	4.172	21963011	204.7E6	17.335	16.961
27)	SA Decachlor...	8.207	9.370	47761168	241.1E6	35.916	34.279
Target Compounds							
2)	A alpha-BHC	3.889	4.568	7195755	71930125	4.026	4.375
3)	MA gamma-BHC...	4.173	4.859	8160453	73190094	4.512	4.698
4)	MA Heptachlor	4.471	5.386	7815817	75166695	4.603	4.965
5)	MB Aldrin	4.718	5.699	8128942	72401285	5.103	5.072
6)	B beta-BHC	4.424	5.023	3759662	33756340	4.854	5.032
7)	B delta-BHC	4.626	5.248	6119749	55057905	3.834m	4.690
8)	B Heptachlo...	5.161	6.088	7420704	80713844	5.041m	7.245 #
9)	A Endosulfan I	5.501	6.451	7520530	60670666	5.154	5.108
10)	B trans-Chl...	5.389	6.325	7875469	64320146	5.253	5.070
11)	B cis-Chlor...	5.447	6.399	7944863	64627995	5.323	5.189
12)	B 4,4'-DDE	5.613	6.550	14574672	115.4E6	10.866	10.605
13)	MA Dieldrin	5.745	6.710	15300780	120.2E6	9.831	9.966
14)	MA Endrin	6.003	6.929	13584487	89755208	9.709	9.229
15)	B Endosulfa...	6.277	7.135	12993672	99210379	10.083	10.351
16)	A 4,4'-DDD	6.130	7.041	11627231	92947818	9.537	9.926
17)	MA 4,4'-DDT	6.371	7.344	10813709	86484119	8.815	9.607
18)	B Endrin al...	6.446	7.259	11812687	85499534	11.900	11.967
19)	B Endosulfa...	6.659	7.484	12414367	84891442	9.908	9.675
20)	A Methoxychlor	6.921	7.797	33898787	204.9E6	49.950	49.711
21)	B Endrin ke...	7.151	7.959	17019906	99904703	11.781m	10.821

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042722\
Data File : PD069263.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2022 12:40
Operator : AR\AJ
Sample : PB144345BS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 21:33:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

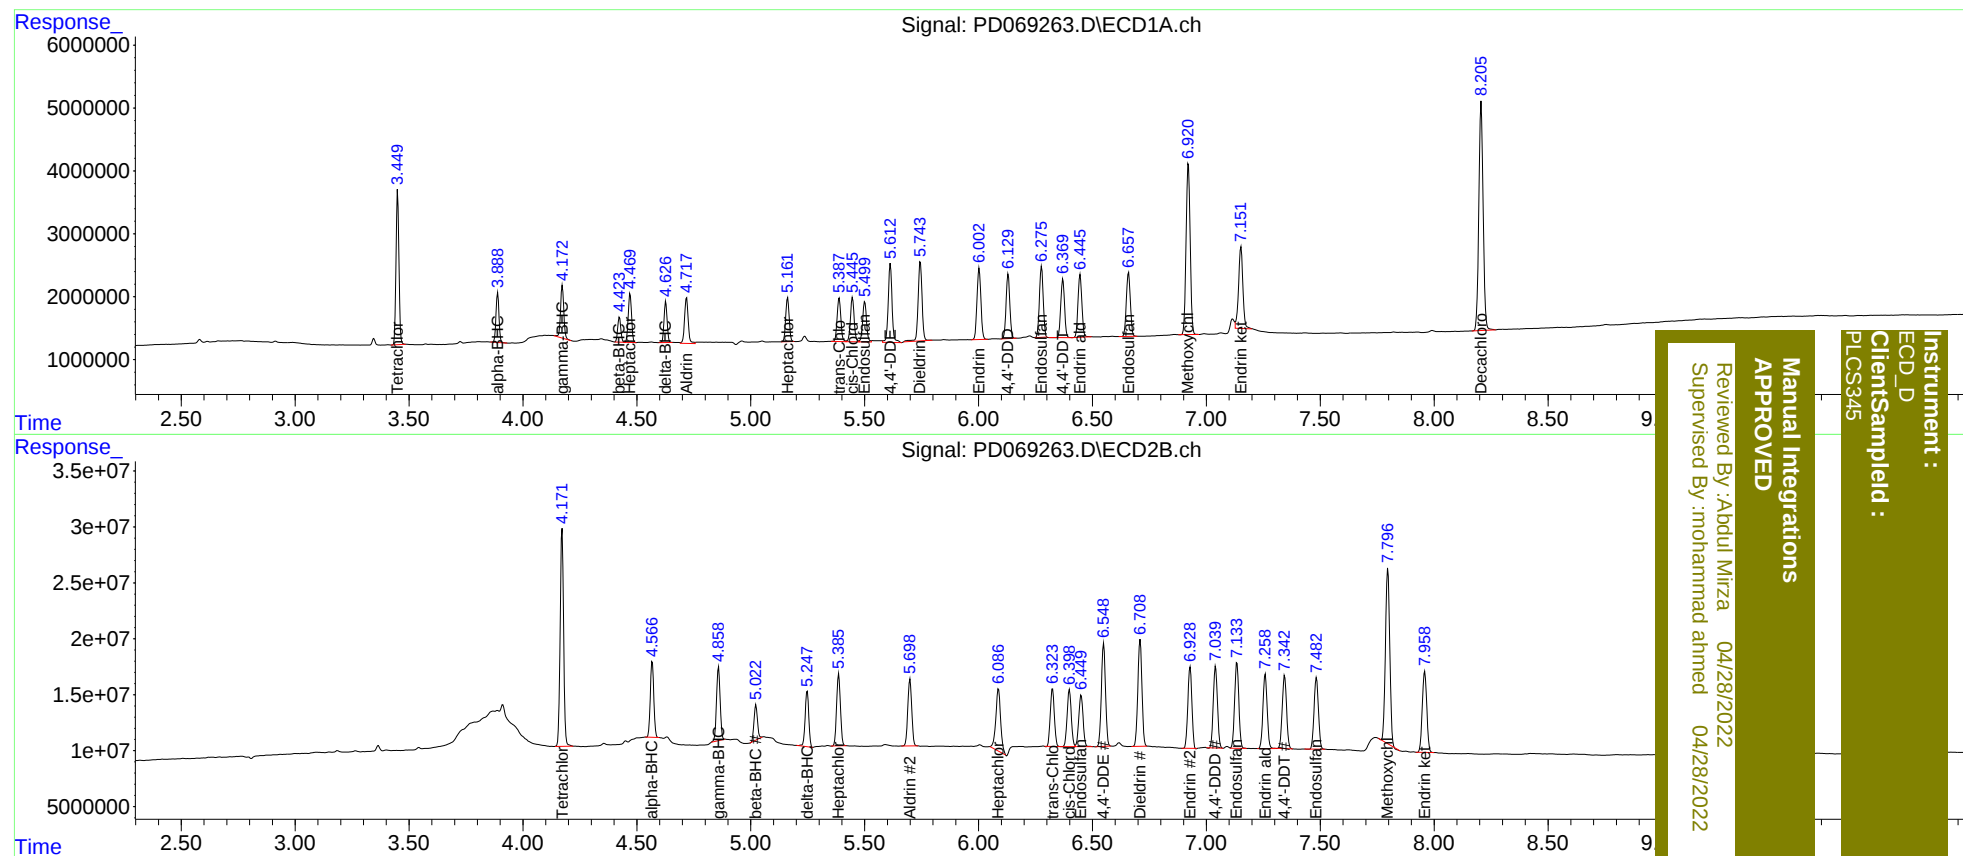

Instrument :
ECD_D
ClientSampled :
PLCS345

Manual Integrations
APPROVED

Reviewed By: Abdul Miza 04/28/2022
Supervised By: mohammad ahmed 04/28/2022