

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042722\
 Data File : PD069266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2022 13:35
 Operator : AR\AJ
 Sample : N2470-03MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFFG0MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/28/2022
 Supervised By : mohammad ahmed 04/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 21:34:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.449	4.170	15626343	164.8E6	12.334	13.657
27)	SA Decachlor...	8.205	9.365	23703198	119.2E6	17.825	16.957m
Target Compounds							
2)	A alpha-BHC	3.889	4.566	97223138	734.4E6	54.391	44.674m
3)	MA gamma-BHC...	4.173	4.858	103.0E6	727.1E6	56.943	46.670
4)	MA Heptachlor	4.470	5.386	92418574	671.9E6	54.433	44.380
5)	MB Aldrin	4.718	5.699	94249268	647.4E6	59.165	45.350
6)	B beta-BHC	4.423	5.021	41433190	169.2E6	53.492	25.222 #
7)	B delta-BHC	4.627	5.247	45347415	256.6E6	28.409	21.862m
8)	B Heptachlo...	5.162	6.087	82603691	546.8E6	56.115	49.078
9)	A Endosulfan I	5.501	6.449	63476997	492.9E6	43.499	41.498m
10)	B trans-Chl...	5.388	6.322	113.5E6	665.0E6	75.689	52.412m#
11)	B cis-Chlor...	5.447	6.399	105.1E6	657.3E6	70.434	52.773 #
12)	B 4,4'-DDE	5.613	6.549	166.0E6	960.9E6	123.758	88.327 #
13)	MA Dieldrin	5.745	6.709	195.7E6	1095.3E6	125.756	90.808 #
14)	MA Endrin	6.003	6.929	152.3E6	842.8E6	108.885	86.658
15)	B Endosulfa...	6.276	7.135	141.9E6	928.1E6	110.116	96.840
16)	A 4,4'-DDD	6.130	7.040	122.8E6	867.5E6	100.699	92.638
17)	MA 4,4'-DDT	6.371	7.343	135.1E6	928.9E6	110.154	103.185
18)	B Endrin al...	6.446	7.258	92137356	634.3E6	92.822	88.780
19)	B Endosulfa...	6.658	7.483	122.4E6	680.8E6	97.650	77.586
20)	A Methoxychlor	6.920	7.797	346.7E6	1897.0E6	510.823	460.317
21)	B Endrin ke...	7.150	7.958	145.2E6	802.2E6	100.537	86.887

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042722\
Data File : PD069266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2022 13:35
Operator : AR\AJ
Sample : N2470-03MSD
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 21:34:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

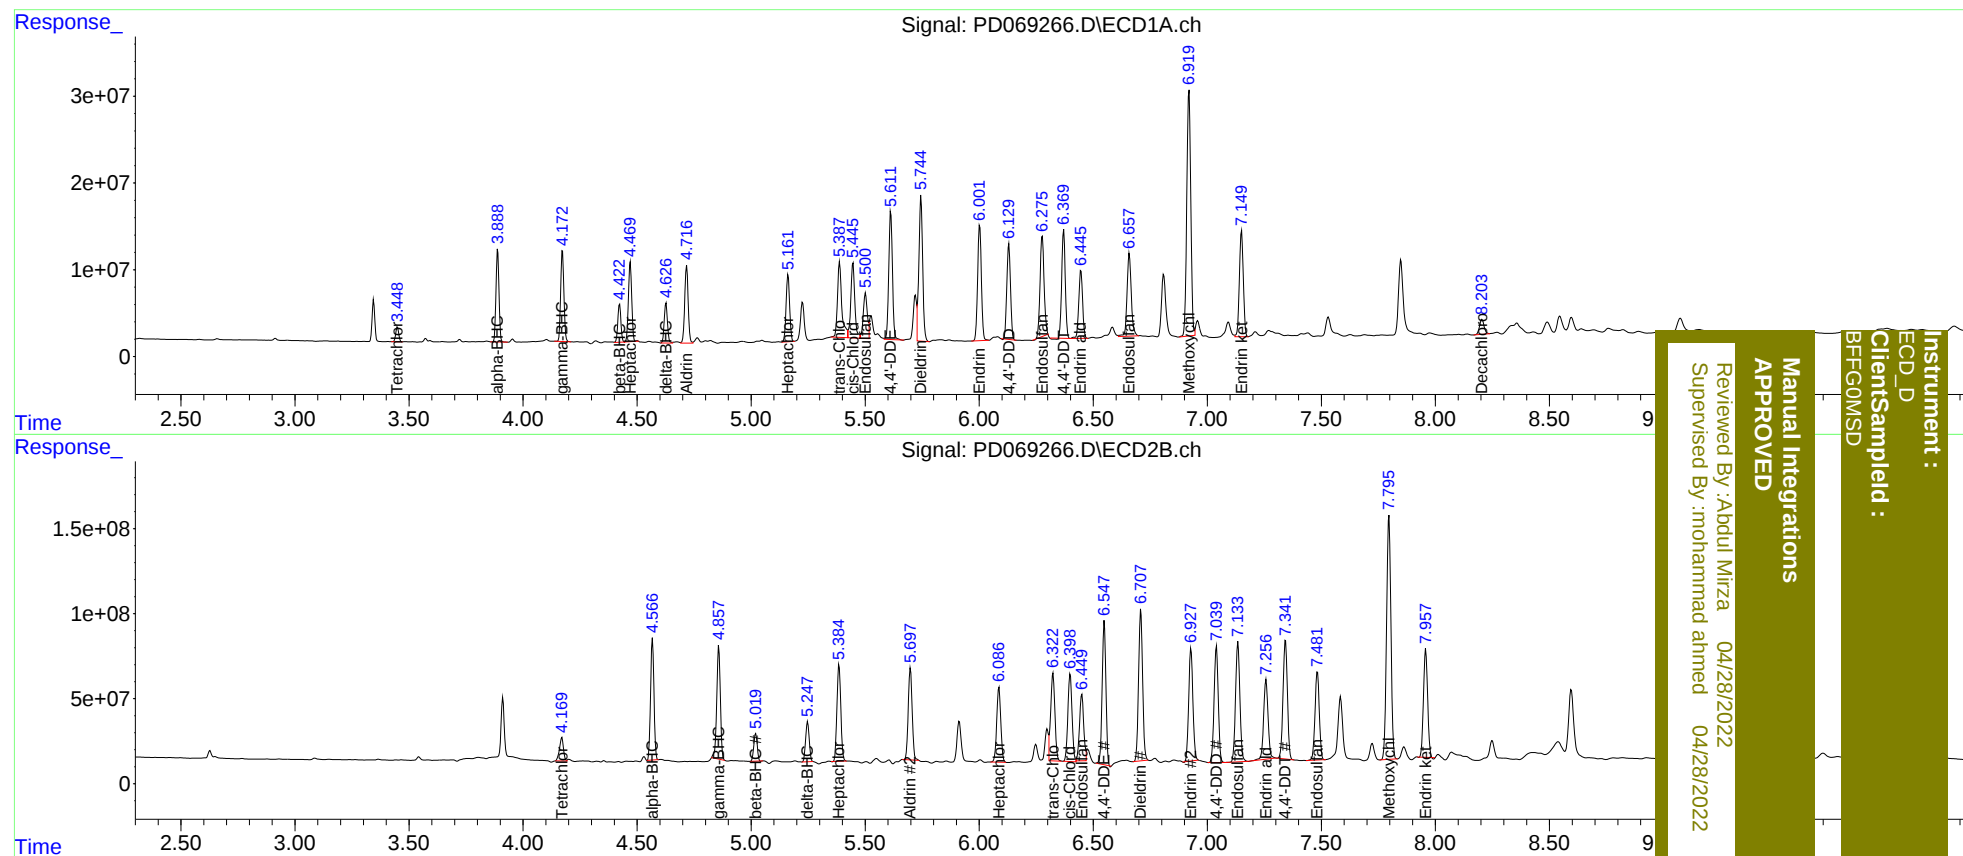

Reviewed By: Abdul Miza 04/28/2022
Supervised By: mohammad ahmed 04/28/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BFG0MSD