

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042722\
 Data File : PD069265.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Apr 2022 13:16
 Operator : AR\AJ
 Sample : N2470-02MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BFFG0MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/28/2022
 Supervised By : mohammad ahmed 04/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 27 21:34:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.170	15975629	169.9E6	12.609	14.078
27)	SA Decachlor...	8.199	9.363	25740386	132.9E6	19.357	18.892m
Target Compounds							
2)	A alpha-BHC	3.883	4.567	99483191	737.2E6	55.656	44.846
3)	MA gamma-BHC...	4.167	4.858	104.5E6	746.0E6	57.785	47.881
4)	MA Heptachlor	4.464	5.385	94980148	693.2E6	55.942	45.789
5)	MB Aldrin	4.711	5.698	95843251	670.1E6	60.166	46.943
6)	B beta-BHC	4.417	5.020	43950293	177.2E6	56.741	26.417 #
7)	B delta-BHC	4.621	5.247	46001817	261.2E6	28.819	22.254
8)	B Heptachlo...	5.156	6.086	84028807	569.1E6	57.083	51.084
9)	A Endosulfan I	5.495	6.448	69281423	536.8E6	47.477	45.196m
10)	B trans-Chl...	5.381	6.321	112.8E6	663.4E6	75.271	52.291m#
11)	B cis-Chlor...	5.440	6.398	108.9E6	687.3E6	72.969	55.181
12)	B 4,4'-DDE	5.606	6.547	173.9E6	989.8E6	129.616	90.983 #
13)	MA Dieldrin	5.738	6.707	199.1E6	1152.3E6	127.920	95.532 #
14)	MA Endrin	5.996	6.928	157.5E6	884.5E6	112.538	90.945
15)	B Endosulfa...	6.270	7.133	159.9E6	971.0E6	124.060	101.317
16)	A 4,4'-DDD	6.123	7.039	128.1E6	902.1E6	105.034	96.333
17)	MA 4,4'-DDT	6.364	7.341	144.5E6	980.1E6	117.787	108.878
18)	B Endrin al...	6.439	7.257	95768821	658.7E6	96.480	92.200
19)	B Endosulfa...	6.652	7.482	130.4E6	717.7E6	104.086	81.795
20)	A Methoxychlor	6.914	7.795	359.4E6	1962.1E6	529.624	476.112
21)	B Endrin ke...	7.145	7.957	150.9E6	859.9E6	104.431	93.144

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD042722\
Data File : PD069265.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Apr 2022 13:16
Operator : AR\AJ
Sample : N2470-02MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 27 21:34:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

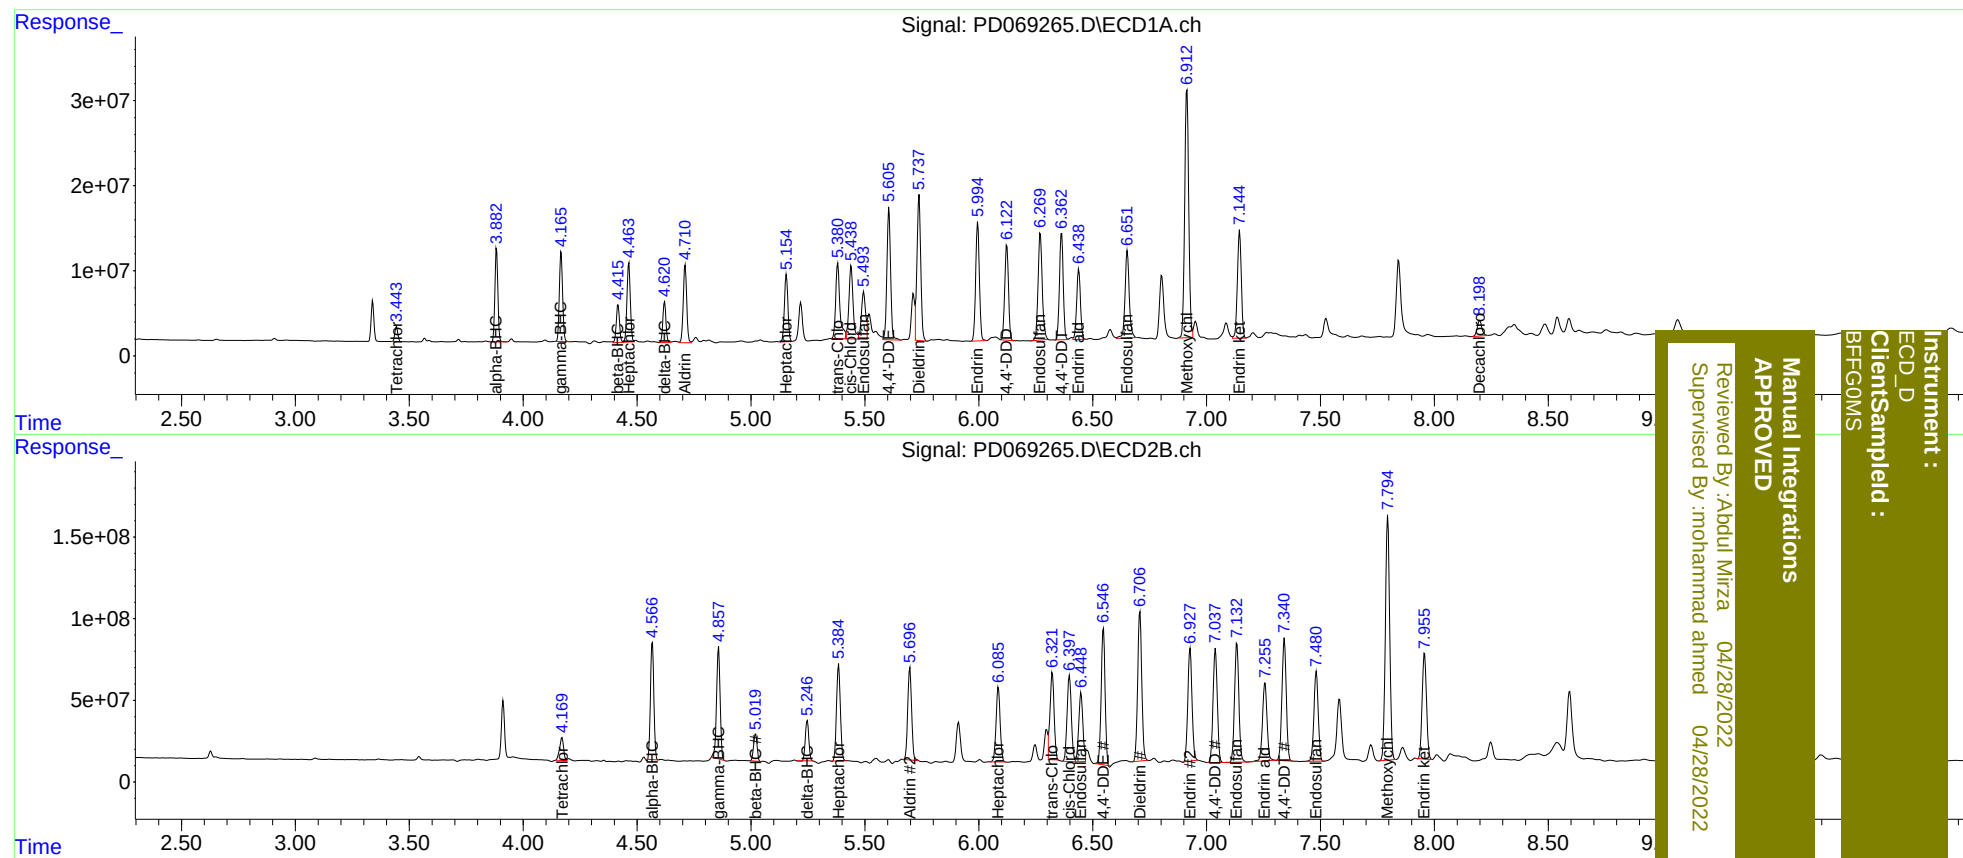

Reviewed By: Abdul Mirza 04/28/2022
Supervised By: mohammad ahmed 04/28/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
BFFGOMS