

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050422\
 Data File : PD069428.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2022 14:50
 Operator : AR\AJ
 Sample : PB144544BS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS544

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/05/2022
 Supervised By :mohammad ahmed 05/05/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 23:19:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.451	4.172	23939438	257.2E6	18.895	21.313
27)	SA Decachlor...	8.207	9.369	44097581	249.6E6	33.161	35.500
Target Compounds							
2)	A alpha-BHC	3.891	4.568	7608166	89992596	4.256	5.474 #
3)	MA gamma-BHC...	4.174	4.859	8040596	86917762	4.445	5.579 #
4)	MA Heptachlor	4.472	5.386	8093900	90372344	4.767	5.970 #
5)	MB Aldrin	4.718	5.699	7982058	83560579	5.011m	5.854
6)	B beta-BHC	4.425	5.023	4055062	48597618	5.235	7.245 #
7)	B delta-BHC	4.627	5.248	6325462	56560636	3.963m	4.818
8)	B Heptachlo...	5.162	6.075	7480313	146.0E6	5.082m	13.106m#
9)	A Endosulfan I	5.501	6.451	6757923	78557119	4.631m	6.614 #
10)	B trans-Chl...	5.388	6.323	8070581	74632412	5.383m	5.883m
11)	B cis-Chlor...	5.447	6.399	7397805	76224081	4.956m	6.120
12)	B 4,4'-DDE	5.613	6.550	13837947	118.0E6	10.317m	10.846
13)	MA Dieldrin	5.745	6.709	14688256	135.6E6	9.437m	11.238
14)	MA Endrin	6.009	6.920	21729207	29093475	15.530	2.992m#
15)	B Endosulfa...	6.278	7.134	12816554	109.9E6	9.946	11.468
16)	A 4,4'-DDD	6.132	7.040	12072706	104.5E6	9.902	11.163
17)	MA 4,4'-DDT	6.372	7.344	9935489	104.7E6	8.099	11.632 #
18)	B Endrin al...	6.448	7.258	11935327	109.6E6	12.024	15.341 #
19)	B Endosulfa...	6.660	7.482	12579522	89005750	10.040	10.144
20)	A Methoxychlor	6.922	7.793	30784759	41299433	45.361	10.022m#
21)	B Endrin ke...	7.150	7.959	32825883	101.2E6	22.722m	10.965 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050422\
Data File : PD069428.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2022 14:50
Operator : AR\AJ
Sample : PB144544BS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 23:19:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

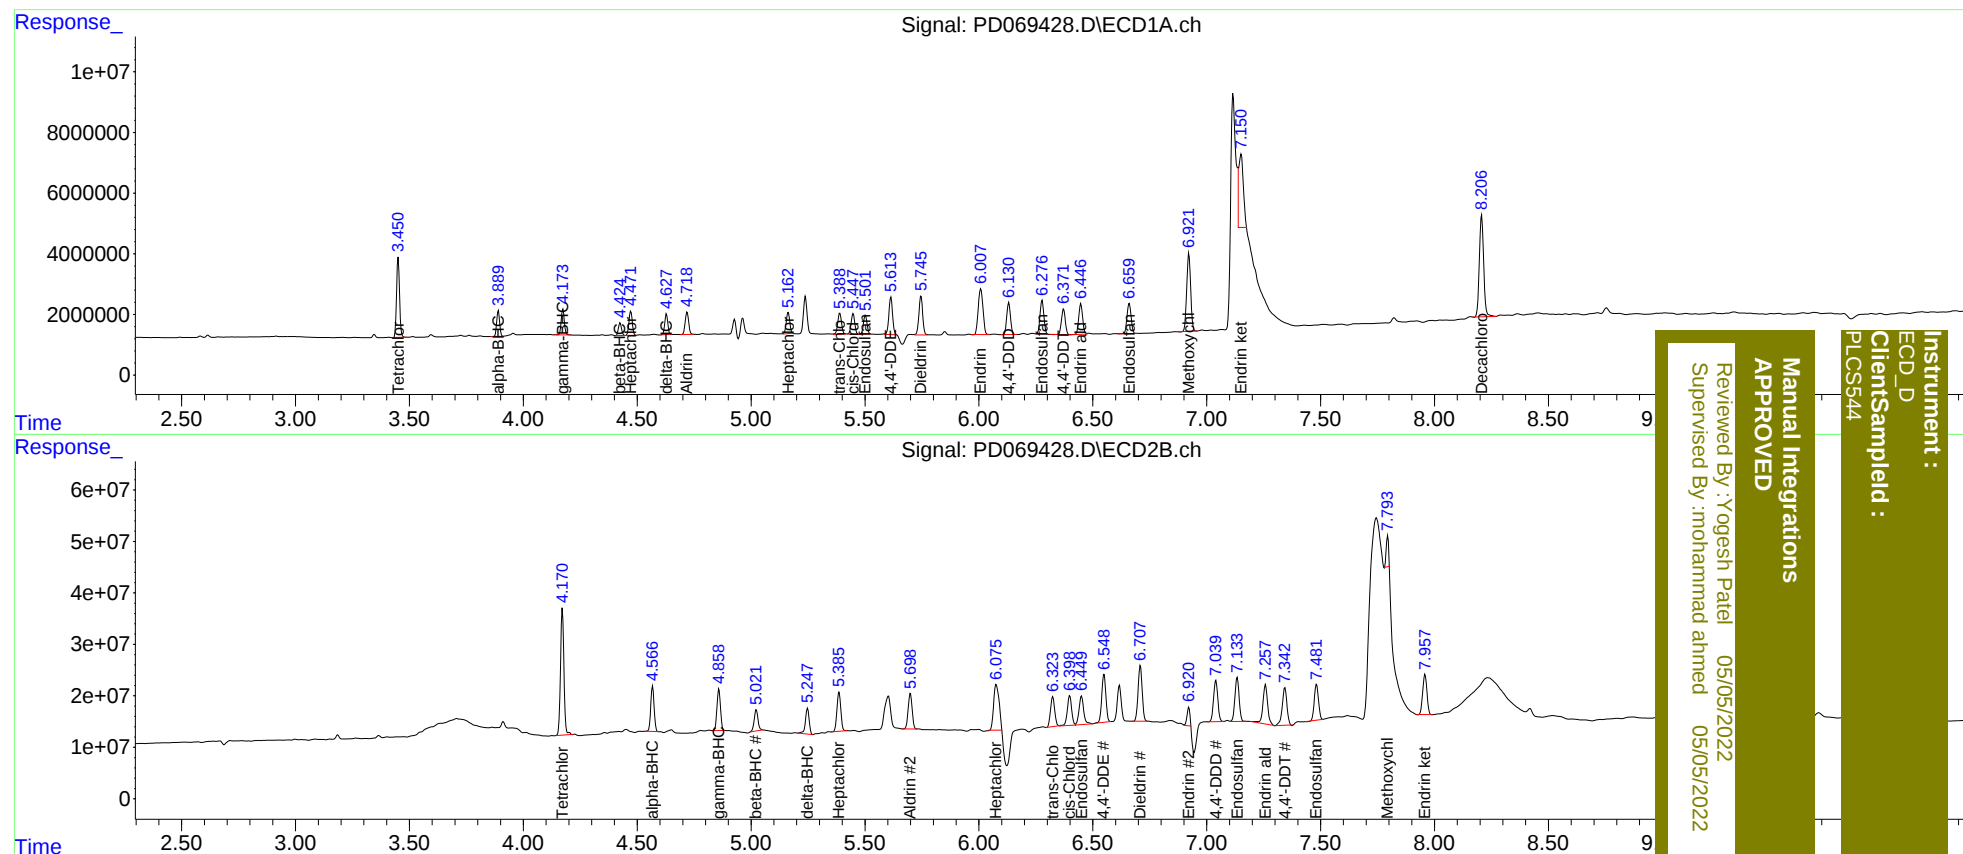

Reviewed By : Yogesh Patel 05/05/2022
Supervised By : mohammad ahmed 05/05/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
PLCS544