

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050422\
 Data File : PD069434.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2022 16:17
 Operator : AR\AJ
 Sample : N2603-24MS
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4A0MS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/05/2022
 Supervised By :mohammad ahmed 05/05/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 23:20:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.171	20275310	224.3E6	16.003	18.587
27)	SA Decachlor...	8.198	9.363	33069502	203.9E6	24.868	29.002m
Target Compounds							
2)	A alpha-BHC	3.883	4.567	88812464	760.4E6	49.686	46.258
3)	MA gamma-BHC...	4.166	4.858	98183119	754.3E6	54.281	48.418
4)	MA Heptachlor	4.463	5.386	87589096	717.2E6	51.589	47.376
5)	MB Aldrin	4.711	5.698	87483010	704.7E6	54.918	49.367
6)	B beta-BHC	4.416	5.021	39964856	149.8E6	51.596	22.325 #
7)	B delta-BHC	4.620	5.248	36562540	211.3E6	22.906	18.000
8)	B Heptachlo...	5.155	6.086	76912049	575.7E6	52.248	51.671
9)	A Endosulfan I	5.494	6.447	50630400	558.8E6	34.696	47.047m#
10)	B trans-Chl...	5.379	6.322	80285502	596.3E6	53.553m	47.000m
11)	B cis-Chlor...	5.439	6.398	78172858	603.6E6	52.372	48.466
12)	B 4,4'-DDE	5.605	6.547	228.4E6	1416.7E6	170.263	130.219
13)	MA Dieldrin	5.737	6.708	175.4E6	1136.9E6	112.722	94.252
14)	MA Endrin	5.995	6.928	144.3E6	837.3E6	103.142	86.092
15)	B Endosulfa...	6.268	7.134	174.7E6	1184.2E6	135.576m	123.556
16)	A 4,4'-DDD	6.122	7.039	117.0E6	934.1E6	95.956	99.750
17)	MA 4,4'-DDT	6.362	7.342	137.7E6	1011.7E6	112.285	112.391
18)	B Endrin al...	6.438	7.257	102.9E6	744.5E6	103.618	104.209
19)	B Endosulfa...	6.651	7.482	107.4E6	725.7E6	85.739	82.702
20)	A Methoxychlor	6.913	7.796	311.9E6	1923.1E6	459.538	466.662
21)	B Endrin ke...	7.144	7.957	137.1E6	887.3E6	94.870	96.109

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050422\
Data File : PD069434.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2022 16:17
Operator : AR\AJ
Sample : N2603-24MS
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 23:20:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

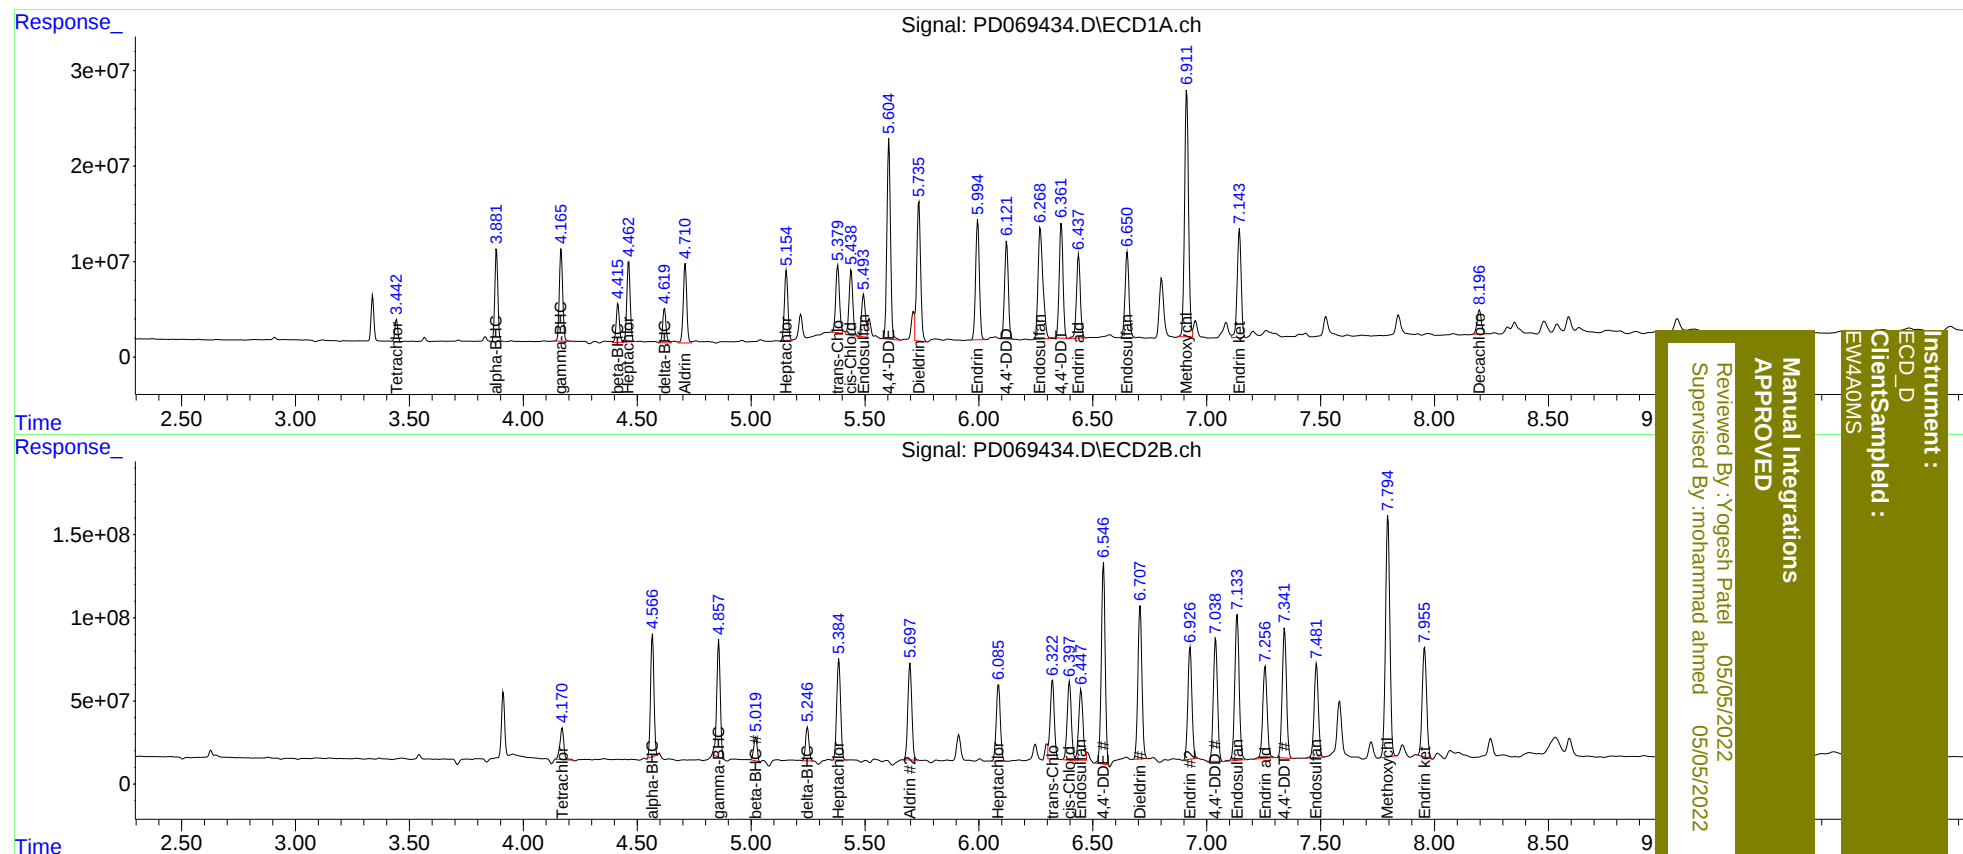

Reviewed By : Yogesh Patel 05/05/2022
Supervised By : mohammad ahmed 05/05/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
EW4AOMS