

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050422\
 Data File : PD069435.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 May 2022 16:31
 Operator : AR\AJ
 Sample : N2603-25MSD
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4A0MSD

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/05/2022
 Supervised By :mohammad ahmed 05/05/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 04 23:21:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 21 02:24:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.444	4.169	20123472	213.6E6	15.883	17.697m
2)	SA Decachlor...	8.197	9.363	32940775	172.2E6	24.771	24.485m
Target Compounds							
2)	A alpha-BHC	3.883	4.566	89239809	762.6E6	49.925	46.390m
3)	MA gamma-BHC...	4.166	4.857	98477402	781.9E6	54.444	50.184m
4)	MA Heptachlor	4.463	5.384	87701145	727.3E6	51.655	48.042m
5)	MB Aldrin	4.710	5.698	87477863	710.2E6	54.914	49.754
6)	B beta-BHC	4.416	5.021	40026589	151.1E6	51.676	22.518 #
7)	B delta-BHC	4.620	5.248	36557389	209.4E6	22.903	17.840
8)	B Heptachlo...	5.154	6.086	76745078	576.5E6	52.135	51.741
9)	A Endosulfan I	5.494	6.447	51650524	551.4E6	35.395	46.422m#
10)	B trans-Chl...	5.379	6.322	80154096	602.5E6	53.465m	47.493m
11)	B cis-Chlor...	5.439	6.398	79652540	610.0E6	53.363	48.981
12)	B 4,4'-DDE	5.605	6.547	228.0E6	1412.6E6	169.973	129.848
13)	MA Dieldrin	5.737	6.707	174.6E6	1140.1E6	112.184	94.518
14)	MA Endrin	5.995	6.927	143.4E6	841.9E6	102.509	86.568
15)	B Endosulfa...	6.269	7.134	162.6E6	1183.8E6	126.183	123.514
16)	A 4,4'-DDD	6.122	7.039	115.5E6	933.9E6	94.744	99.728
17)	MA 4,4'-DDT	6.362	7.342	136.3E6	1003.1E6	111.132	111.437
18)	B Endrin al...	6.438	7.257	101.2E6	756.5E6	101.912	105.884
19)	B Endosulfa...	6.651	7.482	105.5E6	724.7E6	84.227	82.585
20)	A Methoxychlor	6.913	7.795	309.1E6	1921.7E6	455.462	466.318
21)	B Endrin ke...	7.143	7.957	135.5E6	892.2E6	93.791	96.642

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050422\
Data File : PD069435.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 May 2022 16:31
Operator : AR\AJ
Sample : N2603-25MSD
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 04 23:21:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD041422CLP.M
Quant Title : GC Extractables
QLast Update : Thu Apr 21 02:24:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

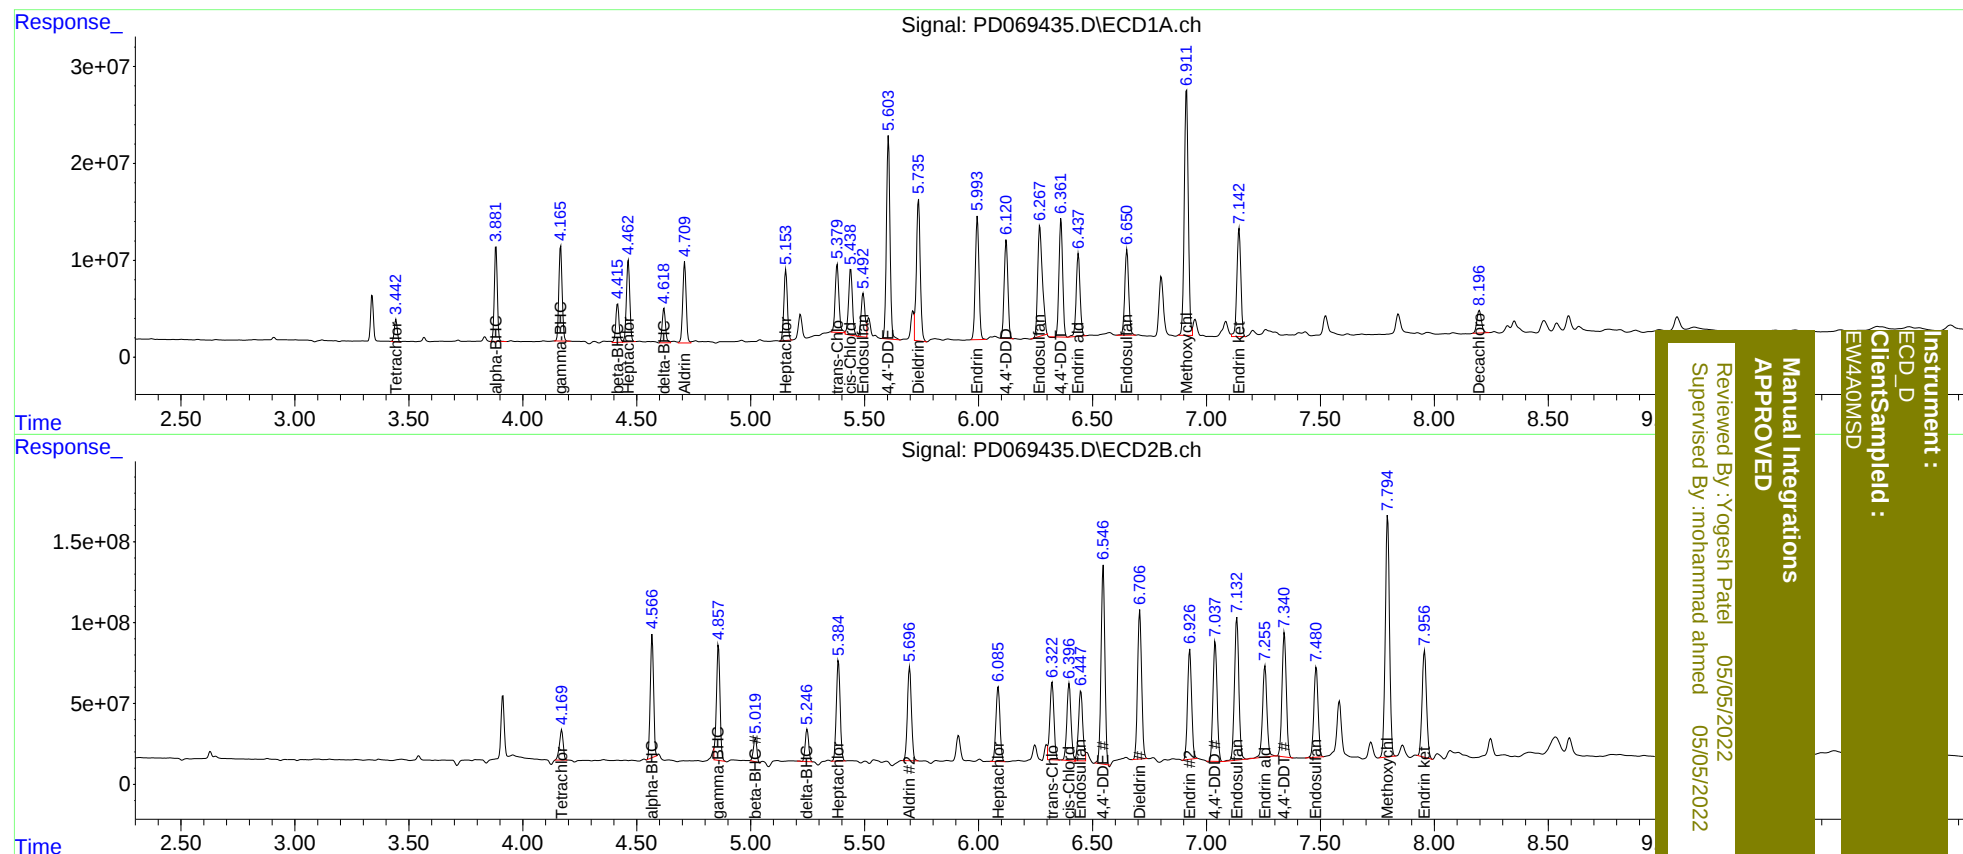

Instrument :
ECD_D
ClientSampled :
EW4A0MSD

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 05/05/2022
Supervised By : mohammad ahmed 05/05/2022