

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050823\
 Data File : PD075357.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 May 2023 22:26
 Operator : AR\AJ
 Sample : INDA413
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3237

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 09 04:25:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu May 04 02:14:07 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.771	47976016	22770012	21.034	21.588
27)	SA Decachlor...	9.092	7.918	87082723	36352066	35.189	38.493
Target Compounds							
2)	A alpha-BHC	4.005	3.273	76995834	31939612	20.022	20.620
3)	MA gamma-BHC...	4.338	3.603	72141596	29530503	20.067	20.090
4)	MA Heptachlor	4.930	3.944	73925683	28998990	19.830	19.846
9)	A Endosulfan I	6.086	5.097	60135755	24163472	19.936	20.134
13)	MA Dieldrin	6.362	5.362	133.3E6	52987135	38.967	38.836
14)	MA Endrin	6.593	5.638	105.7E6	44511156	36.565	36.595
16)	A 4,4'-DDD	6.726	5.786	105.9E6	43071474	43.812	43.446
17)	MA 4,4'-DDT	7.042	6.038	82272561	32987205	32.413	32.730
20)	A Methoxychlor	7.517	6.613	247.8E6	98591134	168.670	172.126

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD050823\
Data File : PD075357.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 May 2023 22:26
Operator : AR\AJ
Sample : INDA413
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 09 04:25:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050323CLP.M
Quant Title : GC Extractables
QLast Update : Thu May 04 02:14:07 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

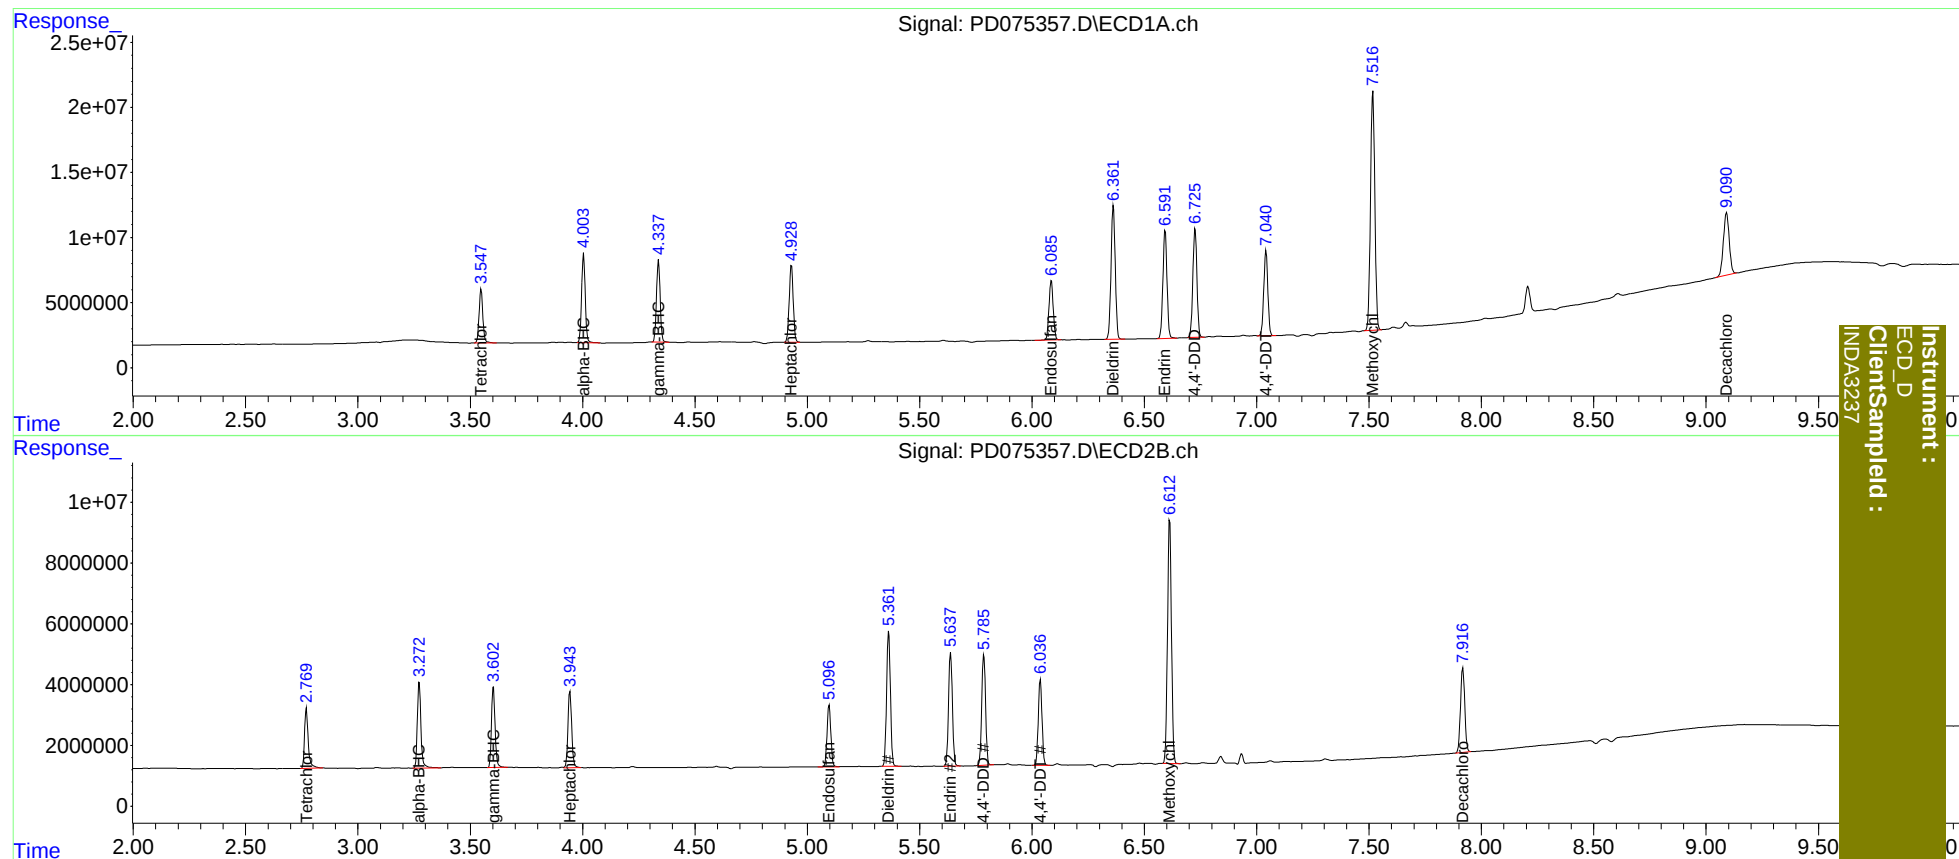

Instrument :
ECD_D
ClientSampled :
INDA3237