

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051321\
 Data File : PD062886.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2021 10:49
 Operator : AR\AJ
 Sample : M2335-01 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 OK-02-050721

Manual Integrations
 APPROVED

Ankita
 5/14/2021 11:14:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 11:48:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
 Quant Title : GC Extractables
 QLast Update : Thu May 06 08:49:38 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.442	3.970	1960862	7414781	2.205	0.640 #
28) SA Decachlor...	8.197	9.026	1962381	21798926	1.854	1.889
Target Compounds						
10) B gamma-Chl...	5.380	6.077	841403	5506284	0.715	0.346m#
11) B alpha-Chl...	5.438	6.147	423079	7890880	0.365m	0.517m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051321\
Data File : PD062886.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2021 10:49
Operator : AR\AJ
Sample : M2335-01 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
OK-02-050721


Manual Integrations
APPROVED

Ankita
5/14/2021 11:14:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 11:48:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD050621.M
Quant Title : GC Extractables
QLast Update : Thu May 06 08:49:38 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

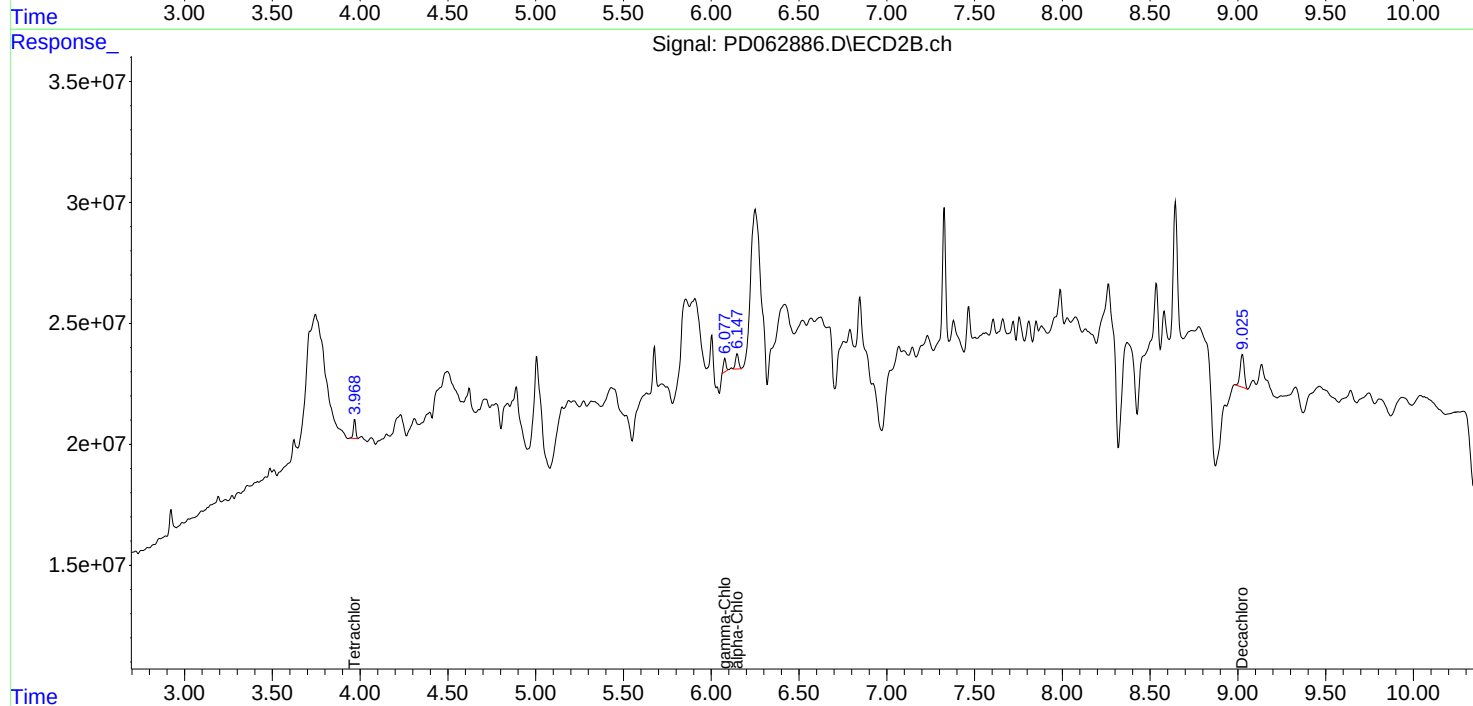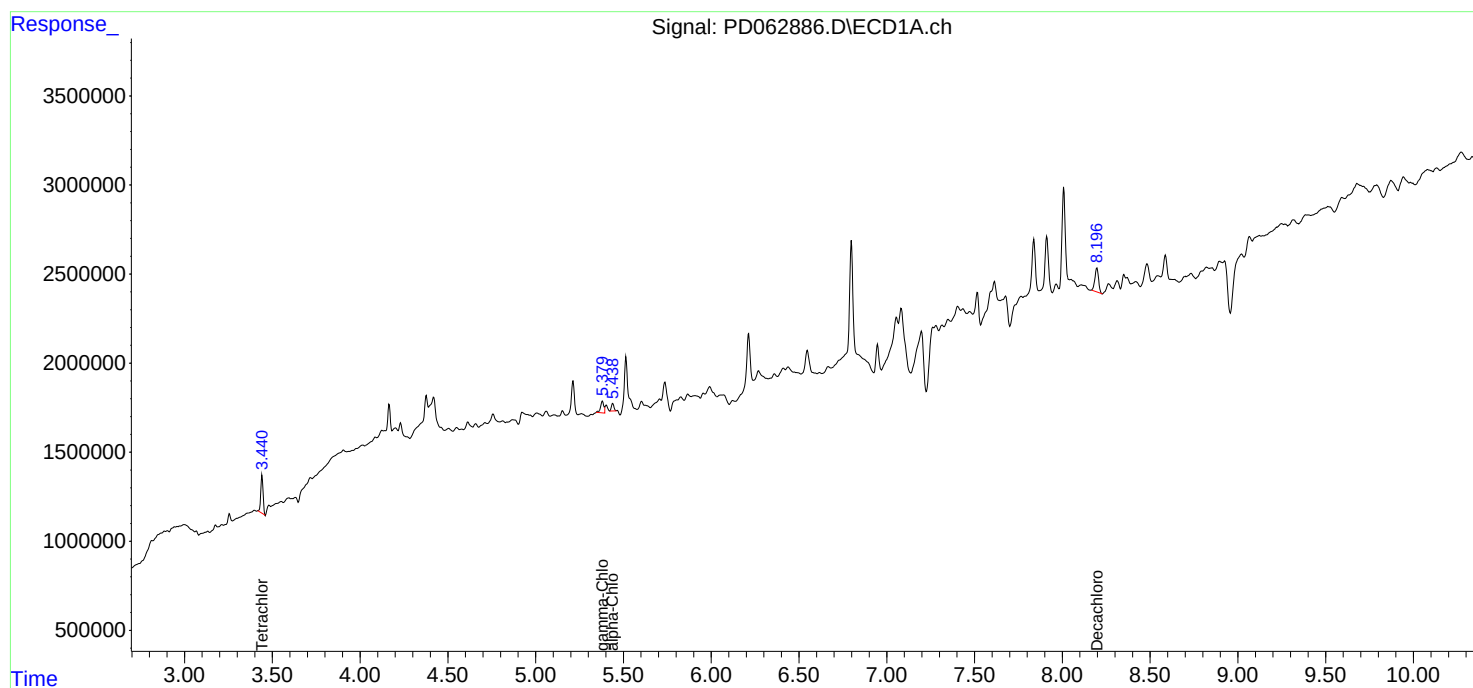

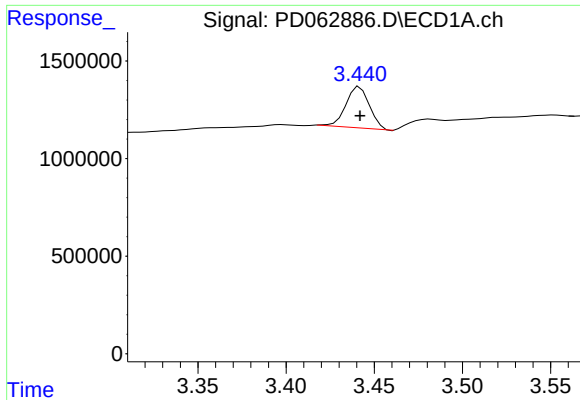


#1 Tetrachloro-m-xylene

R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 1960862
Conc: 2.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
OK-02-050721


Manual Integrations
APPROVED

Ankita
5/14/2021 11:14:21 AM

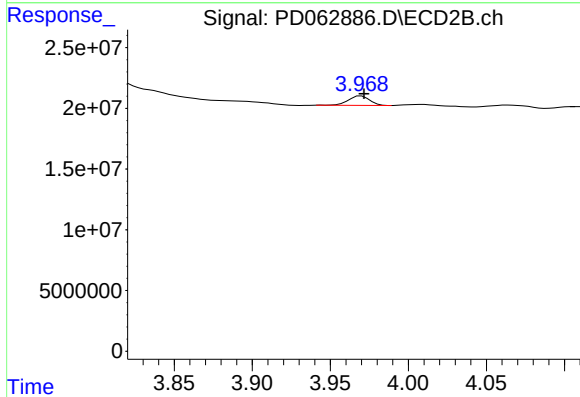


#1 Tetrachloro-m-xylene

R.T.: 3.970 min
Delta R.T.: -0.002 min
Response: 7414781
Conc: 0.64 ng/ml

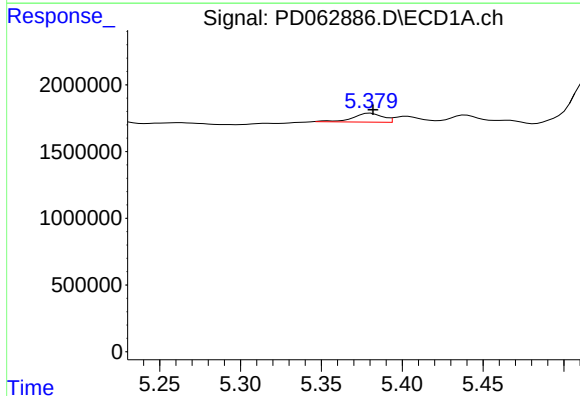


#10 gamma-Chlordane

R.T.: 5.380 min
Delta R.T.: -0.001 min
Response: 841403
Conc: 0.71 ng/ml

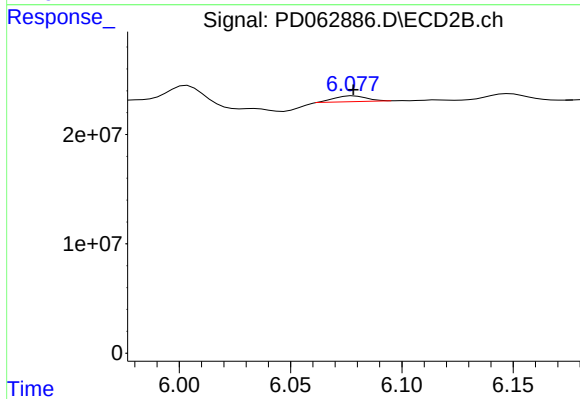

#10 gamma-Chlordane

R.T.: 6.077 min
Delta R.T.: -0.001 min
Response: 5506284
Conc: 0.35 ng/ml m

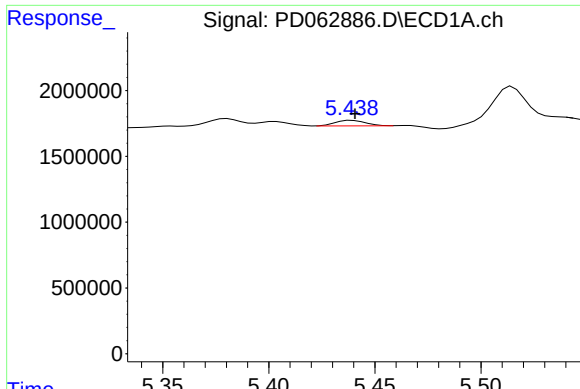


#11 alpha-Chlordane

R.T.: 5.438 min
Delta R.T.: -0.003 min
Response: 423079
Conc: 0.37 ng/ml m

Instrument :
ECD_D
ClientSampleId :
OK-02-050721


Manual Integrations
APPROVED

Ankita
5/14/2021 11:14:21 AM

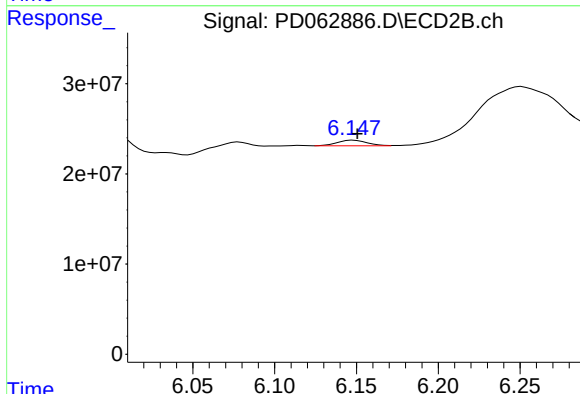


#11 alpha-Chlordane

R.T.: 6.147 min
Delta R.T.: -0.004 min
Response: 7890880
Conc: 0.52 ng/ml m

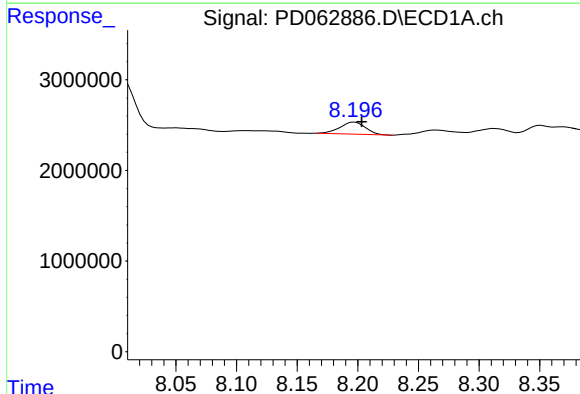

#28 Decachlorobiphenyl

R.T.: 8.197 min
Delta R.T.: -0.006 min
Response: 1962381
Conc: 1.85 ng/ml

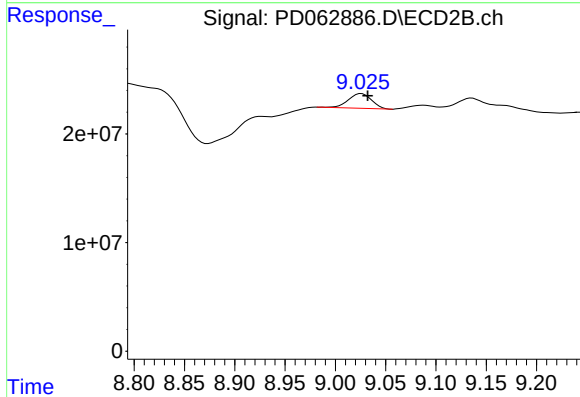

#28 Decachlorobiphenyl

R.T.: 9.026 min
Delta R.T.: -0.006 min
Response: 21798926
Conc: 1.89 ng/ml