

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051324\
 Data File : PD082758.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2024 12:43
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 15:12:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051324.M
 Quant Title : GC Extractables
 QLast Update : Mon May 13 15:07:37 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.774	97478476	315.1E6	74.822	75.008
28)	SA Decachlor...	9.121	7.906	129.2E6	252.5E6	75.063	74.857
Target Compounds							
23)	Chlordane-1	4.733	3.769	70030018	135.6E6	741.328	743.185
24)	Chlordane-2	5.264	4.344	70515660	150.0E6	742.953	740.877
25)	Chlordane-3	5.978	4.974	296.1E6	446.5E6	743.198	744.018
26)	Chlordane-4	6.060	5.037	349.0E6	424.1E6	743.598	743.439
27)	Chlordane-5	6.914	5.931	61161146	150.2E6	740.905	740.172



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051324\
Data File : PD082758.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2024 12:43
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 15:12:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051324.M
Quant Title : GC Extractables
QLast Update : Mon May 13 15:07:37 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

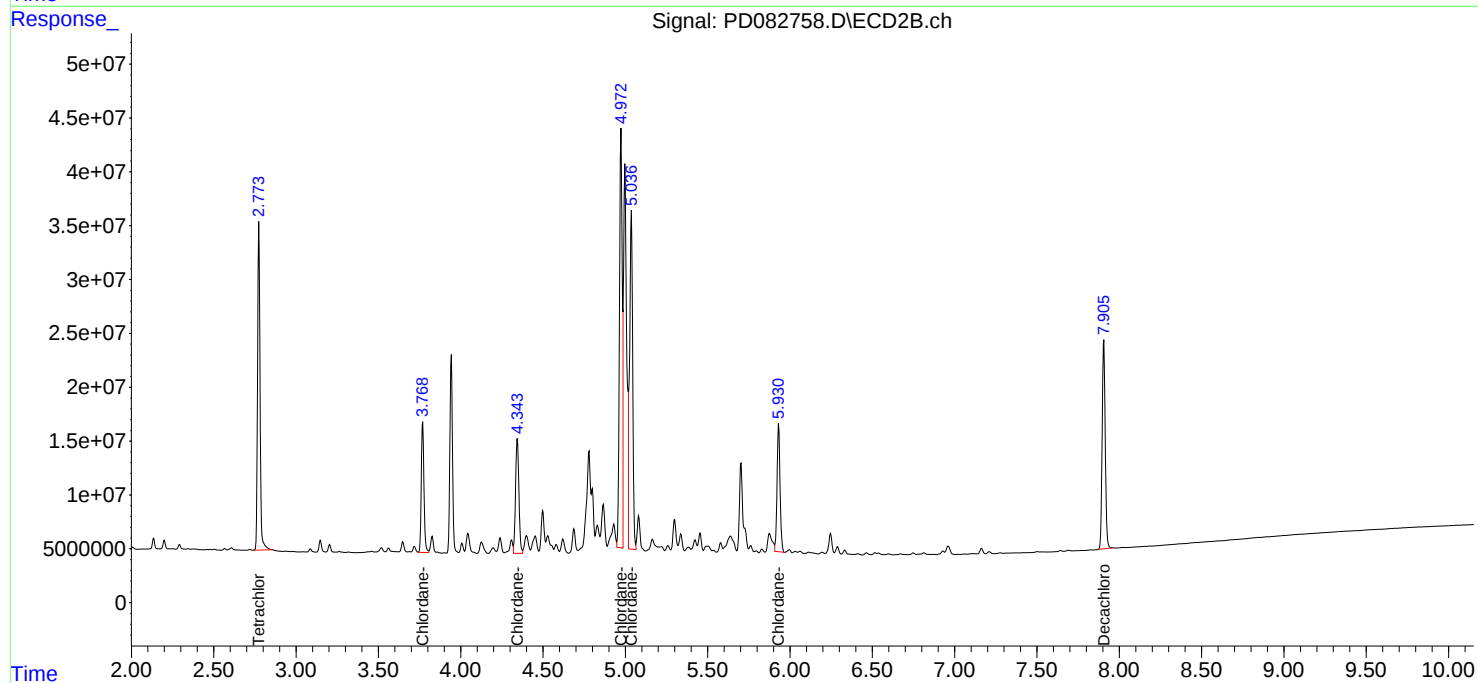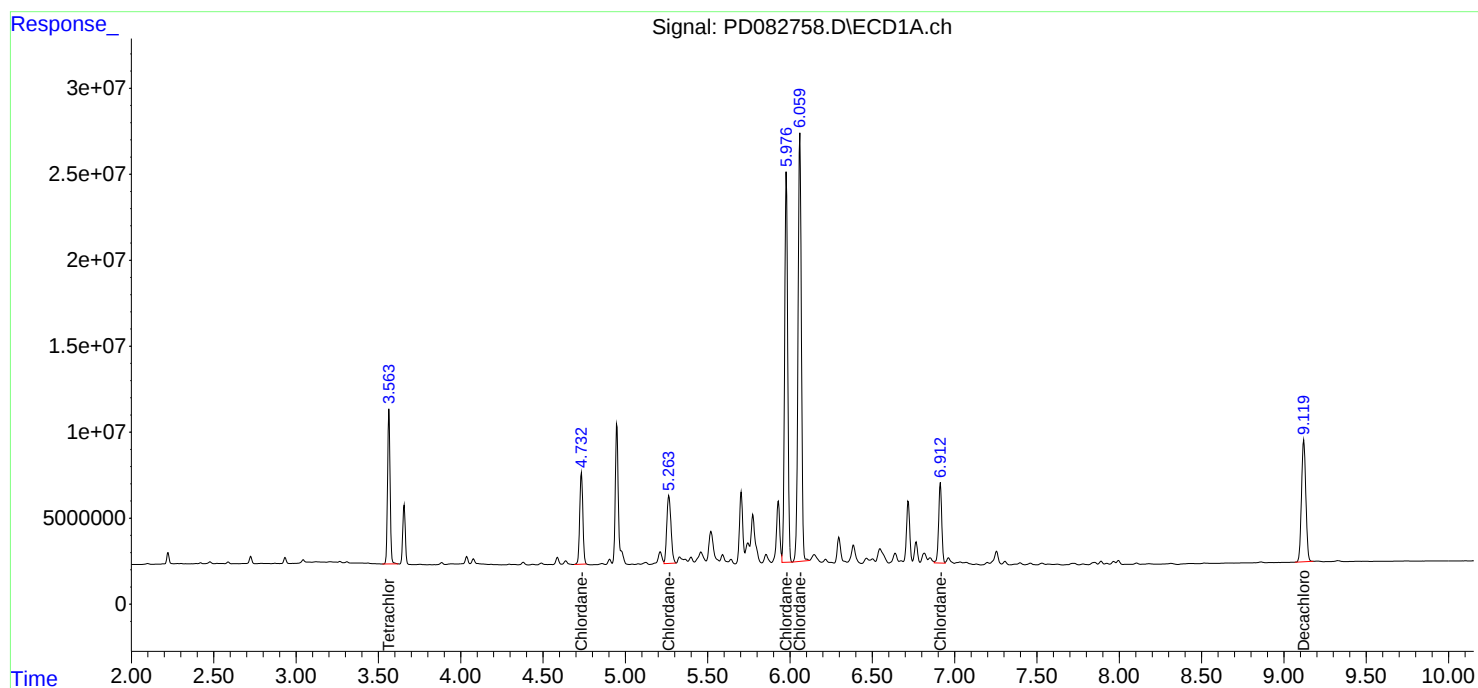


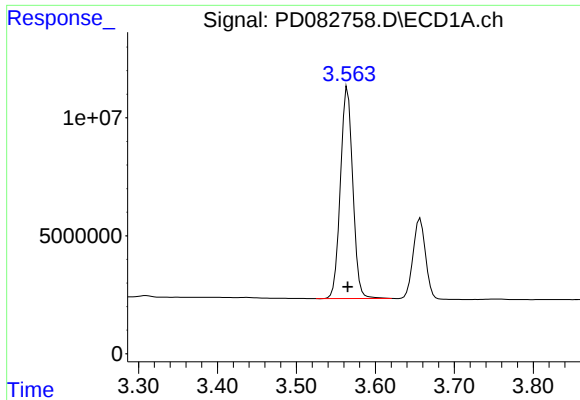

#1 Tetrachloro-m-xylene


R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 97478476
Conc: 74.82 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

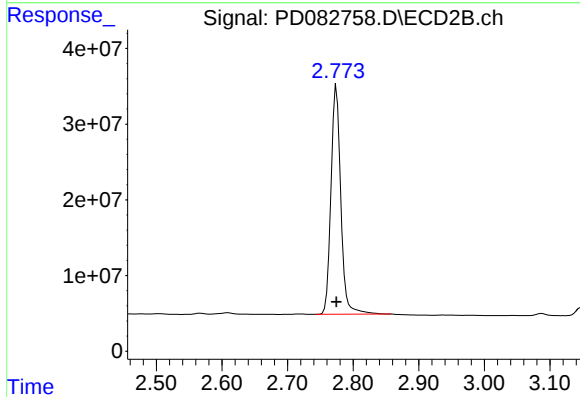


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: 0.000 min
Response: 315066134
Conc: 75.01 ng/ml

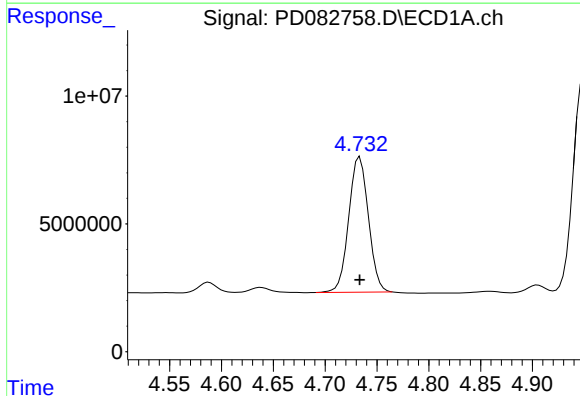


#23 Chlordane-1

R.T.: 4.733 min
Delta R.T.: 0.000 min
Response: 70030018
Conc: 741.33 ng/ml

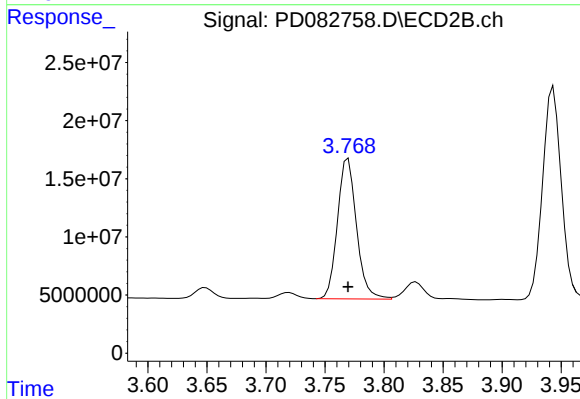

#23 Chlordane-1


R.T.: 3.769 min
Delta R.T.: 0.000 min
Response: 135637839
Conc: 743.19 ng/ml

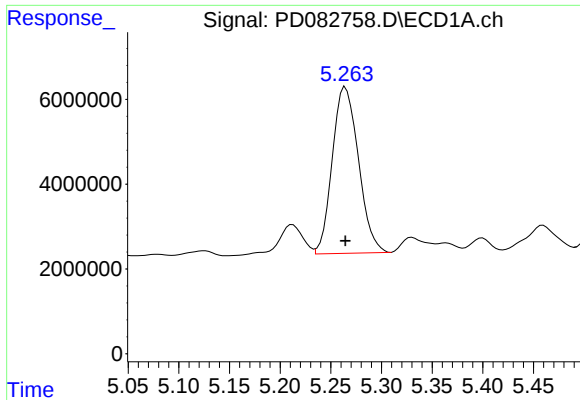

#24 Chlordane-2


R.T.: 5.264 min
Delta R.T.: 0.000 min
Response: 70515660
Conc: 742.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

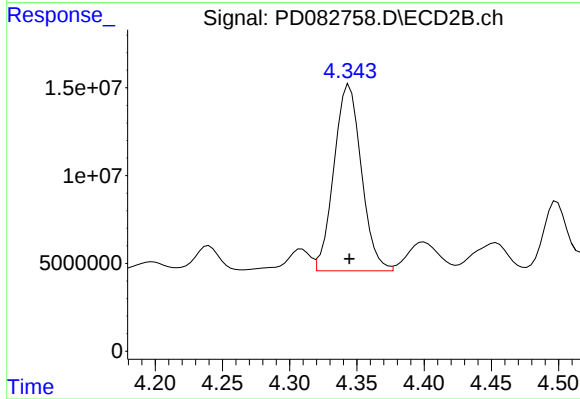


#24 Chlordane-2

R.T.: 4.344 min
Delta R.T.: 0.000 min
Response: 150036638
Conc: 740.88 ng/ml

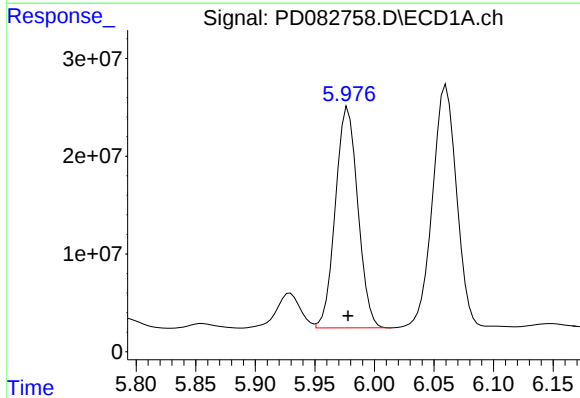


#25 Chlordane-3

R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 296095921
Conc: 743.20 ng/ml

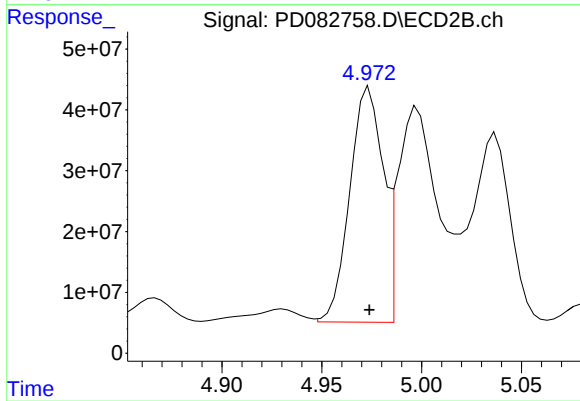

#25 Chlordane-3


R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 446532252
Conc: 744.02 ng/ml

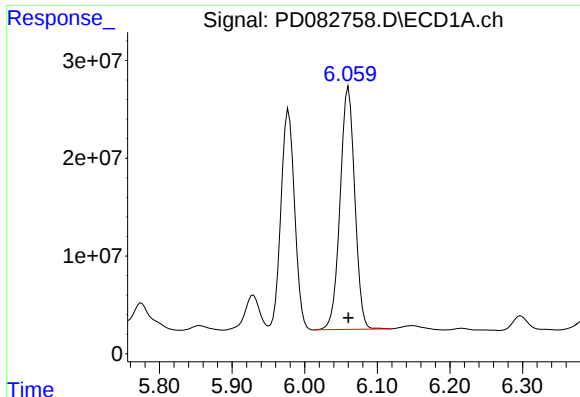

#26 Chlordane-4


R.T.: 6.060 min
Delta R.T.: 0.000 min
Response: 349010914
Conc: 743.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

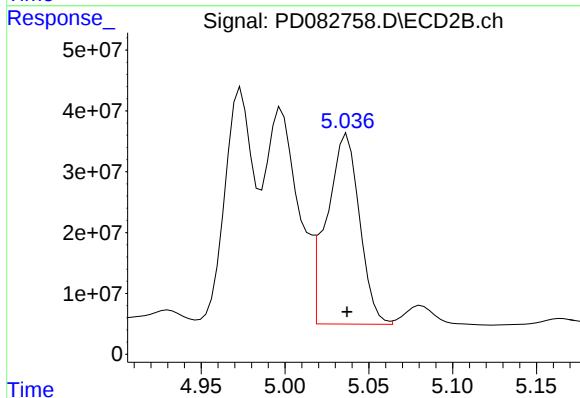


#26 Chlordane-4

R.T.: 5.037 min
Delta R.T.: 0.000 min
Response: 424111785
Conc: 743.44 ng/ml

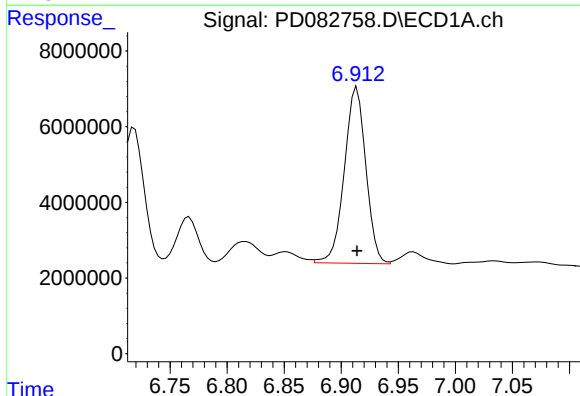


#27 Chlordane-5

R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 61161146
Conc: 740.91 ng/ml

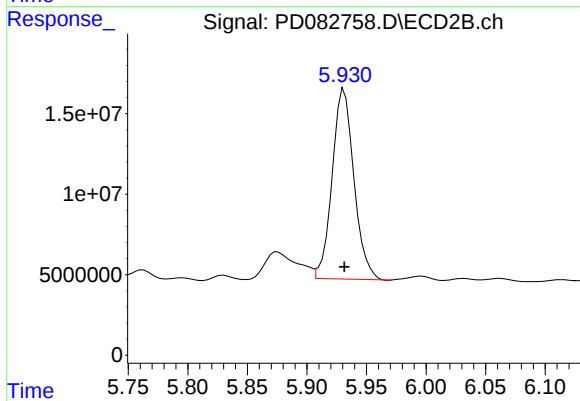

#27 Chlordane-5


R.T.: 5.931 min
Delta R.T.: 0.000 min
Response: 150175857
Conc: 740.17 ng/ml

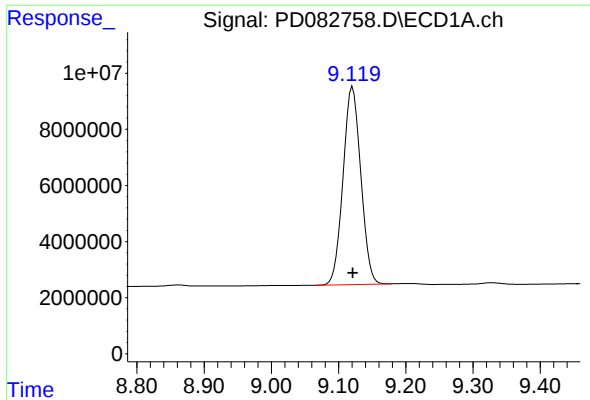

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: 0.000 min
Response: 129172978
Conc: 75.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC750

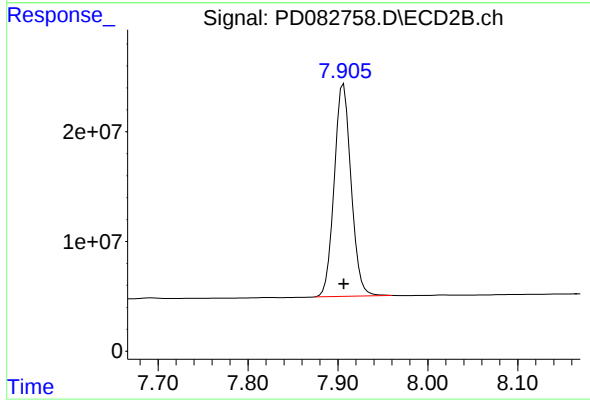

#28 Decachlorobiphenyl

R.T.: 7.906 min
Delta R.T.: 0.000 min
Response: 252462816
Conc: 74.86 ng/ml