

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051324\
 Data File : PD082751.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2024 11:10
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 15:40:51 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051324.M
 Quant Title : GC Extractables
 QLast Update : Mon May 13 15:39:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.565	2.776	29688297	75699475	19.176	19.100
28)	SA Decachlor...	9.121	7.906	40142326	74901749	20.102	19.378
Target Compounds							
9)	A Endosulfan I	6.107	5.093	19004417	39031187	8.801	8.462
10)	B gamma-Chl...	5.977	4.973	20956302	45021158	9.253	9.006
12)	B 4,4'-DDE	6.228	5.226	41416513	85740567	18.930	18.368
13)	MA Dieldrin	6.383	5.357	40838502	89815778	18.261	17.870
19)	B Endosulfa...	7.199	6.327	33855966	73852918	19.188	18.522
20)	A Methoxychlor	7.539	6.605	84055418	182.0E6	91.698	89.577
21)	B Endrin ke...	7.687	6.833	36130497	84057299	18.798	18.491



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051324\
Data File : PD082751.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2024 11:10
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 15:40:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051324.M
Quant Title : GC Extractables
QLast Update : Mon May 13 15:39:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

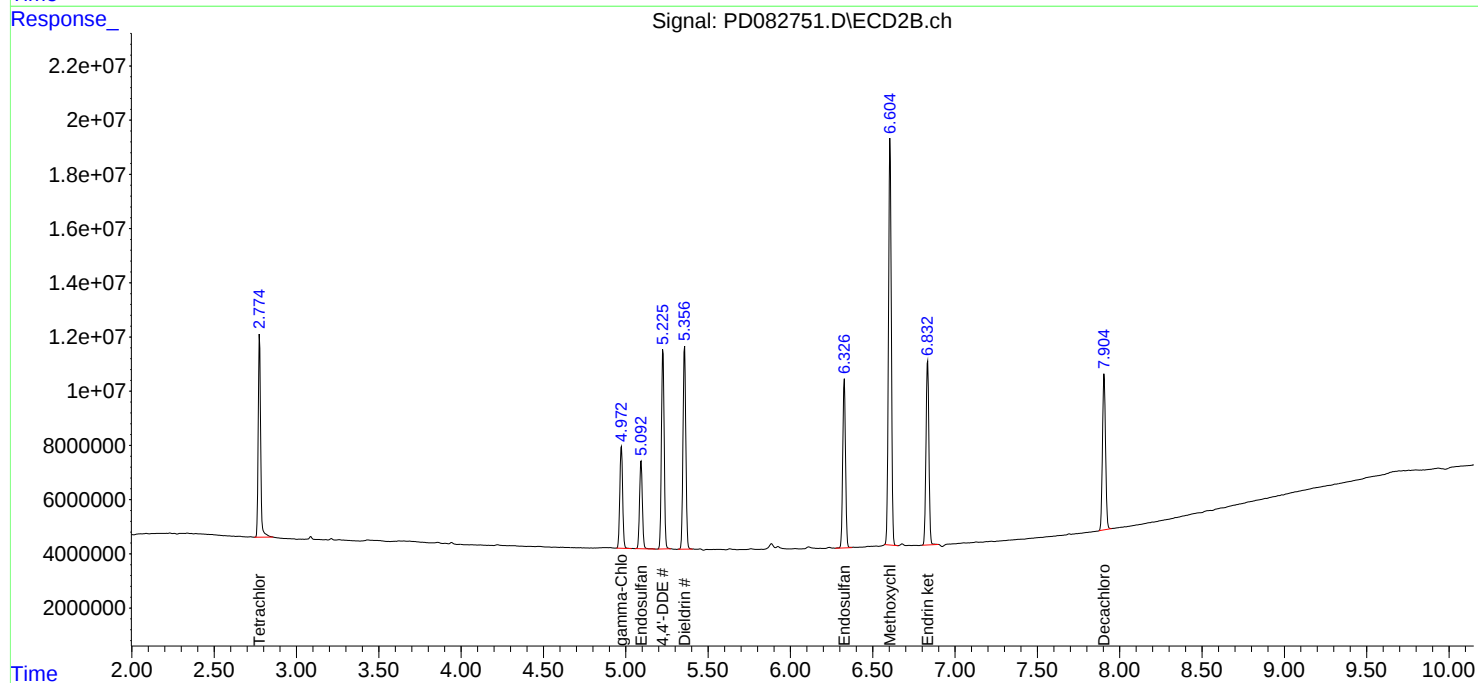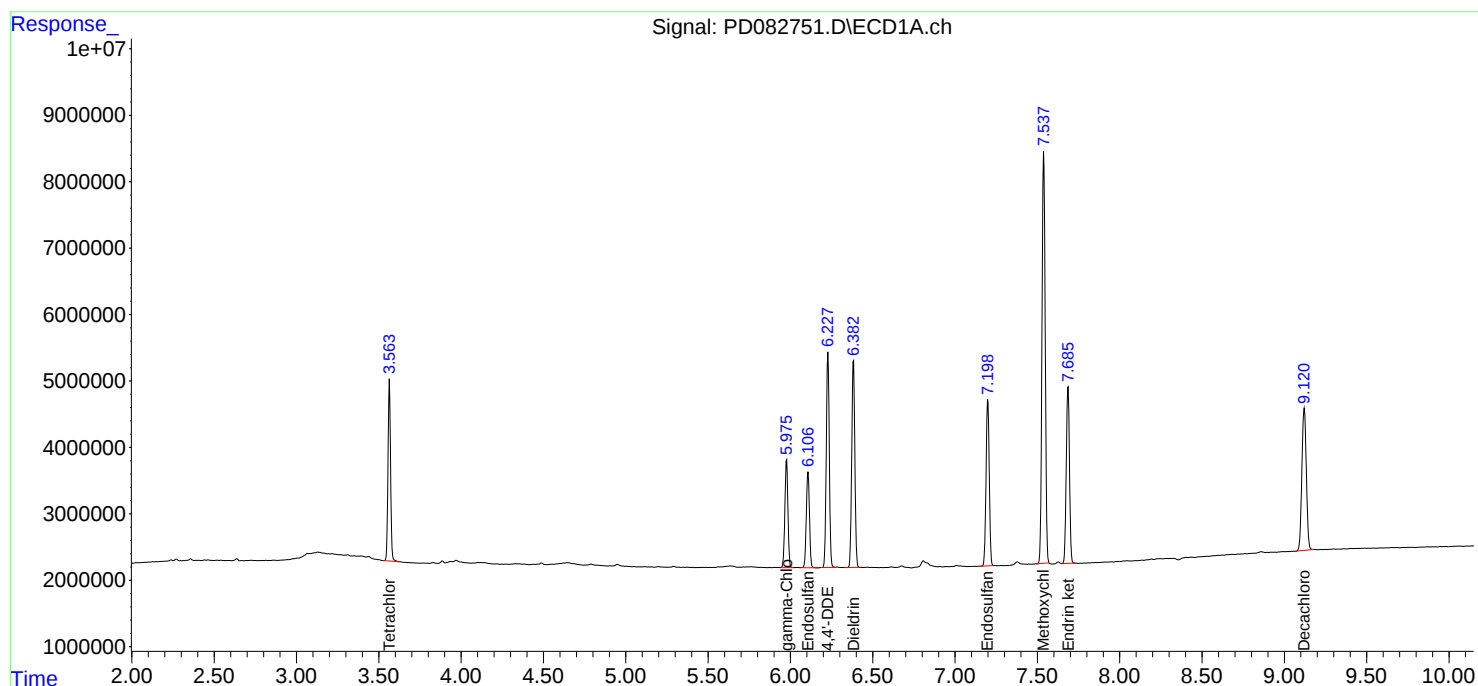


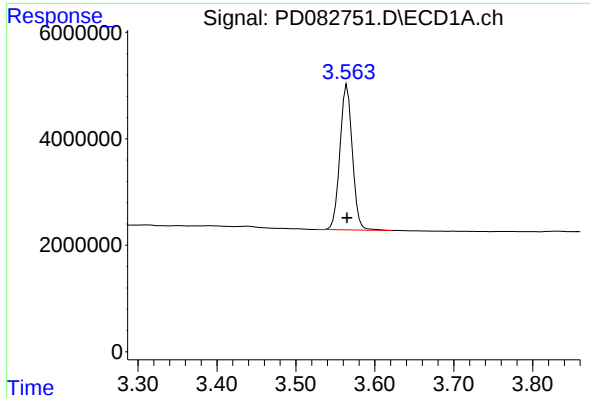

#1 Tetrachloro-m-xylene


R.T.: 3.565 min
Delta R.T.: 0.000 min
Response: 29688297
Conc: 19.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

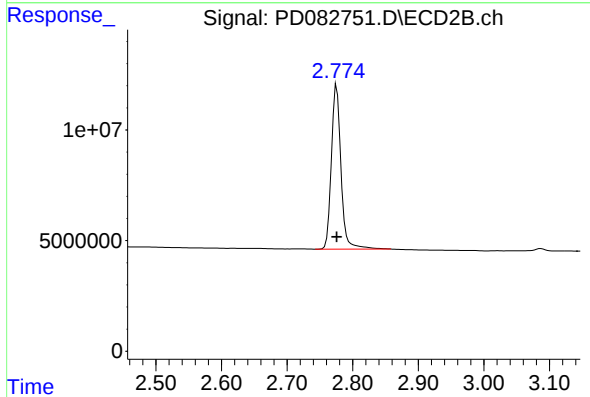


#1 Tetrachloro-m-xylene

R.T.: 2.776 min
Delta R.T.: 0.000 min
Response: 75699475
Conc: 19.10 ng/ml

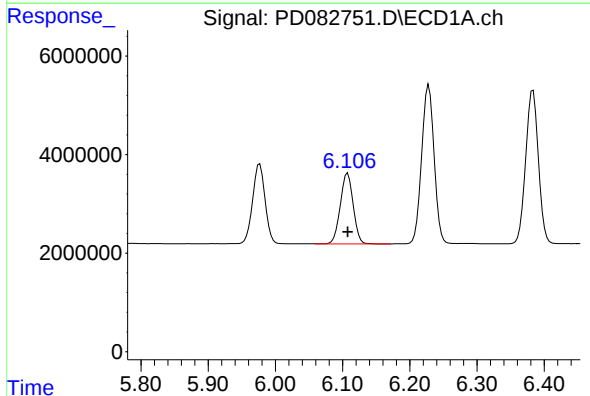


#9 Endosulfan I

R.T.: 6.107 min
Delta R.T.: 0.000 min
Response: 19004417
Conc: 8.80 ng/ml

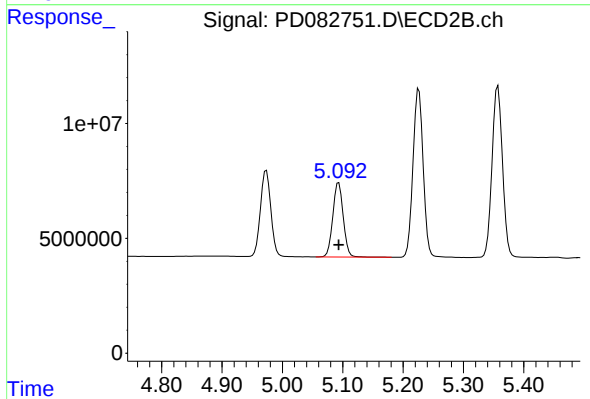

#9 Endosulfan I


R.T.: 5.093 min
Delta R.T.: 0.000 min
Response: 39031187
Conc: 8.46 ng/ml

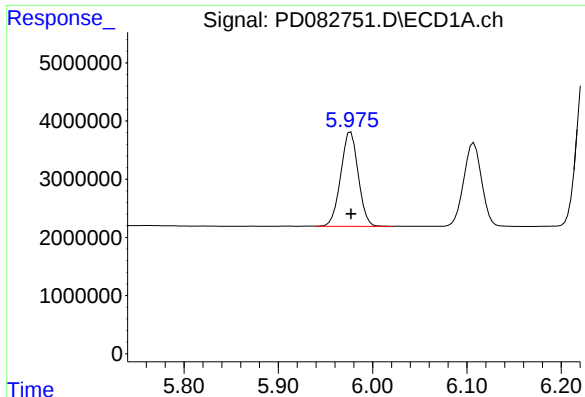

#10 gamma-Chlordane


R.T.: 5.977 min
Delta R.T.: 0.000 min
Response: 20956302
Conc: 9.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

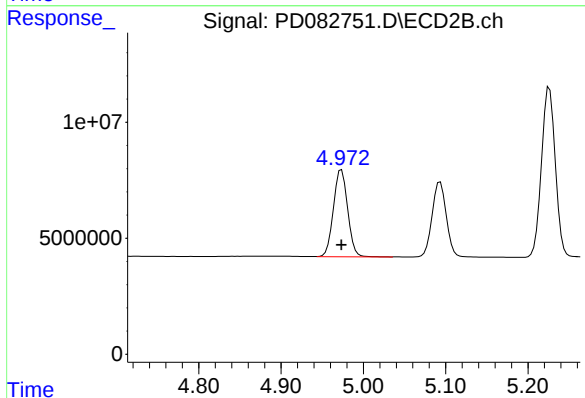


#10 gamma-Chlordane

R.T.: 4.973 min
Delta R.T.: 0.000 min
Response: 45021158
Conc: 9.01 ng/ml

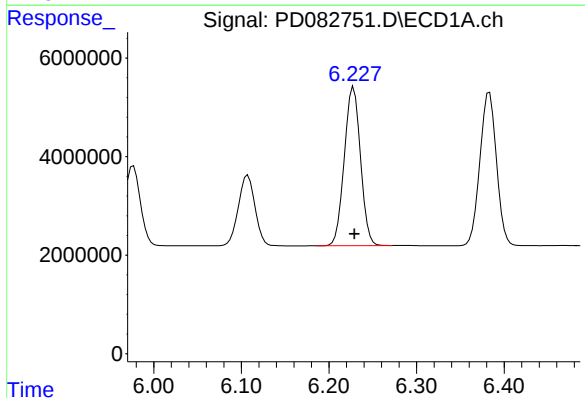


#12 4,4'-DDE

R.T.: 6.228 min
Delta R.T.: -0.001 min
Response: 41416513
Conc: 18.93 ng/ml

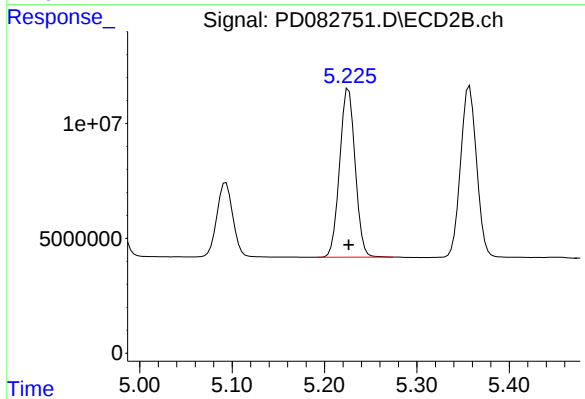

#12 4,4'-DDE


R.T.: 5.226 min
Delta R.T.: 0.000 min
Response: 85740567
Conc: 18.37 ng/ml

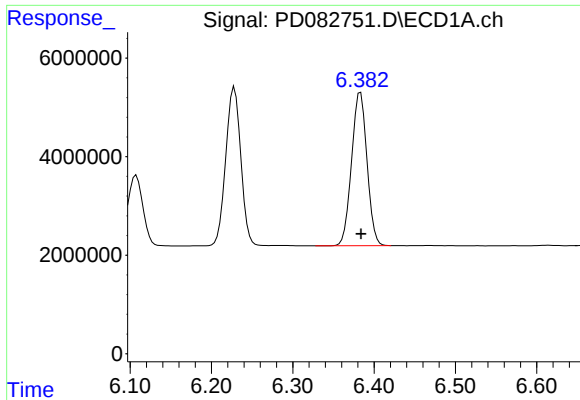

#13 Dieldrin


R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 40838502
Conc: 18.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

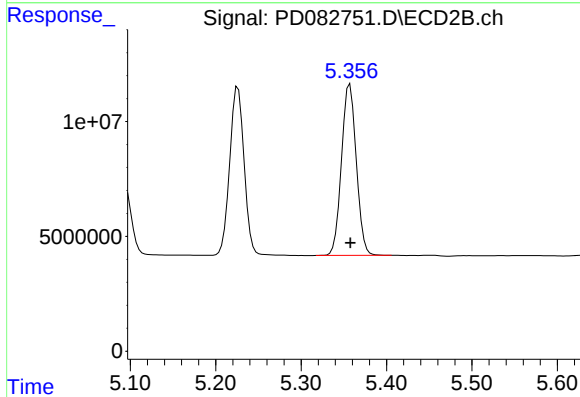


#13 Dieldrin

R.T.: 5.357 min
Delta R.T.: 0.000 min
Response: 89815778
Conc: 17.87 ng/ml

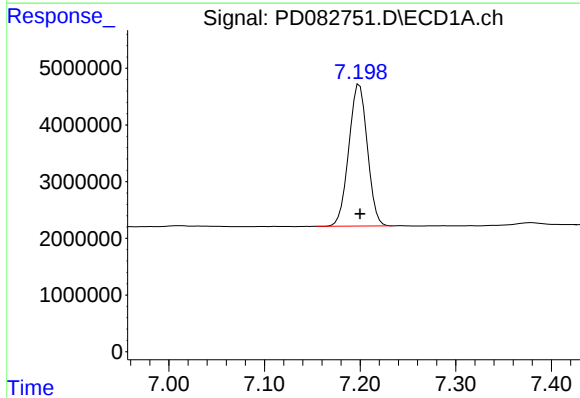


#19 Endosulfan Sulfate

R.T.: 7.199 min
Delta R.T.: 0.000 min
Response: 33855966
Conc: 19.19 ng/ml

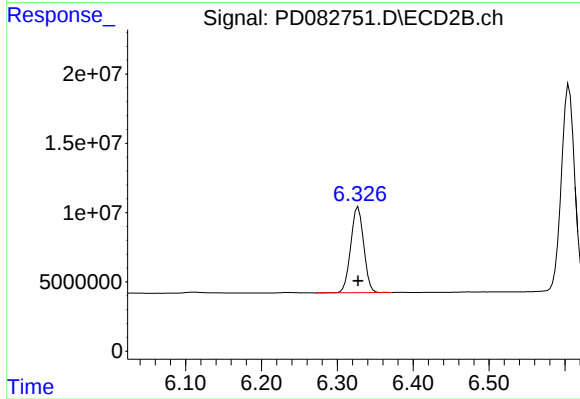

#19 Endosulfan Sulfate


R.T.: 6.327 min
Delta R.T.: 0.000 min
Response: 73852918
Conc: 18.52 ng/ml

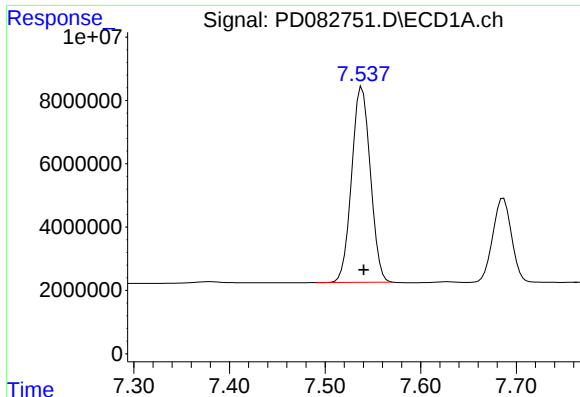

#20 Methoxychlor


R.T.: 7.539 min
Delta R.T.: -0.002 min
Response: 84055418
Conc: 91.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

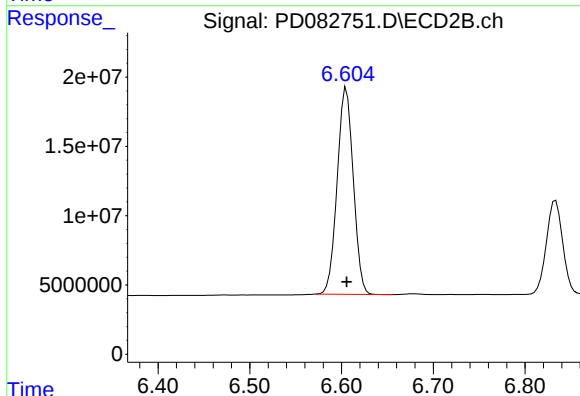


#20 Methoxychlor

R.T.: 6.605 min
Delta R.T.: 0.000 min
Response: 182015674
Conc: 89.58 ng/ml

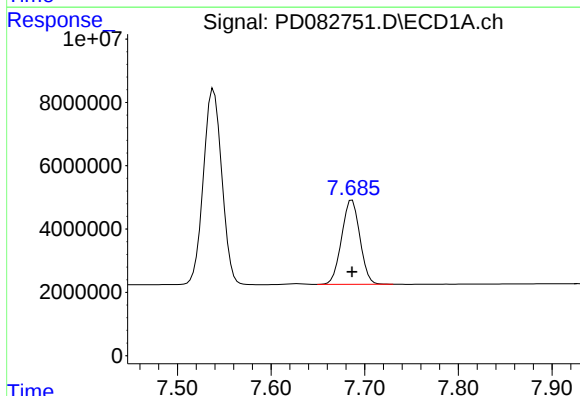


#21 Endrin ketone

R.T.: 7.687 min
Delta R.T.: 0.000 min
Response: 36130497
Conc: 18.80 ng/ml

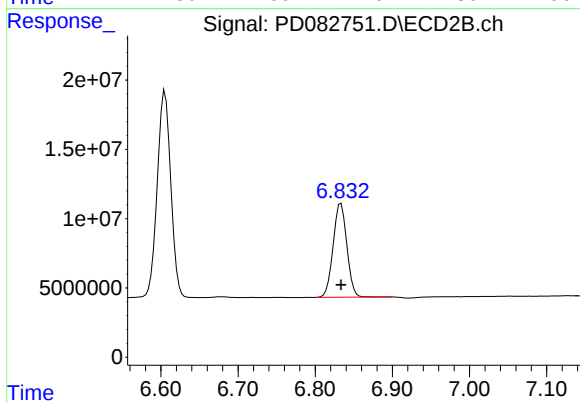

#21 Endrin ketone


R.T.: 6.833 min
Delta R.T.: 0.000 min
Response: 84057299
Conc: 18.49 ng/ml

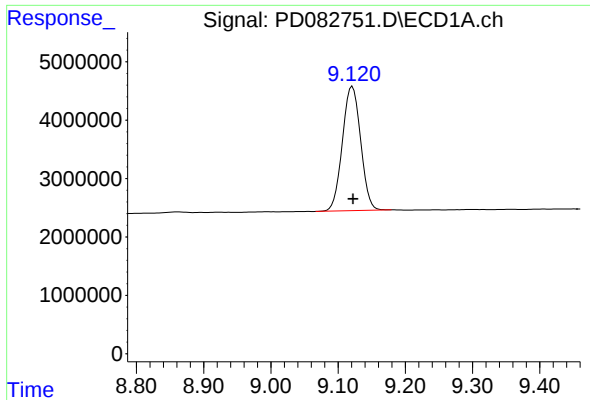

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: -0.001 min
Response: 40142326
Conc: 20.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

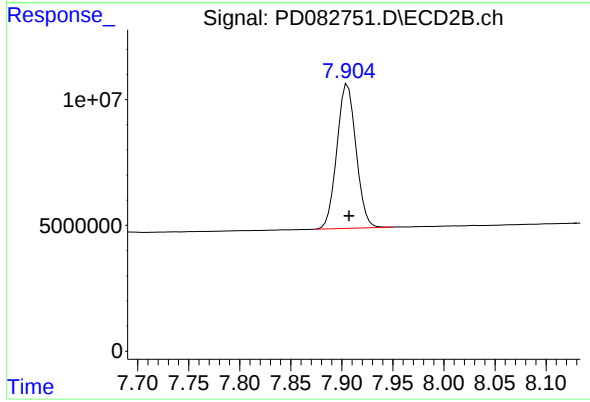

#28 Decachlorobiphenyl

R.T.: 7.906 min
Delta R.T.: -0.001 min
Response: 74901749
Conc: 19.38 ng/ml