

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051324\
 Data File : PD082768.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2024 14:57
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD051324

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 15:17:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051324.M
 Quant Title : GC Extractables
 QLast Update : Mon May 13 15:16:46 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.564	2.774	66794576	216.6E6	48.730	50.109
28)	SA Decachlor...	9.121	7.906	91168771	180.0E6	47.846	48.384
Target Compounds							
23)	Chlordane-1	4.733	3.769	46799993	92525853	488.812	505.145
24)	Chlordane-2	5.265	4.344	47977715	104.8E6	484.775	494.654
25)	Chlordane-3	5.978	4.973	195.4E6	304.3E6	495.954	504.891
26)	Chlordane-4	6.060	5.036	232.2E6	289.8E6	494.255	504.396
27)	Chlordane-5	6.913	5.931	40388489	102.5E6	490.918	508.107



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD051324\
Data File : PD082768.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2024 14:57
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD051324

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 15:17:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD051324.M
Quant Title : GC Extractables
QLast Update : Mon May 13 15:16:46 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

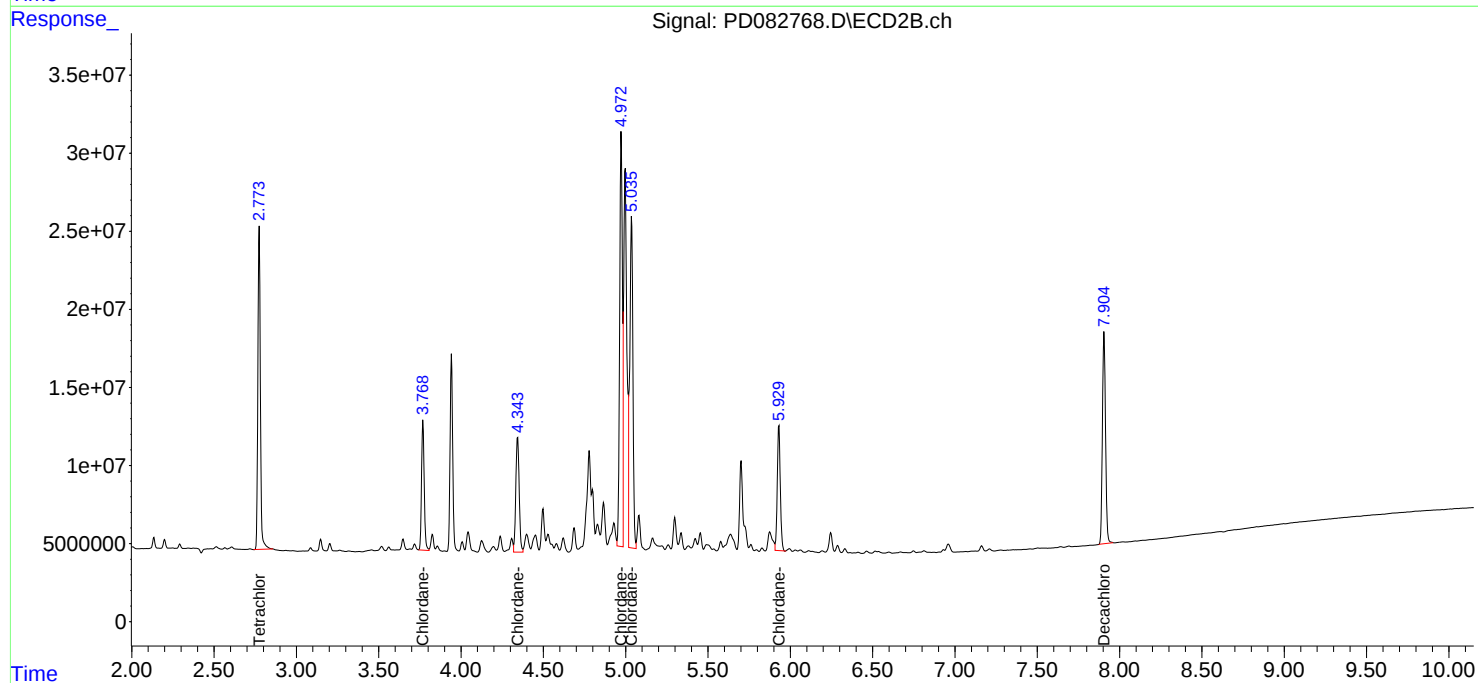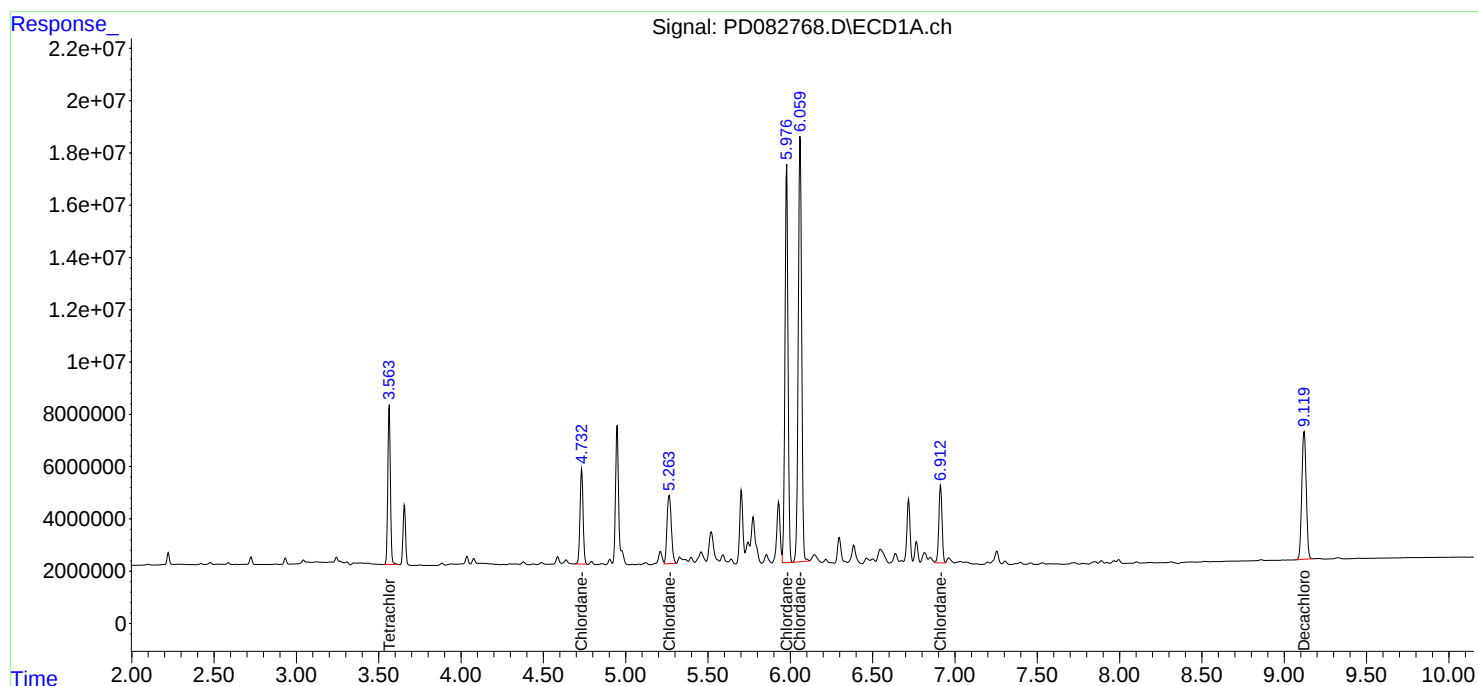


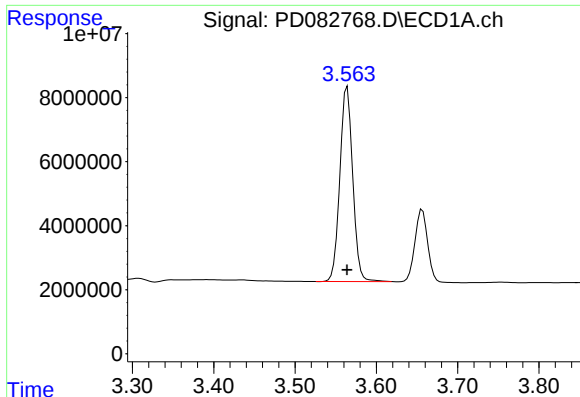

#1 Tetrachloro-m-xylene


R.T.: 3.564 min
Delta R.T.: 0.000 min
Response: 66794576
Conc: 48.73 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD051324

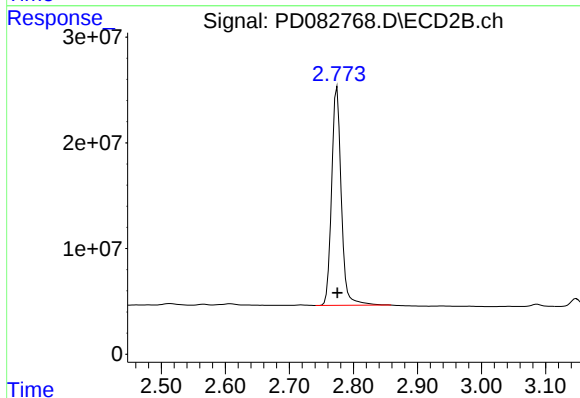


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: 0.000 min
Response: 216579153
Conc: 50.11 ng/ml

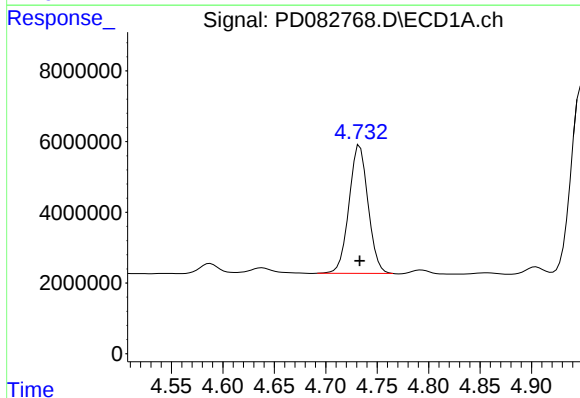


#23 Chlordane-1

R.T.: 4.733 min
Delta R.T.: 0.000 min
Response: 46799993
Conc: 488.81 ng/ml

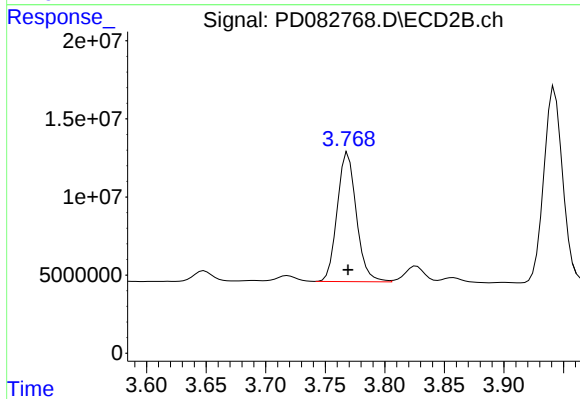

#23 Chlordane-1


R.T.: 3.769 min
Delta R.T.: 0.000 min
Response: 92525853
Conc: 505.14 ng/ml

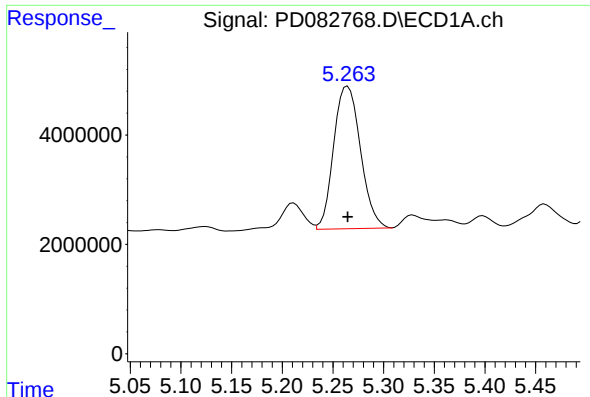

#24 Chlordane-2


R.T.: 5.265 min
Delta R.T.: 0.000 min
Response: 47977715
Conc: 484.78 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD051324

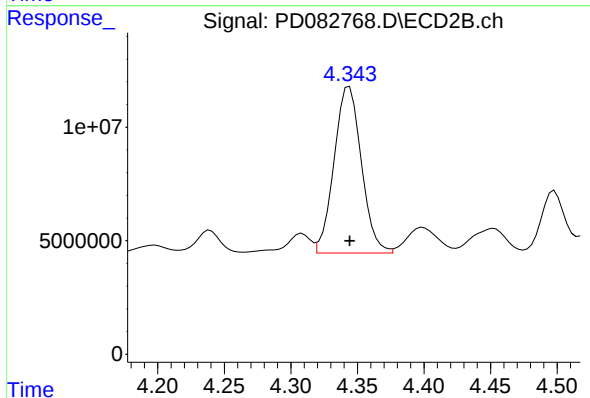


#24 Chlordane-2

R.T.: 4.344 min
Delta R.T.: 0.000 min
Response: 104807296
Conc: 494.65 ng/ml

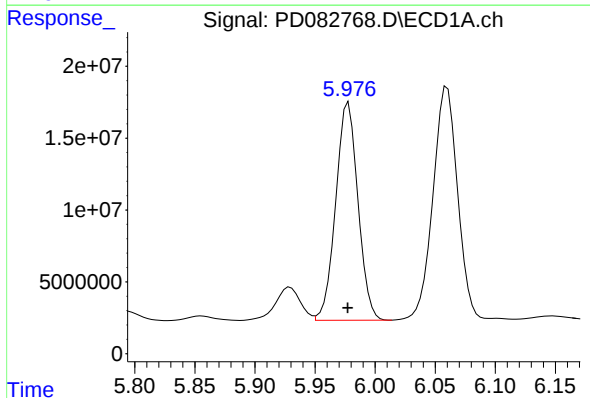


#25 Chlordane-3

R.T.: 5.978 min
Delta R.T.: 0.000 min
Response: 195433722
Conc: 495.95 ng/ml

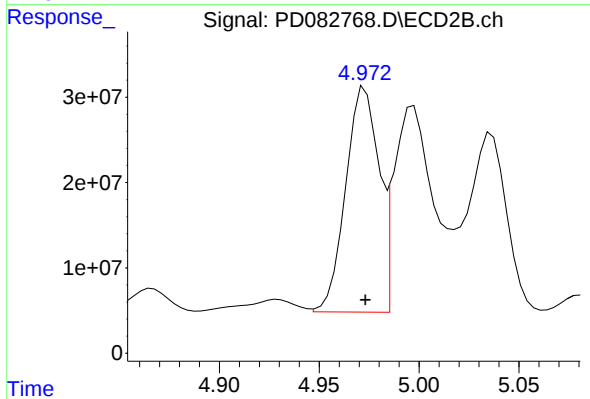

#25 Chlordane-3


R.T.: 4.973 min
Delta R.T.: 0.000 min
Response: 304280147
Conc: 504.89 ng/ml

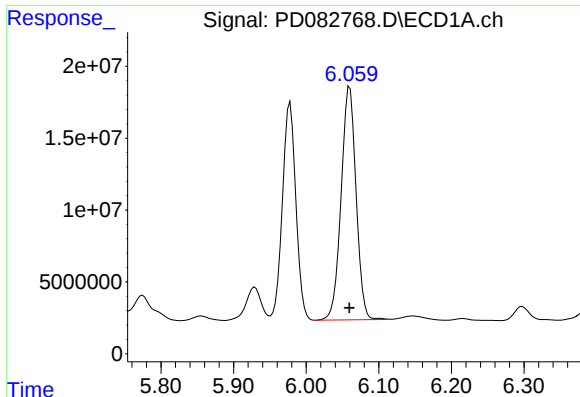

#26 Chlordane-4


R.T.: 6.060 min
Delta R.T.: 0.000 min
Response: 232175478
Conc: 494.26 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD051324

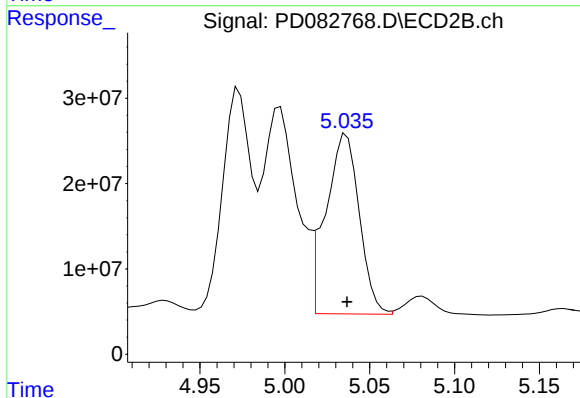


#26 Chlordane-4

R.T.: 5.036 min
Delta R.T.: 0.000 min
Response: 289841505
Conc: 504.40 ng/ml

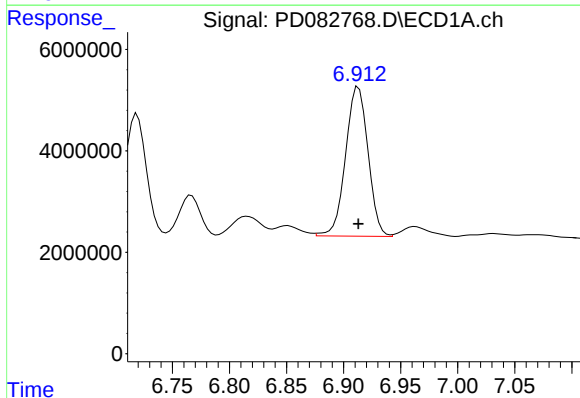


#27 Chlordane-5

R.T.: 6.913 min
Delta R.T.: 0.000 min
Response: 40388489
Conc: 490.92 ng/ml

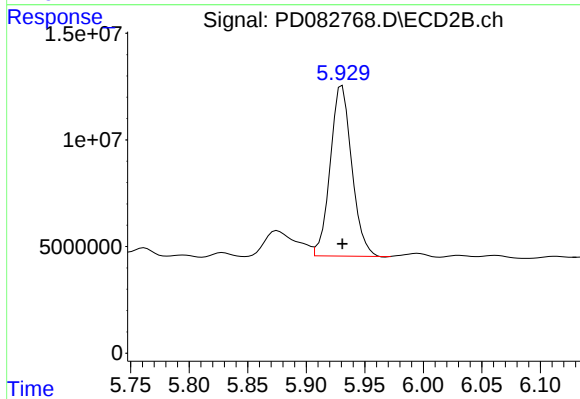

#27 Chlordane-5


R.T.: 5.931 min
Delta R.T.: 0.000 min
Response: 102460313
Conc: 508.11 ng/ml

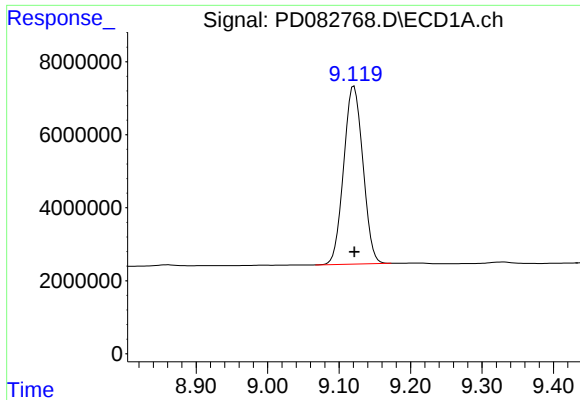

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: 0.000 min
Response: 91168771
Conc: 47.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
ICVPD051324

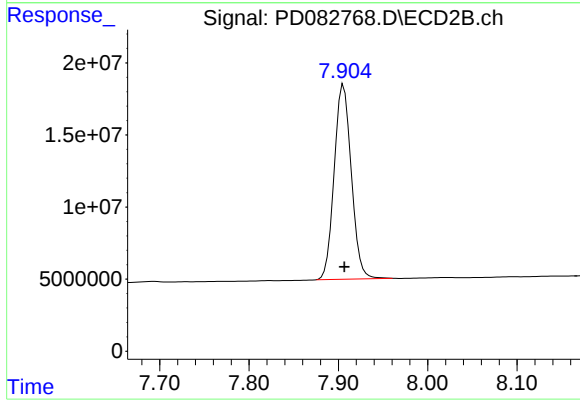

#28 Decachlorobiphenyl

R.T.: 7.906 min
Delta R.T.: 0.000 min
Response: 180021448
Conc: 48.38 ng/ml