

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060122\
 Data File : PD069930.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2022 09:36
 Operator : AR\AJ
 Sample : PB145093BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS093

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/01/2022
 Supervised By : Ankita Jodhani 06/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 11:40:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052922CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon May 30 09:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.441	4.168	21587968	214.3E6	21.061	21.861
27)	SA Decachlor...	8.193	9.362	47692770	276.6E6	45.334	45.767
Target Compounds							
2)	A alpha-BHC	3.878	4.564	6639990	77868621	4.572m	5.578
3)	MA gamma-BHC...	4.162	4.855	7477291	70156077	5.261m	5.307
4)	MA Heptachlor	4.458	5.382	6727042	72013287	4.960m	5.522
5)	MB Aldrin	4.707	5.694	6693348	72139350	4.908	5.577
6)	B beta-BHC	4.413	5.019	3346971	32137388	5.066	5.377
7)	B delta-BHC	4.617	5.244	3927487	33560016	2.789	2.833
8)	B Heptachlo...	5.150	6.082	6551197	67468190	5.228	6.412
9)	A Endosulfan I	5.489	6.445	6013599	59452724	5.213	5.864
10)	B trans-Chl...	5.376	6.319	6596680	63766800	5.204	5.656
11)	B cis-Chlor...	5.435	6.393	6429585	62500119	5.128	5.734
12)	B 4,4'-DDE	5.600	6.544	11797451	111.6E6	10.312	11.433
13)	MA Dieldrin	5.732	6.703	12672008	119.1E6	10.264	11.562
14)	MA Endrin	5.990	6.923	11284386	88467713	10.337	10.988
15)	B Endosulfa...	6.264	7.129	11644865	98582742	10.408	11.420
16)	A 4,4'-DDD	6.116	7.035	9881473	89974738	10.209m	11.434
17)	MA 4,4'-DDT	6.356	7.338	9410091	89458491	10.061m	11.921
18)	B Endrin al...	6.434	7.253	9385391	77080073	10.819	11.790
19)	B Endosulfa...	6.646	7.478	10686184	83689020	9.764	10.488
20)	A Methoxychlor	6.907	7.790	28969500	211.8E6	54.606m	60.939m
21)	B Endrin ke...	7.138	7.953	13576620	100.1E6	11.033m	12.019

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060122\
 Data File : PD069930.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2022 09:36
 Operator : AR\AJ
 Sample : PB145093BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 11:40:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052922CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon May 30 09:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

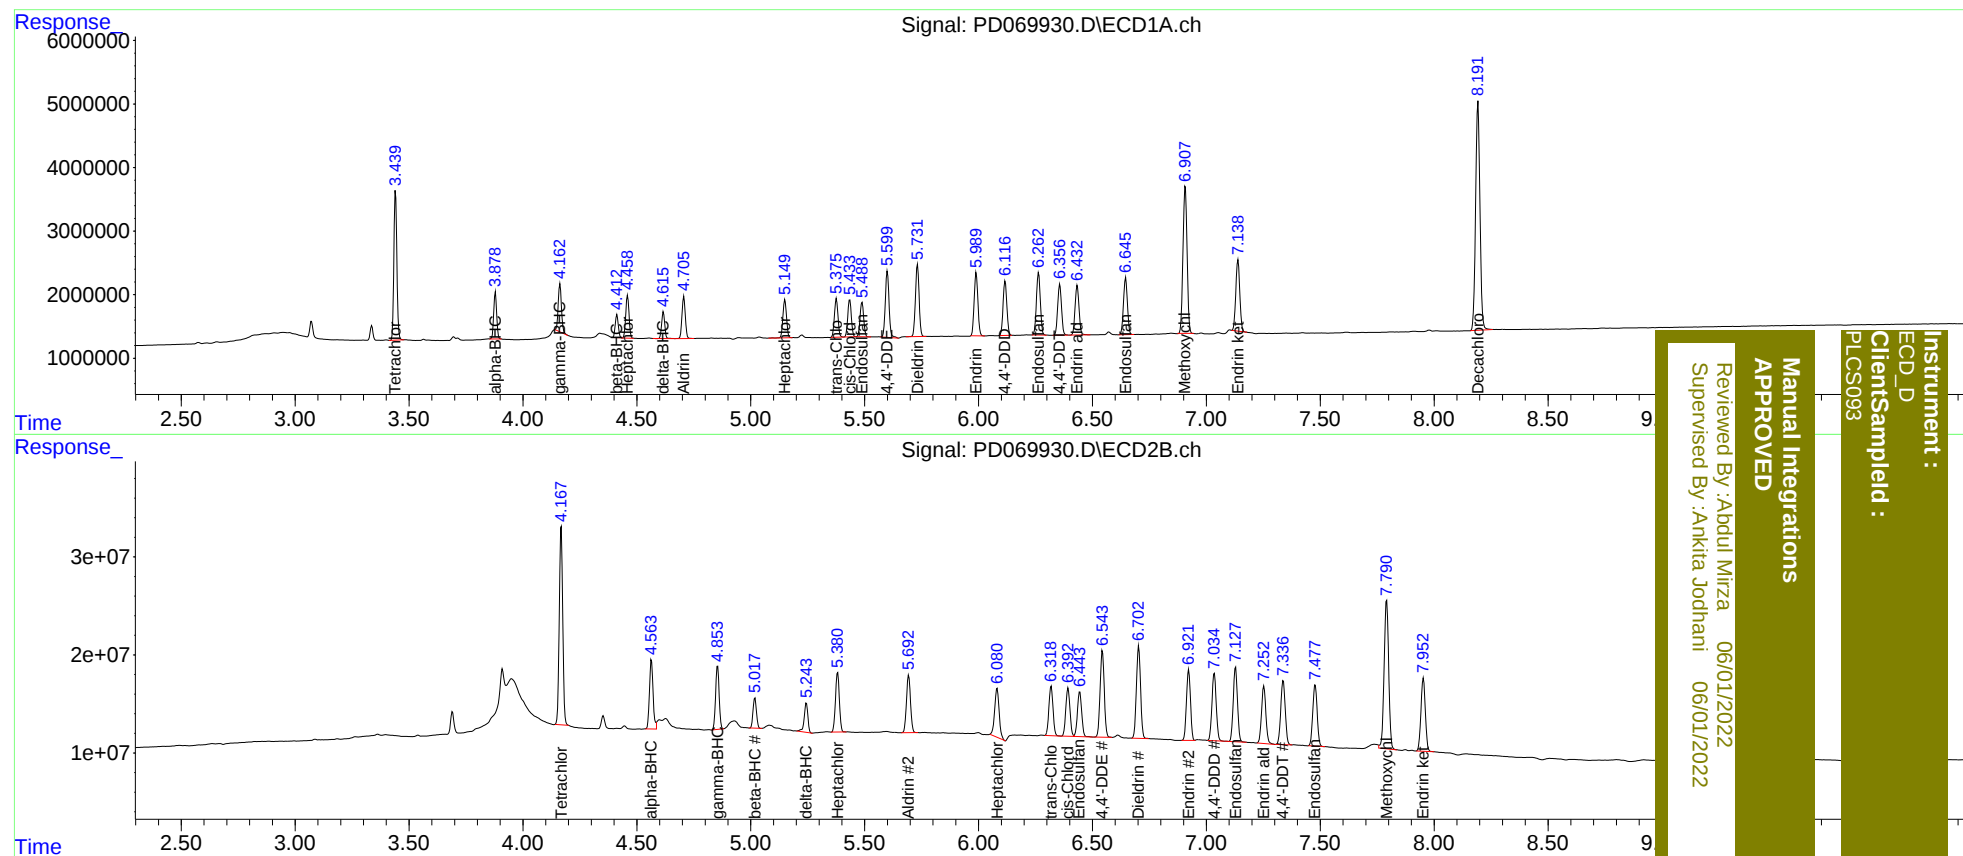

Reviewed By: Abdul Mirza 06/01/2022
 Supervised By: Ankita Jodhani 06/01/2022

Manual Integrations
 APPROVED

Instrument :
 ECD_D
 Client Sampled :
 PLCS093