

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060122\
 Data File : PD069931.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jun 2022 11:41
 Operator : AR\AJ
 Sample : N2815-10
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 X3A89

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/01/2022
 Supervised By : Ankita Jodhani 06/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 11:58:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052922CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon May 30 09:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.446	4.168	18421171	187.9E6	17.971	19.169
27)	SA Decachlor...	8.199	9.364	40363036	228.5E6	38.367	37.803
Target Compounds							
4)	MA Heptachlor	4.465	5.382	45017681	427.6E6	33.192	32.783
6)	B beta-BHC	4.419	5.019	38143369	362.7E6	57.738	60.693
9)	A Endosulfan I	5.495	6.446	56092110	462.2E6	48.621	45.583
10)	B trans-Chl...	5.382	6.320	72345237	581.4E6	57.069	51.563
11)	B cis-Chlor...	5.441	6.395	50562605	428.0E6	40.324	39.268
12)	B 4,4'-DDE	5.607	6.545	15242549	123.7E6	13.324	12.671
13)	MA Dieldrin	5.738	6.705	139.5E6	1057.4E6	112.951	102.617
14)	MA Endrin	5.997	6.923	159.0E6	741.6E6	145.624	92.115m#
15)	B Endosulfa...	6.270	7.131	109.0E6	779.3E6	97.464	90.267
16)	A 4,4'-DDD	6.122	7.036	51315714	383.7E6	53.014m	48.756
17)	MA 4,4'-DDT	6.362	7.337	53331495	698.6E6	57.021m	93.097 #
18)	B Endrin al...	6.440	7.254	20129228	155.8E6	23.203	23.838
21)	B Endrin ke...	7.146	7.954	66765622	437.1E6	54.259	52.482

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD060122\
Data File : PD069931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jun 2022 11:41
Operator : AR\AJ
Sample : N2815-10
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 11:58:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD052922CLP.M
Quant Title : GC Extractables
QLast Update : Mon May 30 09:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

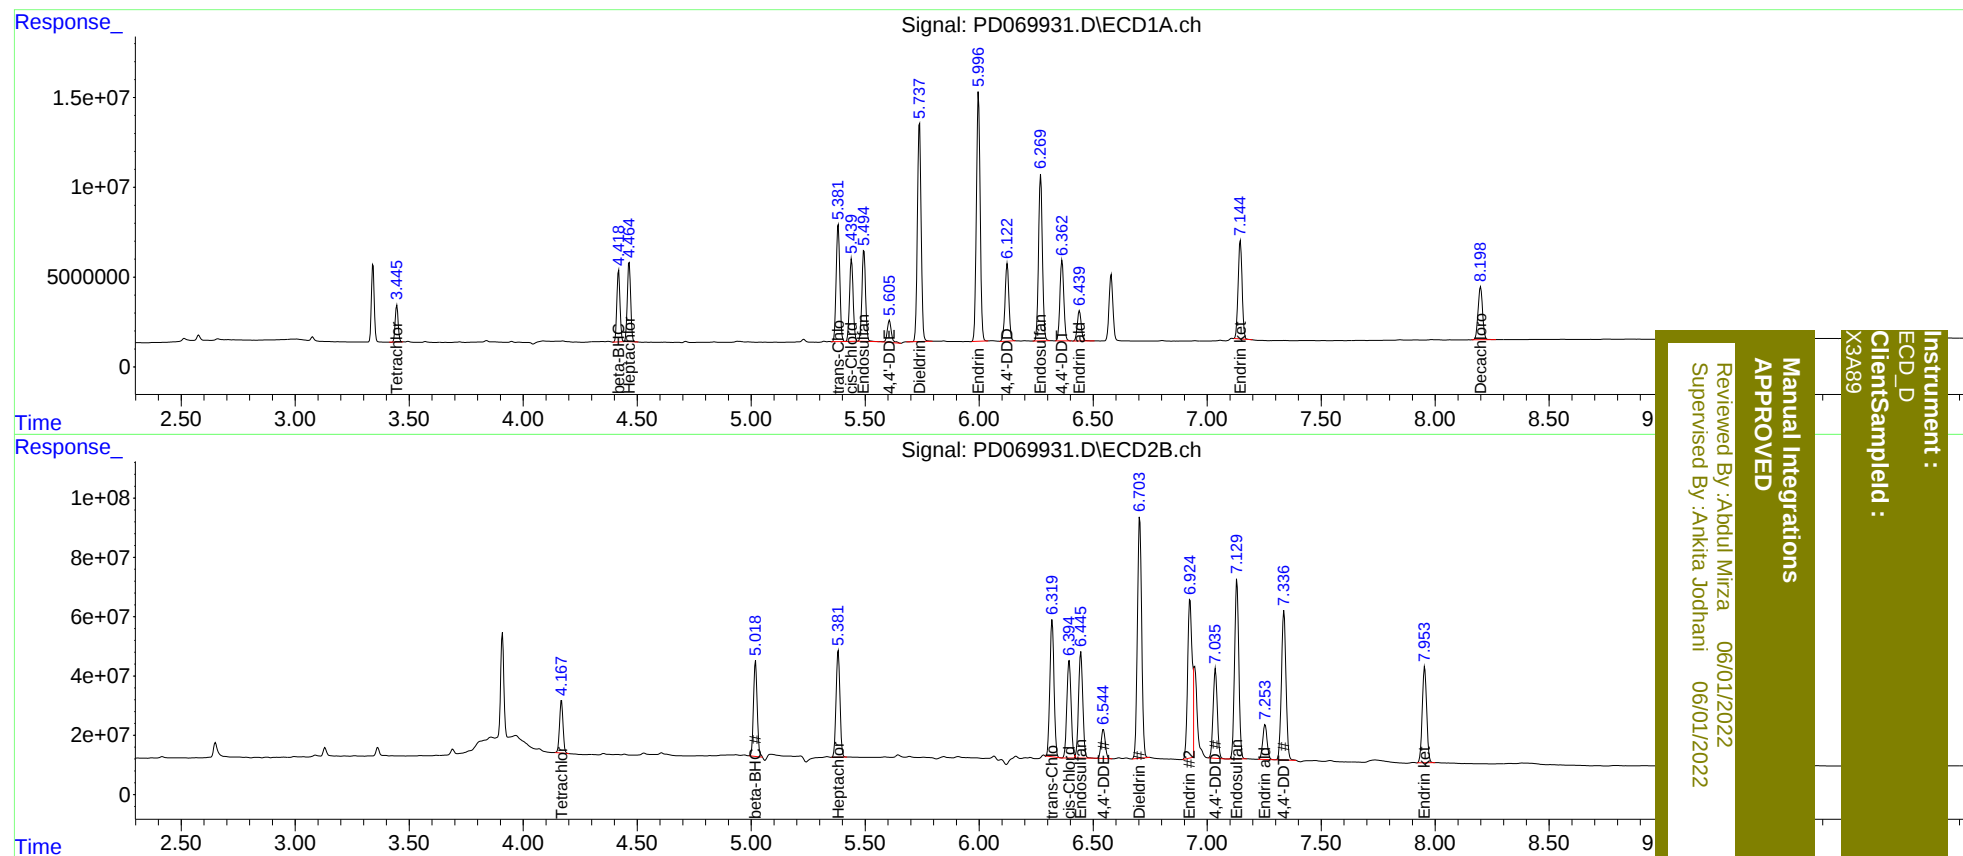

Reviewed By: Abdul Mirza 06/01/2022
Supervised By: Ankita Jodhani 06/01/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
X3A89