

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061021\
 Data File : PD063727.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2021 13:56
 Operator : AR\AJ
 Sample : PB136871BS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS871

Manual Integrations
 APPROVED

Ankita
 6/14/2021 2:38:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 04:01:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.442	3.971	25314355	249.1E6	18.442	17.697
27)	SA Decachlor...	8.198	9.026	58591054	482.0E6	36.063	32.853
Target Compounds							
2)	A alpha-BHC	3.878	4.358	9249519	108.1E6	4.530	4.890m
3)	MA gamma-BHC...	4.161	4.643	10031099	94841683	4.983	4.642
4)	MA Heptachlor	4.462	5.151	8306524	92901267	4.269	4.471
5)	MB Aldrin	4.710	5.455	8118968	97723374	4.322	4.748
6)	B beta-BHC	4.413	4.815	4430326	48493921	4.763	5.421
7)	B delta-BHC	4.617	5.030	8341967	136.6E6	4.274	6.190 #
8)	B Heptachlo...	5.153	5.842	7911069	109.2E6	4.497	5.489
9)	A Endosulfan I	5.492	6.198	7243015	83685431	4.405	4.686
10)	B trans-Chl...	5.380	6.075	8002441	90200736	4.378	4.526
11)	B cis-Chlor...	5.439	6.148	7861901	88573330	4.433	4.686
12)	B 4,4'-DDE	5.602	6.305	15570223	175.8E6	8.623	9.291
13)	MA Dieldrin	5.735	6.454	15906246	177.7E6	8.491	9.287
14)	MA Endrin	5.994	6.671	13435390	134.3E6	8.313	8.483
15)	B Endosulfa...	6.266	6.881	13468554	155.5E6	8.968	10.271
16)	A 4,4'-DDD	6.119	6.795	12844288	149.3E6	8.692	9.831
17)	MA 4,4'-DDT	6.360	7.093	11090479	123.5E6	7.305	8.038
18)	B Endrin al...	6.436	7.004	12810248	134.9E6	9.831	10.217m
19)	B Endosulfa...	6.649	7.228	12211880	145.0E6	8.504	9.307
20)	A Methoxychlor	6.906	7.551	35757641	317.4E6	43.331	43.985
21)	B Endrin ke...	7.141	7.698	17490867	151.1E6	9.916	9.804

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061021\
Data File : PD063727.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2021 13:56
Operator : AR\AJ
Sample : PB136871BS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 04:01:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

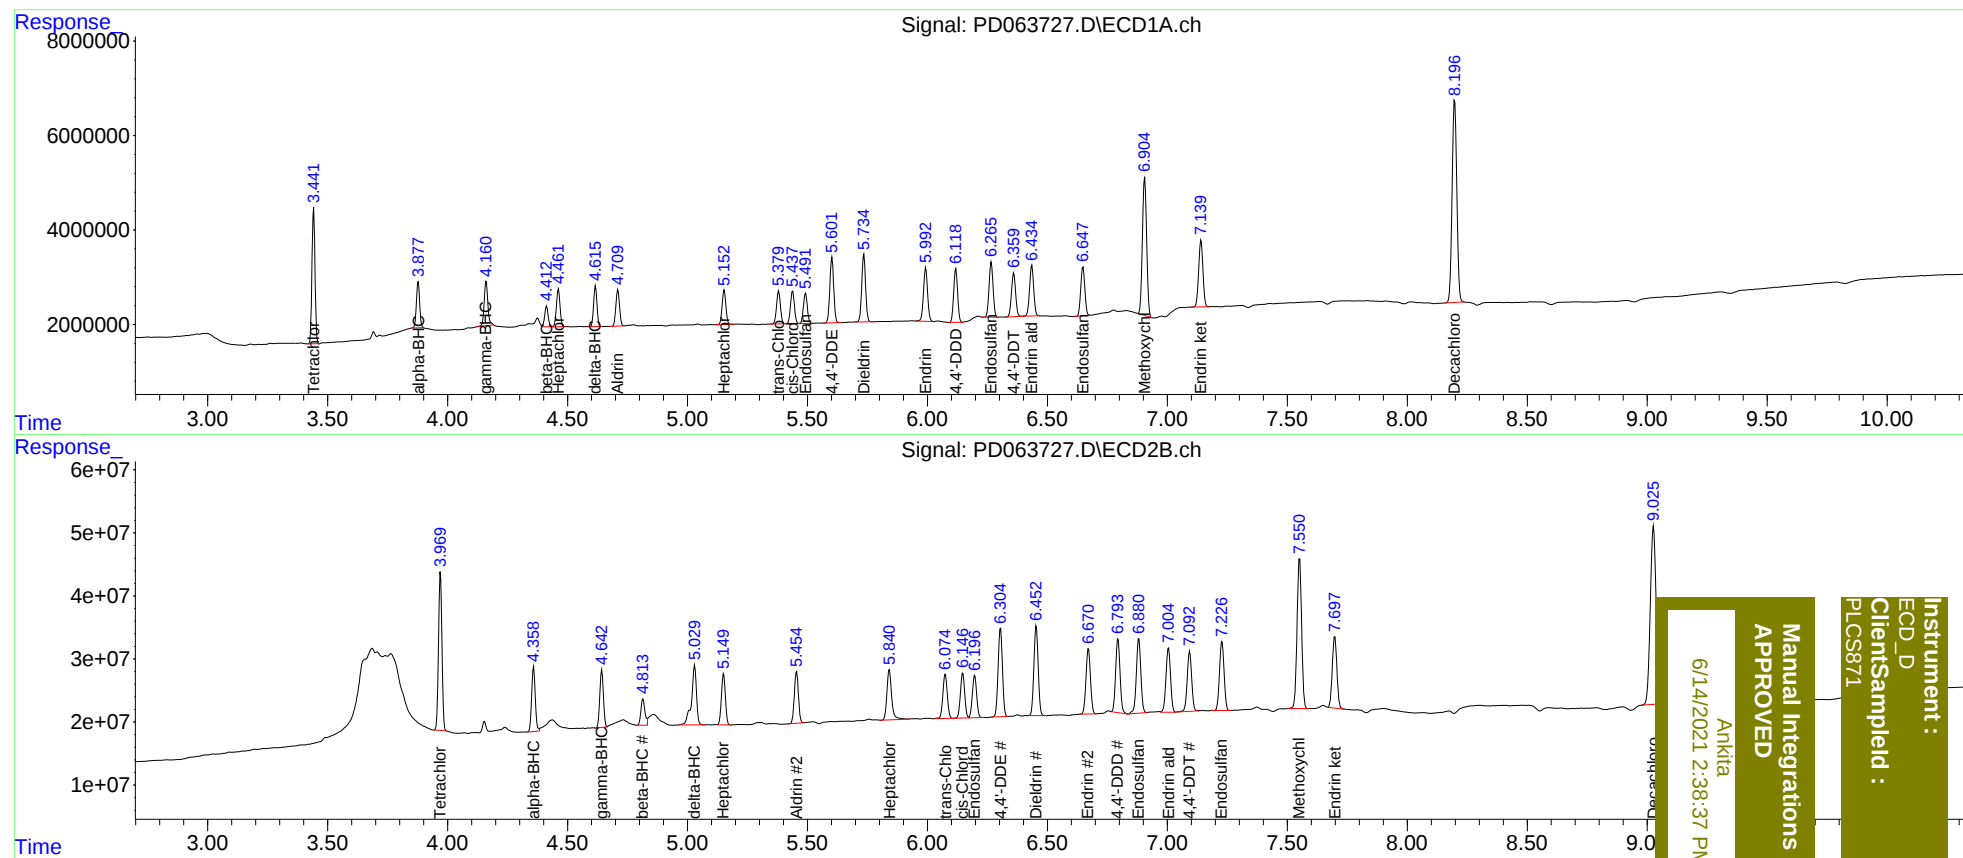

Manual Integrations
APPROVED

Ankita
6/14/2021 2:38:37 PM

Instrument :
ECD_D
ClientSample :
PLCS871