

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061021\
 Data File : PD063738.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2021 16:40
 Operator : AR\AJ
 Sample : M2608-03MS
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW119MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 04:46:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.970	24049845	238.2E6	17.521	16.921
27)	SA Decachlor...	8.196	9.025	54229597	482.7E6	33.378	32.897
Target Compounds							
2)	A alpha-BHC	3.875	4.358	101.5E6	939.7E6	49.689	42.521
3)	MA gamma-BHC...	4.158	4.643	95746812	847.6E6	47.558	41.488
4)	MA Heptachlor	4.459	5.150	83979043	751.5E6	43.157	36.166
5)	MB Aldrin	4.707	5.455	81951734	776.3E6	43.628	37.719
6)	B beta-BHC	4.410	4.813	39771297	334.3E6	42.755	37.370
7)	B delta-BHC	4.614	5.030	94563038	865.5E6	48.454	39.232
8)	B Heptachlo...	5.150	5.840	82165761	795.8E6	46.709	39.985
9)	A Endosulfan I	5.489	6.197	75531417	761.3E6	45.940	42.631
10)	B trans-Chl...	5.377	6.075	81166296	806.6E6	44.400	40.478
11)	B cis-Chlor...	5.436	6.147	79337503	784.4E6	44.732	41.499
12)	B 4,4'-DDE	5.600	6.304	158.6E6	1551.2E6	87.828	81.975
13)	MA Dieldrin	5.733	6.454	171.4E6	1666.3E6	91.520	87.086
14)	MA Endrin	5.990	6.671	149.6E6	1368.4E6	92.594	86.416
15)	B Endosulfa...	6.264	6.880	145.1E6	1382.1E6	96.620	91.305
16)	A 4,4'-DDD	6.116	6.794	140.5E6	1398.4E6	95.060	92.054
17)	MA 4,4'-DDT	6.357	7.092	136.4E6	1246.3E6	89.834	81.091
18)	B Endrin al...	6.432	7.004	123.7E6	1157.9E6	94.945	87.724
19)	B Endosulfa...	6.646	7.228	132.6E6	1358.6E6	92.365	87.179
20)	A Methoxychlor	6.904	7.551	357.9E6	2895.7E6	433.674	401.342
21)	B Endrin ke...	7.138	7.697	178.2E6	1348.1E6	101.037	87.480

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061021\
Data File : PD063738.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2021 16:40
Operator : AR\AJ
Sample : M2608-03MS
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 04:46:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

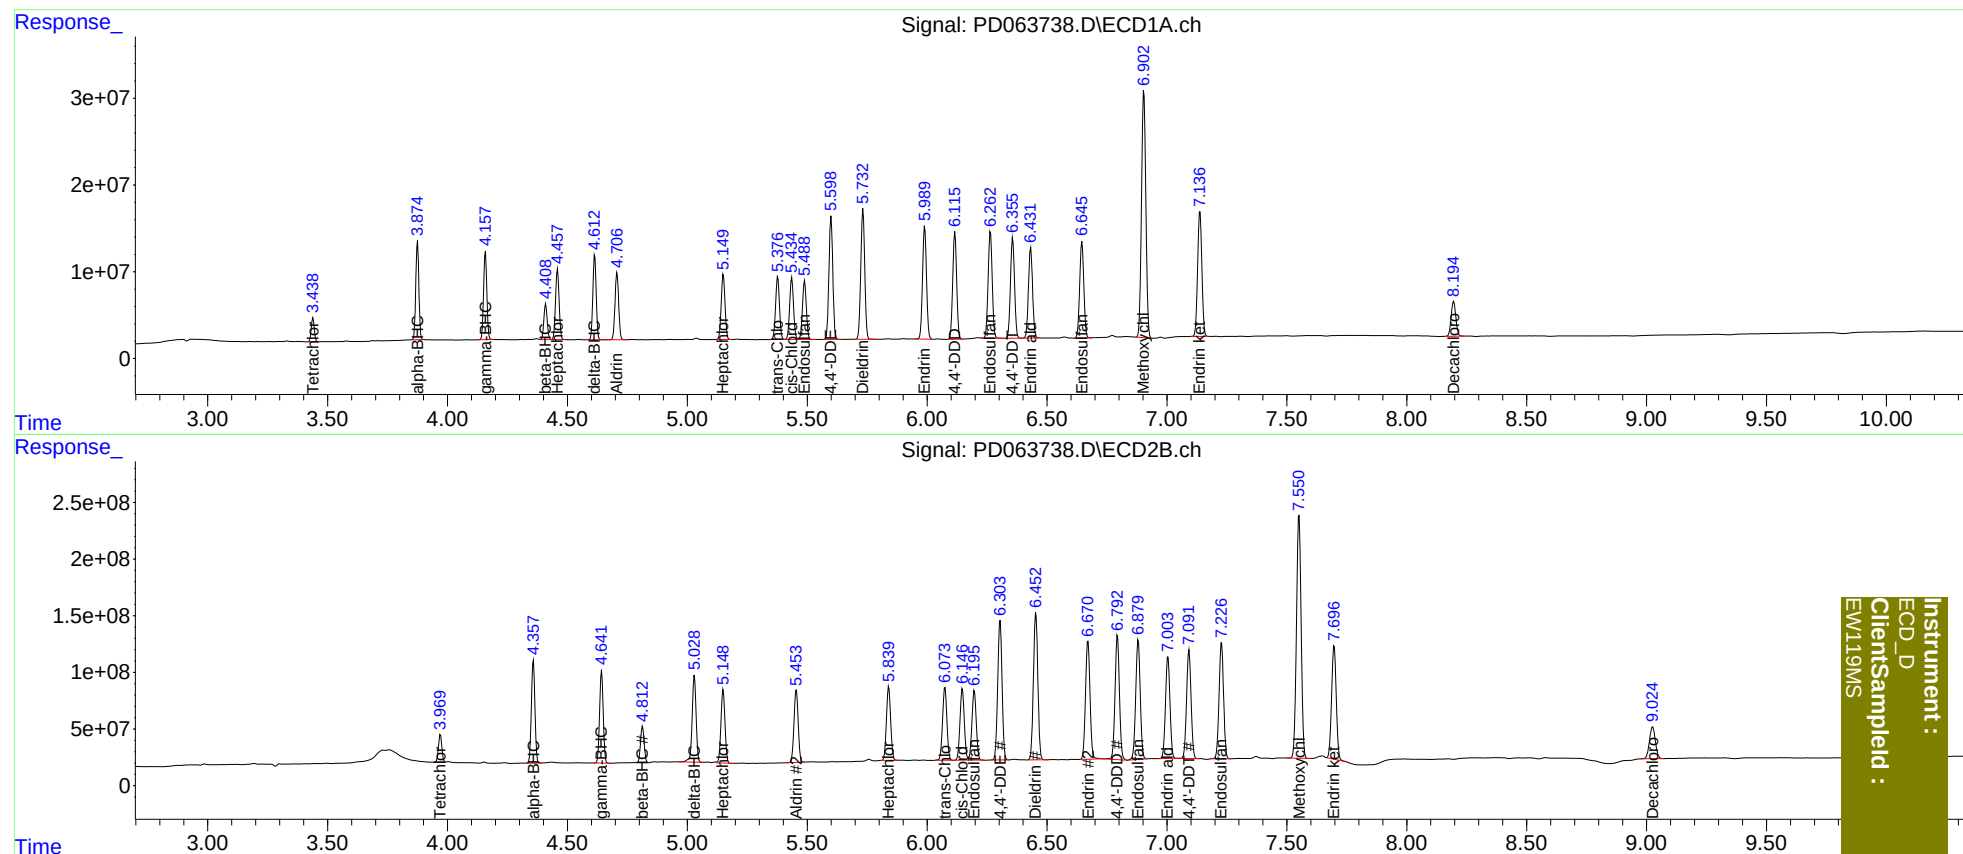

Instrument :
ECD_D
ClientSampled :
EW119MS