

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061021\
 Data File : PD063739.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2021 16:54
 Operator : AR\AJ
 Sample : M2608-04MSD
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW119MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 04:49:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.970	25041569	252.8E6	18.244	17.960
2)	SA Decachlor...	8.194	9.026	56709879	496.0E6	34.905	33.804
Target Compounds							
2)	A alpha-BHC	3.875	4.359	104.9E6	1033.5E6	51.358	46.765
3)	MA gamma-BHC...	4.158	4.643	98879922	961.2E6	49.114	47.047
4)	MA Heptachlor	4.459	5.150	85721255	863.4E6	44.052	41.550
5)	MB Aldrin	4.707	5.454	84416138	873.7E6	44.940	42.451
6)	B beta-BHC	4.409	4.813	40961927	388.5E6	44.035	43.425
7)	B delta-BHC	4.613	5.030	97325032	930.2E6	49.869	42.169
8)	B Heptachlo...	5.150	5.840	84453591	835.8E6	48.009	41.996
9)	A Endosulfan I	5.488	6.196	78137815	797.4E6	47.525	44.650
10)	B trans-Chl...	5.377	6.074	84220388	835.7E6	46.071	41.939
11)	B cis-Chlor...	5.435	6.147	82035665	820.7E6	46.254	43.422
12)	B 4,4'-DDE	5.599	6.304	167.0E6	1621.1E6	92.489	85.669
13)	MA Dieldrin	5.732	6.453	180.9E6	1733.3E6	96.581	90.587
14)	MA Endrin	5.989	6.671	156.2E6	1409.8E6	96.674	89.031
15)	B Endosulfa...	6.263	6.881	151.7E6	1438.2E6	100.992	95.016
16)	A 4,4'-DDD	6.116	6.794	148.6E6	1470.5E6	100.567	96.800
17)	MA 4,4'-DDT	6.356	7.093	141.2E6	1283.9E6	93.024	83.534
18)	B Endrin al...	6.432	7.004	128.5E6	1190.8E6	98.637	90.217
19)	B Endosulfa...	6.645	7.227	139.9E6	1416.1E6	97.414	90.869
20)	A Methoxychlor	6.903	7.551	367.1E6	2986.7E6	444.821	413.957
21)	B Endrin ke...	7.137	7.697	184.3E6	1425.4E6	104.486	92.501

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061021\
Data File : PD063739.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2021 16:54
Operator : AR\AJ
Sample : M2608-04MSD
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 04:49:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

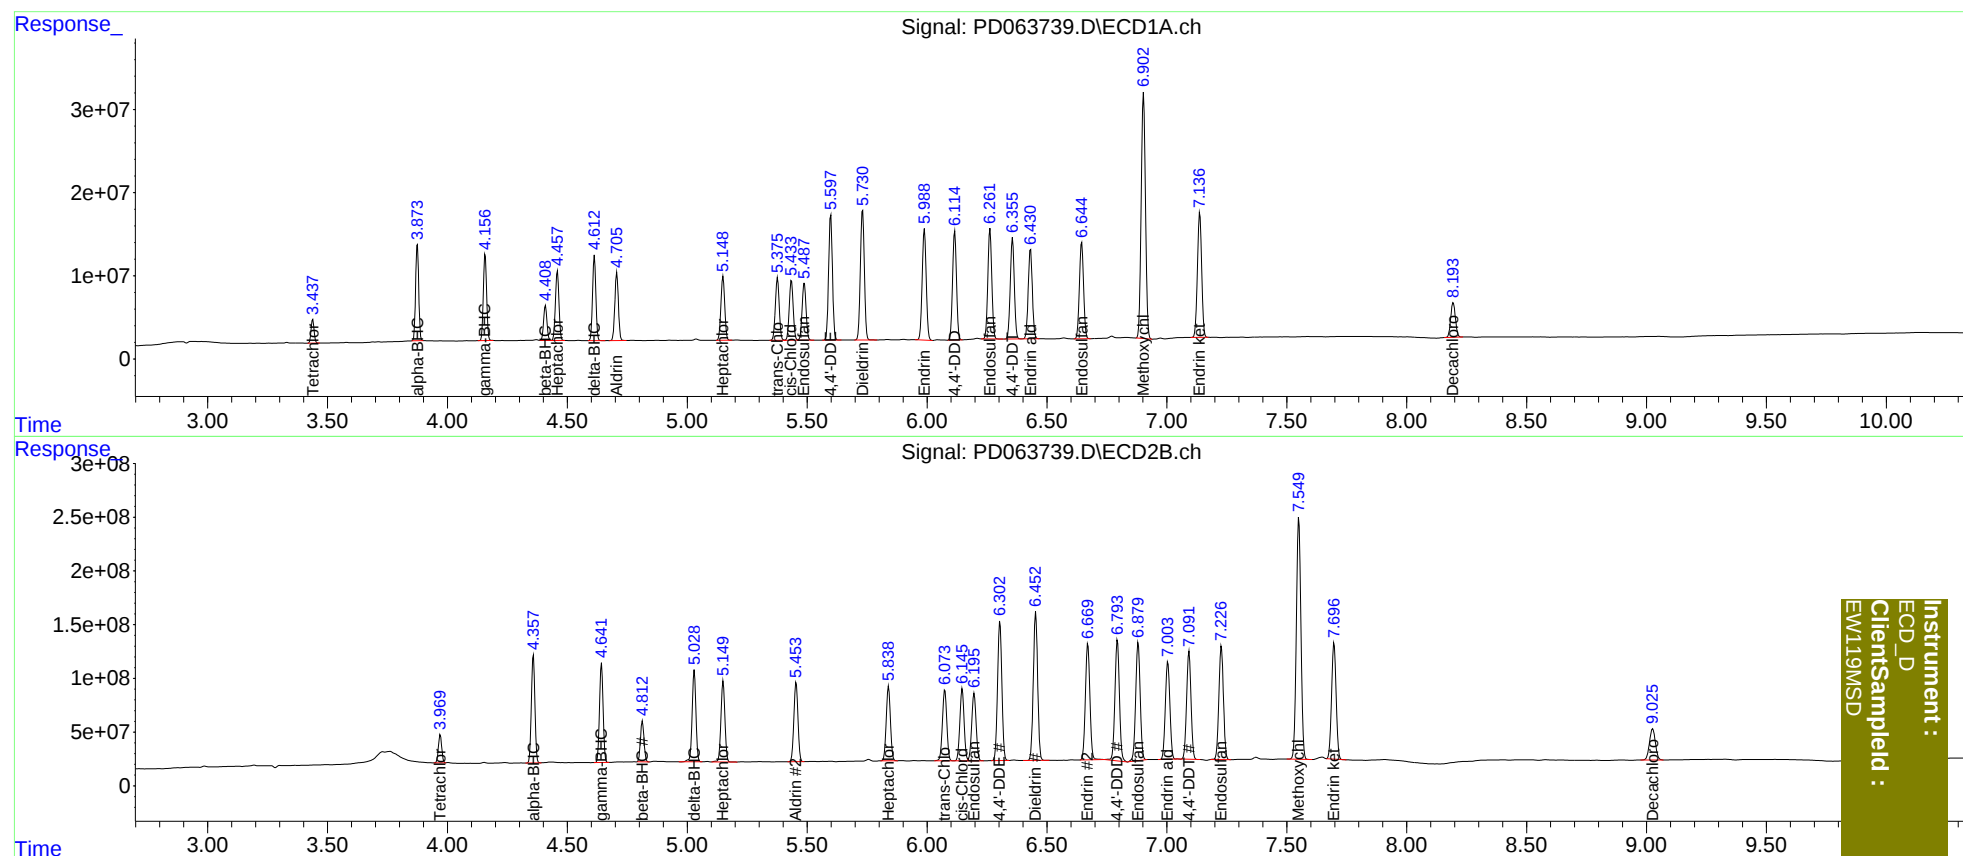

Instrument :
ECD_D
ClientSampled :
EW119MSD