

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061021\
 Data File : PD063743.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2021 17:49
 Operator : AR\AJ
 Sample : M2618-10
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BG5T5

Manual Integrations
 APPROVED

Ankita
 6/14/2021 2:38:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 04:05:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.970	23219211	217.2E6	16.916	15.426
27)	SA Decachlor...	8.194	9.025	39627364	327.0E6	24.391	22.289
Target Compounds							
8)	B Heptachlo...	5.157	5.846	594562	36112338	0.338m	1.815m#
10)	B trans-Chl...	5.375	6.061	1036956	39483695	0.567m	1.981m#
11)	B cis-Chlor...	5.424	6.146	3458400	10595498	1.950	0.561 #
16)	A 4,4'-DDD	6.116	6.793	911544	16816951	0.617m	1.107m#
17)	MA 4,4'-DDT	6.353	7.090	947911	12700769	0.624	0.826m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061021\
Data File : PD063743.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2021 17:49
Operator : AR\AJ
Sample : M2618-10
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 04:05:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

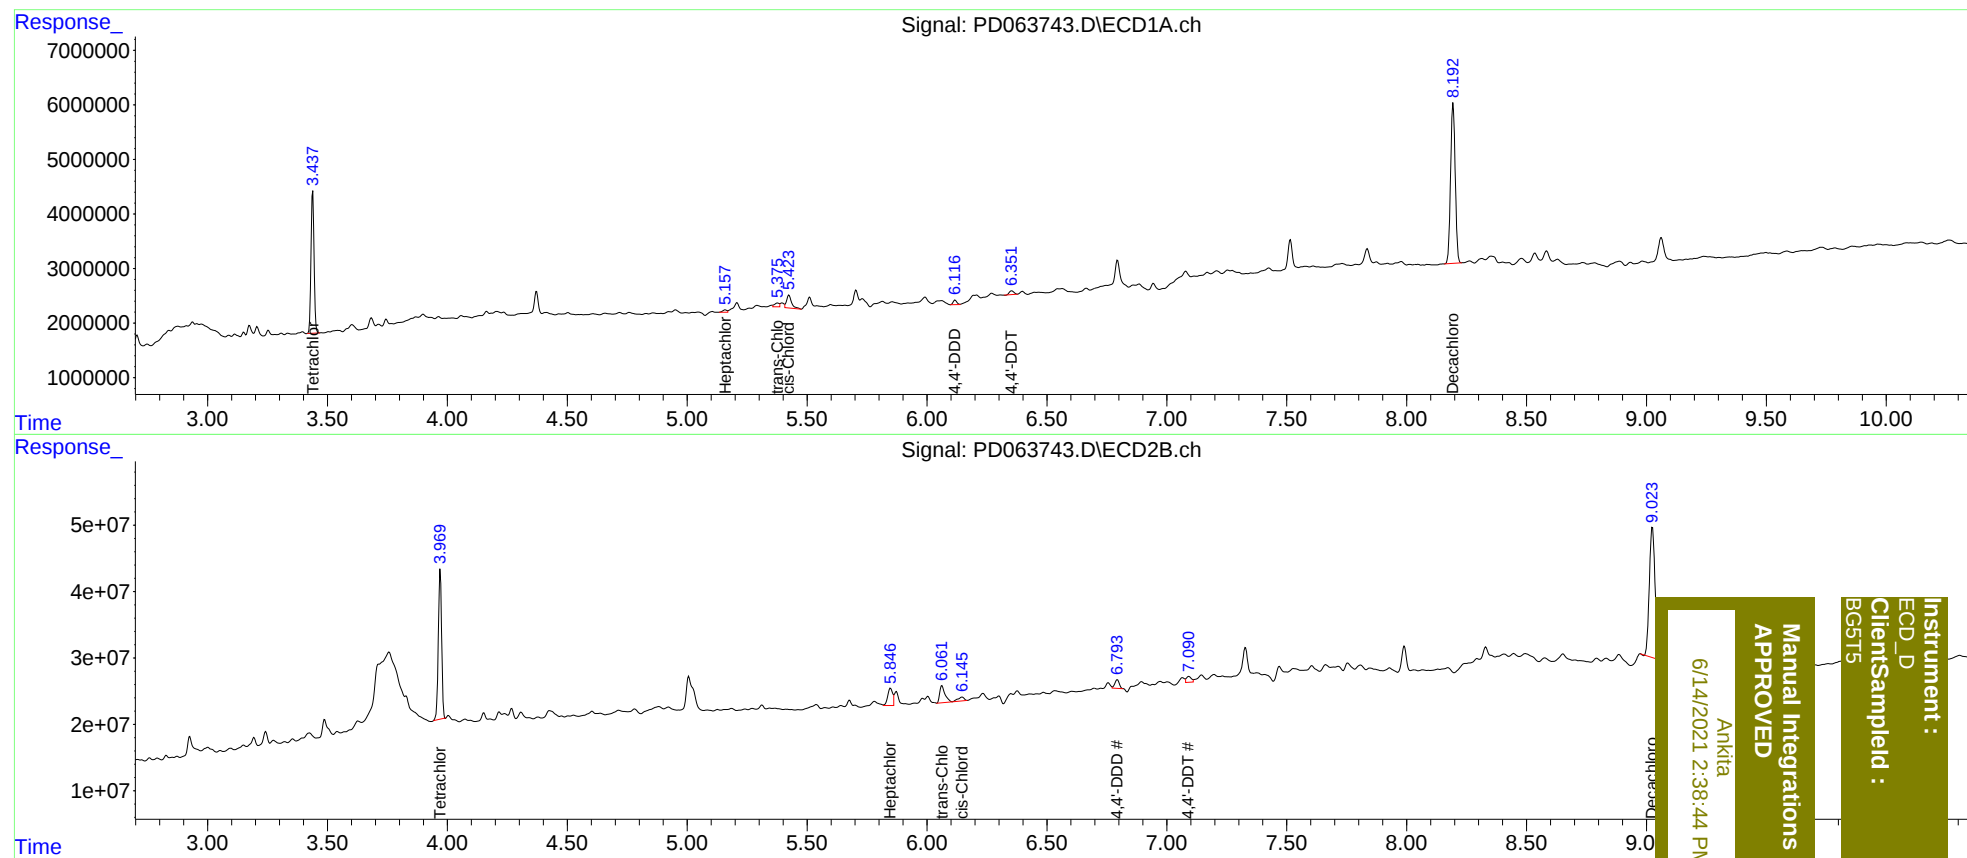

Manual Integrations
APPROVED

Ankita
6/14/2021 2:38:44 PM

Instrument :
ECD_D
ClientSampled :
BG5T5