

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061021\
 Data File : PD063723.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2021 12:59
 Operator : AR\AJ
 Sample : M2618-13MS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BG5S8MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 04:26:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.971	27740071	283.6E6	20.210	20.145
27)	SA Decachlor...	8.195	9.025	62457259	526.2E6	38.442	35.860
Target Compounds							
2)	A alpha-BHC	3.875	4.359	113.6E6	1120.0E6	55.653	50.678
3)	MA gamma-BHC...	4.158	4.643	108.1E6	1037.5E6	53.718	50.781
4)	MA Heptachlor	4.459	5.150	99254497	962.4E6	51.007	46.317
5)	MB Aldrin	4.706	5.454	96184207	974.4E6	51.205	47.344
6)	B beta-BHC	4.409	4.814	43356847	407.3E6	46.609	45.534
7)	B delta-BHC	4.613	5.030	106.8E6	1013.1E6	54.713	45.926
8)	B Heptachlo...	5.150	5.840	93403080	915.8E6	53.097	46.017
9)	A Endosulfan I	5.488	6.197	84029701	849.0E6	51.109	47.538
10)	B trans-Chl...	5.377	6.075	92441068	919.3E6	50.568	46.133
11)	B cis-Chlor...	5.435	6.147	90250376	886.4E6	50.885	46.898
12)	B 4,4'-DDE	5.599	6.304	190.2E6	1812.5E6	105.331	95.780
13)	MA Dieldrin	5.732	6.453	196.2E6	1858.7E6	104.719	97.142
14)	MA Endrin	5.990	6.671	170.8E6	1548.1E6	105.704	97.764
15)	B Endosulfa...	6.263	6.880	160.8E6	1525.1E6	107.085	100.752
16)	A 4,4'-DDD	6.116	6.794	161.3E6	1537.4E6	109.184	101.203
17)	MA 4,4'-DDT	6.357	7.092	156.4E6	1419.2E6	102.992	92.337
18)	B Endrin al...	6.432	7.004	135.3E6	1270.0E6	103.843	96.215
19)	B Endosulfa...	6.646	7.227	147.6E6	1508.2E6	102.759	96.782
20)	A Methoxychlor	6.903	7.551	396.9E6	3243.1E6	481.008	449.494
21)	B Endrin ke...	7.137	7.697	195.2E6	1510.3E6	110.687	98.012

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061021\
Data File : PD063723.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2021 12:59
Operator : AR\AJ
Sample : M2618-13MS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 04:26:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

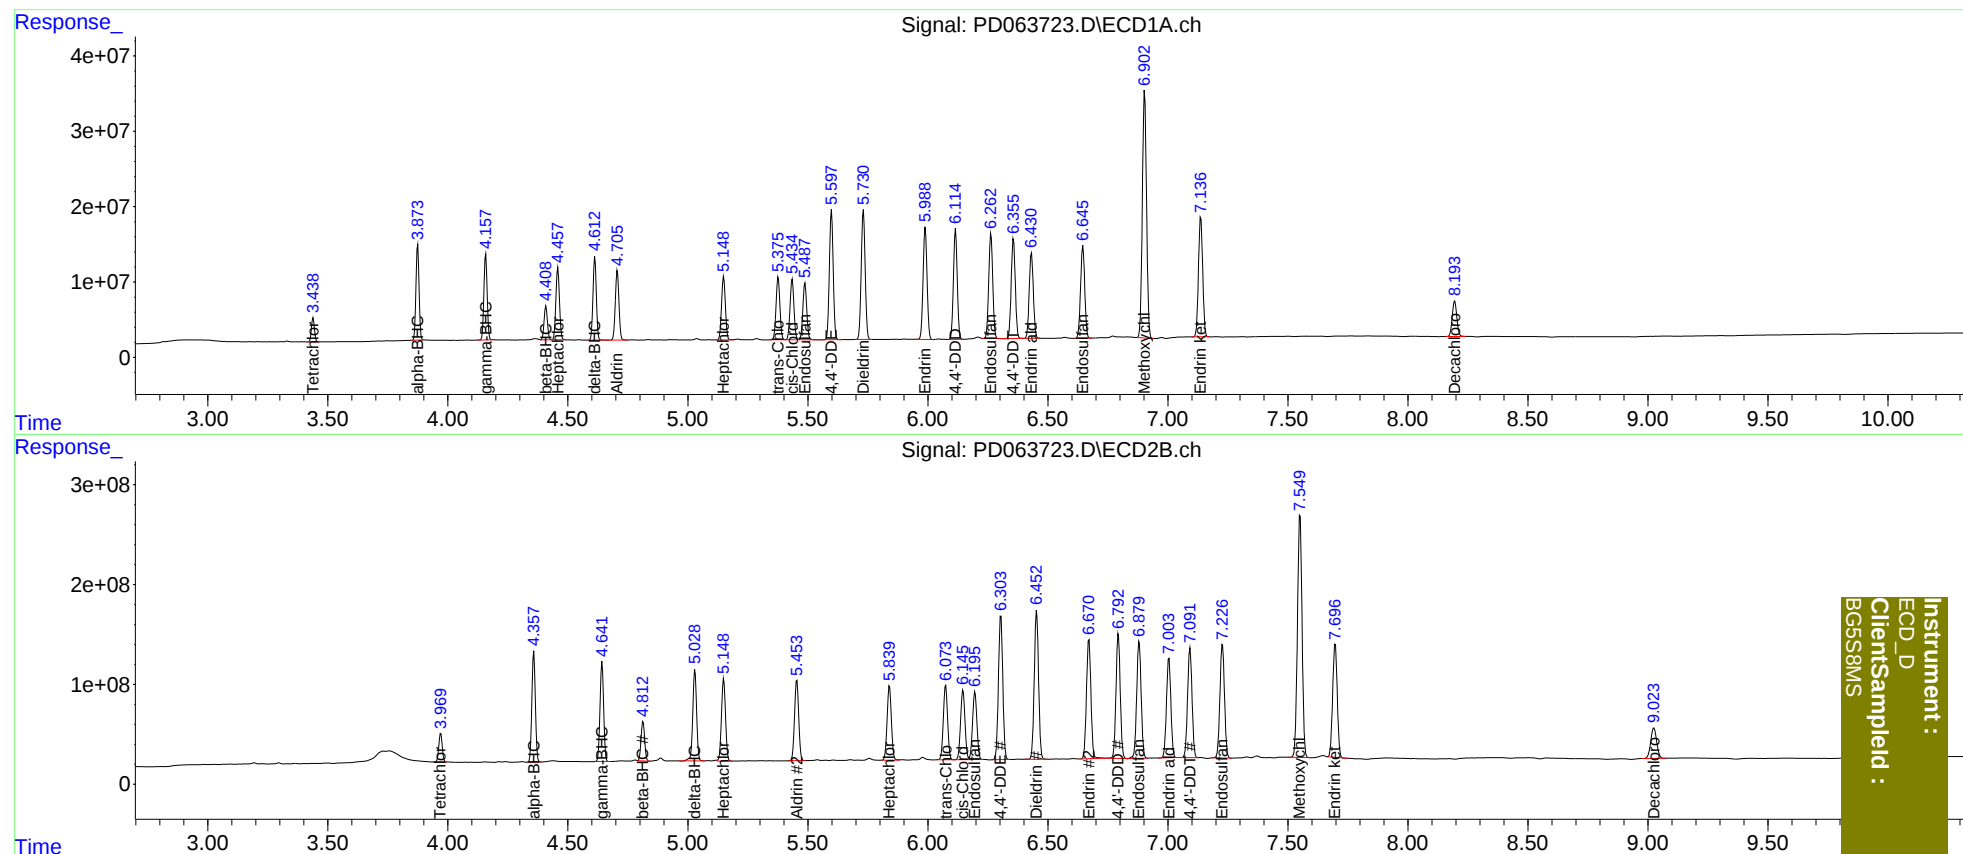

Instrument :
ECD_D
Client Sampled :
BG5S8MS