

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061021\
 Data File : PD063724.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2021 13:13
 Operator : AR\AJ
 Sample : M2618-14MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BG5S8MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 04:26:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 03 06:08:10 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	3.970	24454915	247.8E6	17.816	17.605
27)	SA Decachlor...	8.194	9.024	55185990	435.6E6	33.967	29.687
Target Compounds							
2)	A alpha-BHC	3.875	4.358	100.9E6	989.0E6	49.415	44.752
3)	MA gamma-BHC...	4.158	4.642	96832356	920.5E6	48.097	45.057
4)	MA Heptachlor	4.458	5.150	90694942	871.5E6	46.608	41.943
5)	MB Aldrin	4.706	5.454	86948062	878.4E6	46.288	42.683
6)	B beta-BHC	4.409	4.813	39204568	361.2E6	42.145	40.375
7)	B delta-BHC	4.612	5.029	94741153	913.9E6	48.545	41.426
8)	B Heptachlo...	5.149	5.840	83413630	817.5E6	47.418	41.075
9)	A Endosulfan I	5.488	6.196	75079371	754.7E6	45.665	42.258
10)	B trans-Chl...	5.376	6.074	82901251	810.5E6	45.349	40.673
11)	B cis-Chlor...	5.434	6.146	81072536	787.4E6	45.711	41.661
12)	B 4,4'-DDE	5.598	6.303	170.9E6	1602.3E6	94.637	84.675
13)	MA Dieldrin	5.731	6.453	175.4E6	1648.5E6	93.617	86.155
14)	MA Endrin	5.989	6.671	153.1E6	1360.1E6	94.726	85.894
15)	B Endosulfa...	6.263	6.880	143.4E6	1350.1E6	95.461	89.195
16)	A 4,4'-DDD	6.115	6.793	143.8E6	1360.7E6	97.342	89.570
17)	MA 4,4'-DDT	6.356	7.092	140.1E6	1250.4E6	92.276	81.356
18)	B Endrin al...	6.431	7.004	121.4E6	1115.1E6	93.129	84.484
19)	B Endosulfa...	6.645	7.227	131.1E6	1328.1E6	91.314	85.226
20)	A Methoxychlor	6.903	7.550	360.2E6	2866.1E6	436.439	397.241
21)	B Endrin ke...	7.137	7.697	174.1E6	1324.5E6	98.685	85.953

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061021\
Data File : PD063724.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2021 13:13
Operator : AR\AJ
Sample : M2618-14MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 04:26:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060321CLP.M
Quant Title : GC Extractables
QLast Update : Thu Jun 03 06:08:10 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

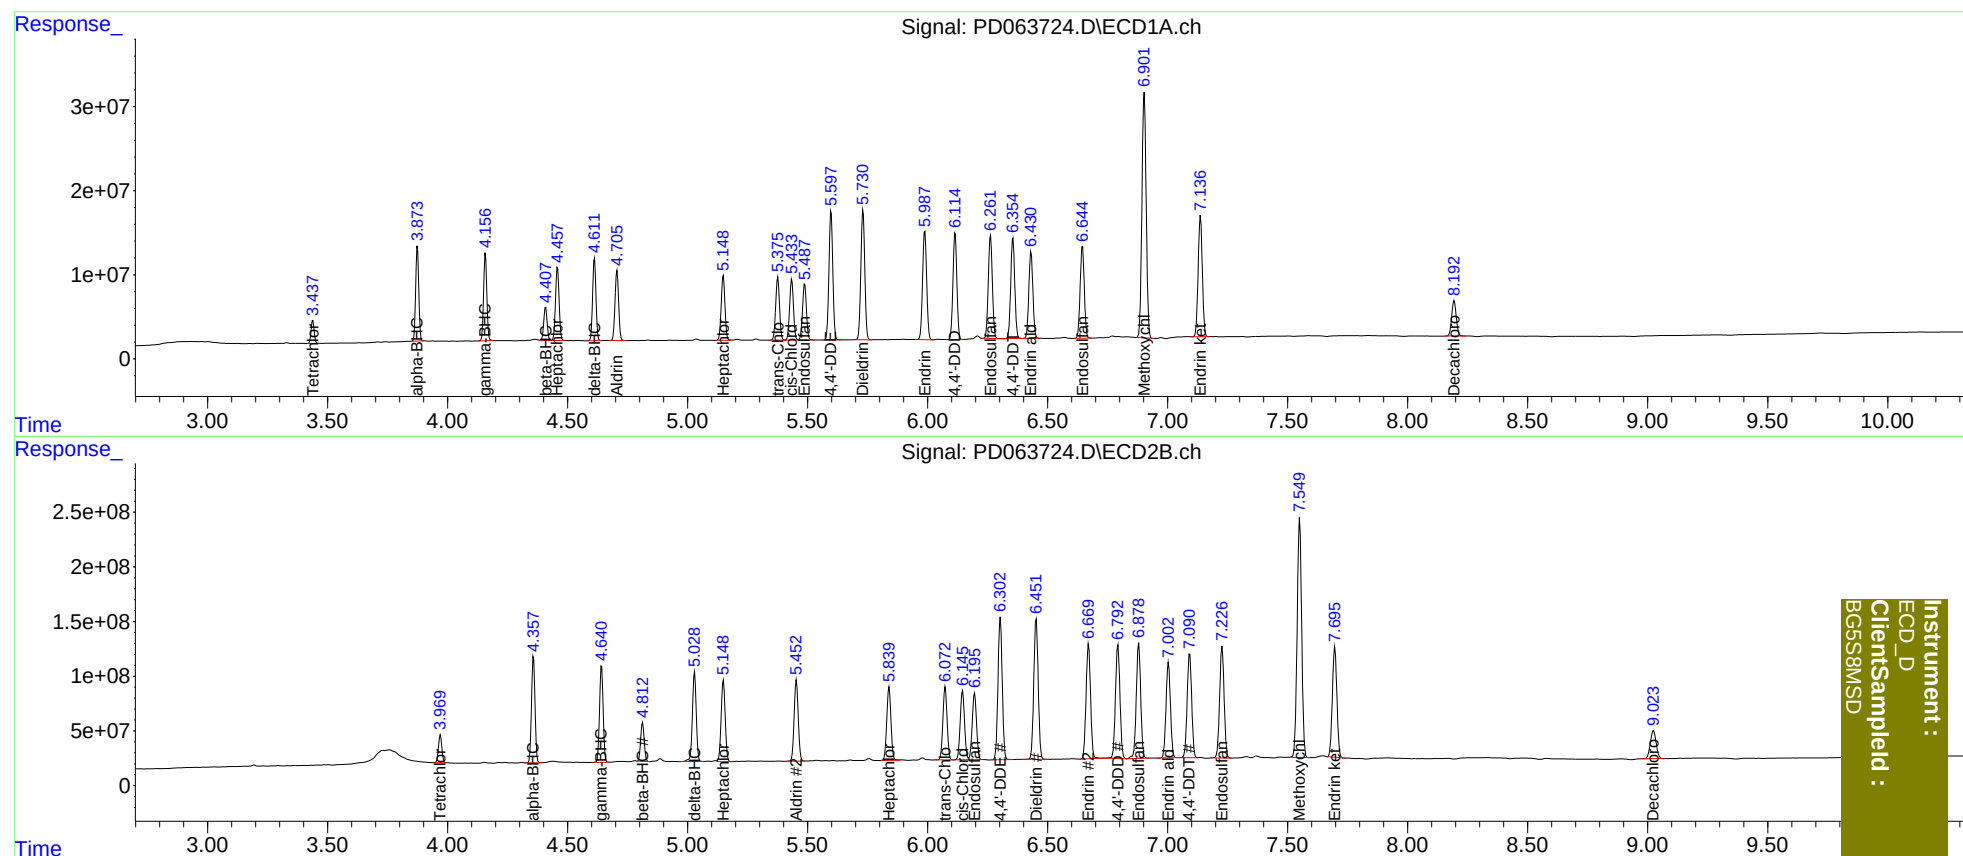

Instrument :
ECD_D
ClientSampled :
BG5S8MSD