

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061024\
 Data File : PD083587.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2024 16:39
 Operator : AR\AJ
 Sample : P2648-18DL 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BHC50DL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/12/2024
 Supervised By : mohammad ahmed 06/13/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 22:11:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.773	1676331	13690994	1.284m	2.512 #
27)	SA Decachlor...	9.107	7.897	13979901	62073818	7.189m	10.223m#
Target Compounds							
9)	A Endosulfan I	6.137	5.116	21825492	111.3E6	11.161m	16.835m#
10)	B trans-Chl...	5.964	4.967	8426300	22419196	4.138m	3.087m#
11)	B cis-Chlor...	6.056	5.031	18110939	29253185	8.697	3.973m#
13)	MA Dieldrin	6.380	5.351	207.5E6	785.5E6	100.349m	107.825m
14)	MA Endrin	6.636	5.627	8195040	9657203	4.851m	1.493m#
16)	A 4,4'-DDD	6.731	5.776	13502410	25827872	9.215m	4.581m#
17)	MA 4,4'-DDT	7.060	6.021	7846776	45322156	5.209m	8.007m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061024\
Data File : PD083587.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2024 16:39
Operator : AR\AJ
Sample : P2648-18DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 22:11:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

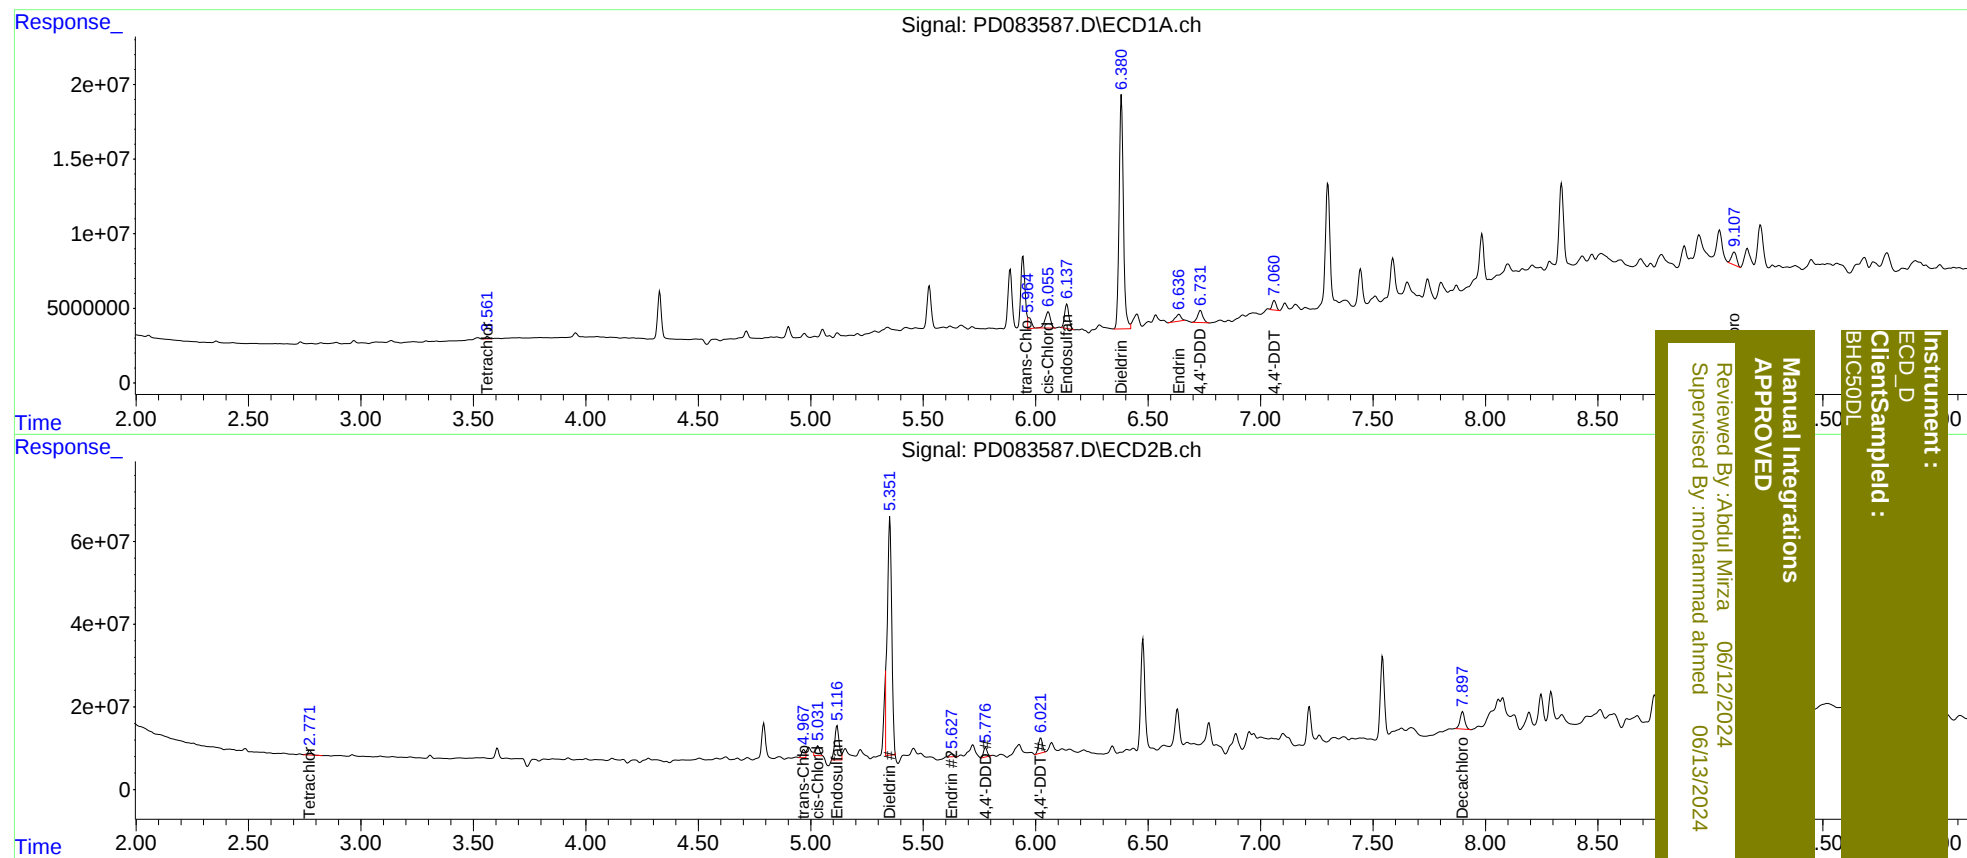

Manual Integrations
APPROVED
Reviewed By: Abdul Miza 06/12/2024
Supervised By: mohammad ahmed 06/13/2024

Instrument :
ECD_D
Client Sampled :
BHC50DL