

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061024\
 Data File : PD083593.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2024 21:05
 Operator : AR\AJ
 Sample : P2659-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BHC24

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/11/2024
 Supervised By : Ankita Jodhani 06/11/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 22:14:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.773	10565690	83858940	8.094m	15.384 #
27)	SA Decachlor...	9.104	7.897	94874654	287.7E6	48.791m	47.383m
Target Compounds							
4)	MA Heptachlor	4.971	3.920	17292327	39967807	7.118m	5.105m#
9)	A Endosulfan I	6.138	5.116	115.2E6	428.1E6	58.896m	64.757m
10)	B trans-Chl...	5.965	4.968	25677260	46562222	12.611m	6.411m#
11)	B cis-Chlor...	6.056	5.031	79307768	79349027	38.084	10.778m#
12)	B 4,4'-DDE	6.226	5.221	14506307	116.3E6	6.994	16.365m#
13)	MA Dieldrin	6.382	5.351	833.3E6	2842.8E6	403.033	390.225m
14)	MA Endrin	6.636	5.626	46115852	49724353	27.299m	7.688m#
15)	B Endosulfa...	6.821	5.925	10985965	86179898	6.108m	13.581m#
16)	A 4,4'-DDD	6.731	5.776	78103680	114.7E6	53.301m	20.345m#
17)	MA 4,4'-DDT	7.062	6.021	58958077	225.5E6	39.137	39.831m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061024\
Data File : PD083593.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2024 21:05
Operator : AR\AJ
Sample : P2659-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 22:14:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

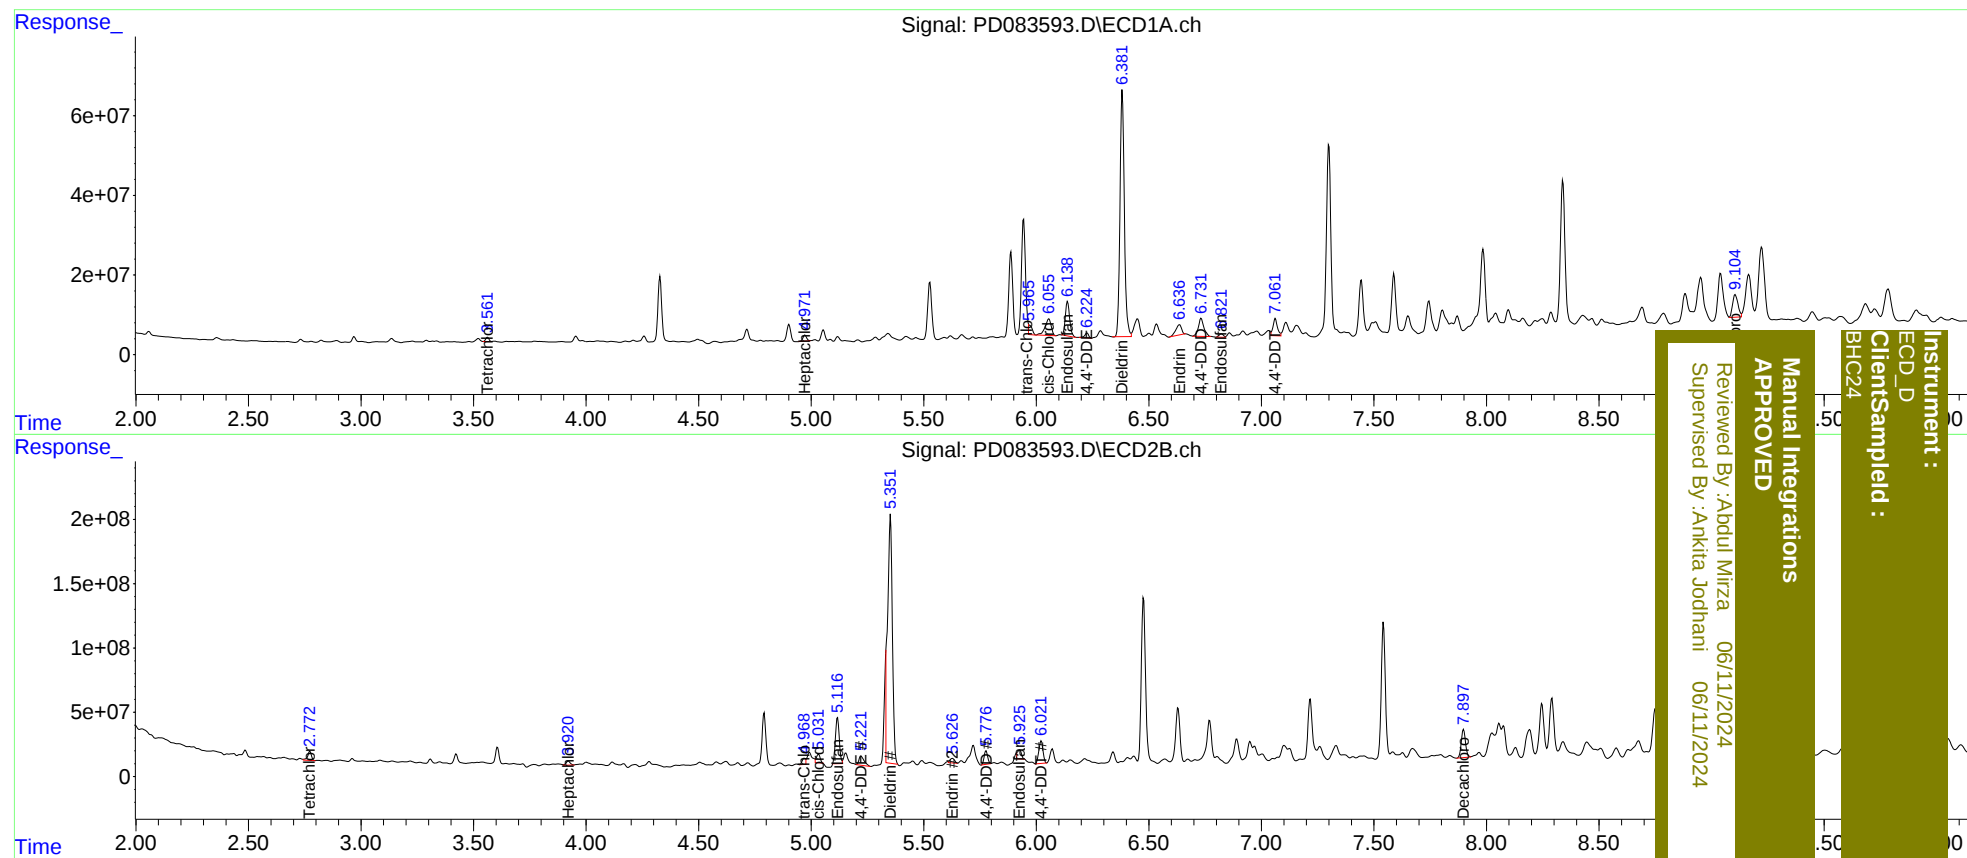

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/11/2024
Supervised By: Ankita Jodhani 06/11/2024

Instrument :
ECD_D
ClientSampled :
BHC24