

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061024\
 Data File : PD083624.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jun 2024 09:55
 Operator : AR\AJ
 Sample : P2659-03DL 2X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BHC26DL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/18/2024
 Supervised By :Ankita Jodhani 06/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 12 15:51:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.561	2.773	8029592	47740897	6.151m	8.758 #
27)	SA Decachlor...	9.101	7.896	36648013	142.8E6	18.847m	23.516m
Target Compounds							
4)	MA Heptachlor	4.970	3.920	8614934	13651853	3.546m	1.744m#
9)	A Endosulfan I	6.137	5.115	50746530	190.9E6	25.950m	28.885m
10)	B trans-Chl...	5.964	4.967	8612648	24490271	4.230m	3.372m
11)	B cis-Chlor...	6.053	5.030	26460900	19929800	12.707m	2.707m#
13)	MA Dieldrin	6.380	5.350	296.7E6	1106.3E6	143.483	151.854m
14)	MA Endrin	6.633	5.623	24892731	20400133	14.736m	3.154m#
16)	A 4,4'-DDD	6.729	5.775	30953685	60730492	21.124m	10.773m#
17)	MA 4,4'-DDT	7.061	6.020	12904451	55520505	8.566m	9.808m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061024\
Data File : PD083624.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jun 2024 09:55
Operator : AR\AJ
Sample : P2659-03DL 2X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 12 15:51:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

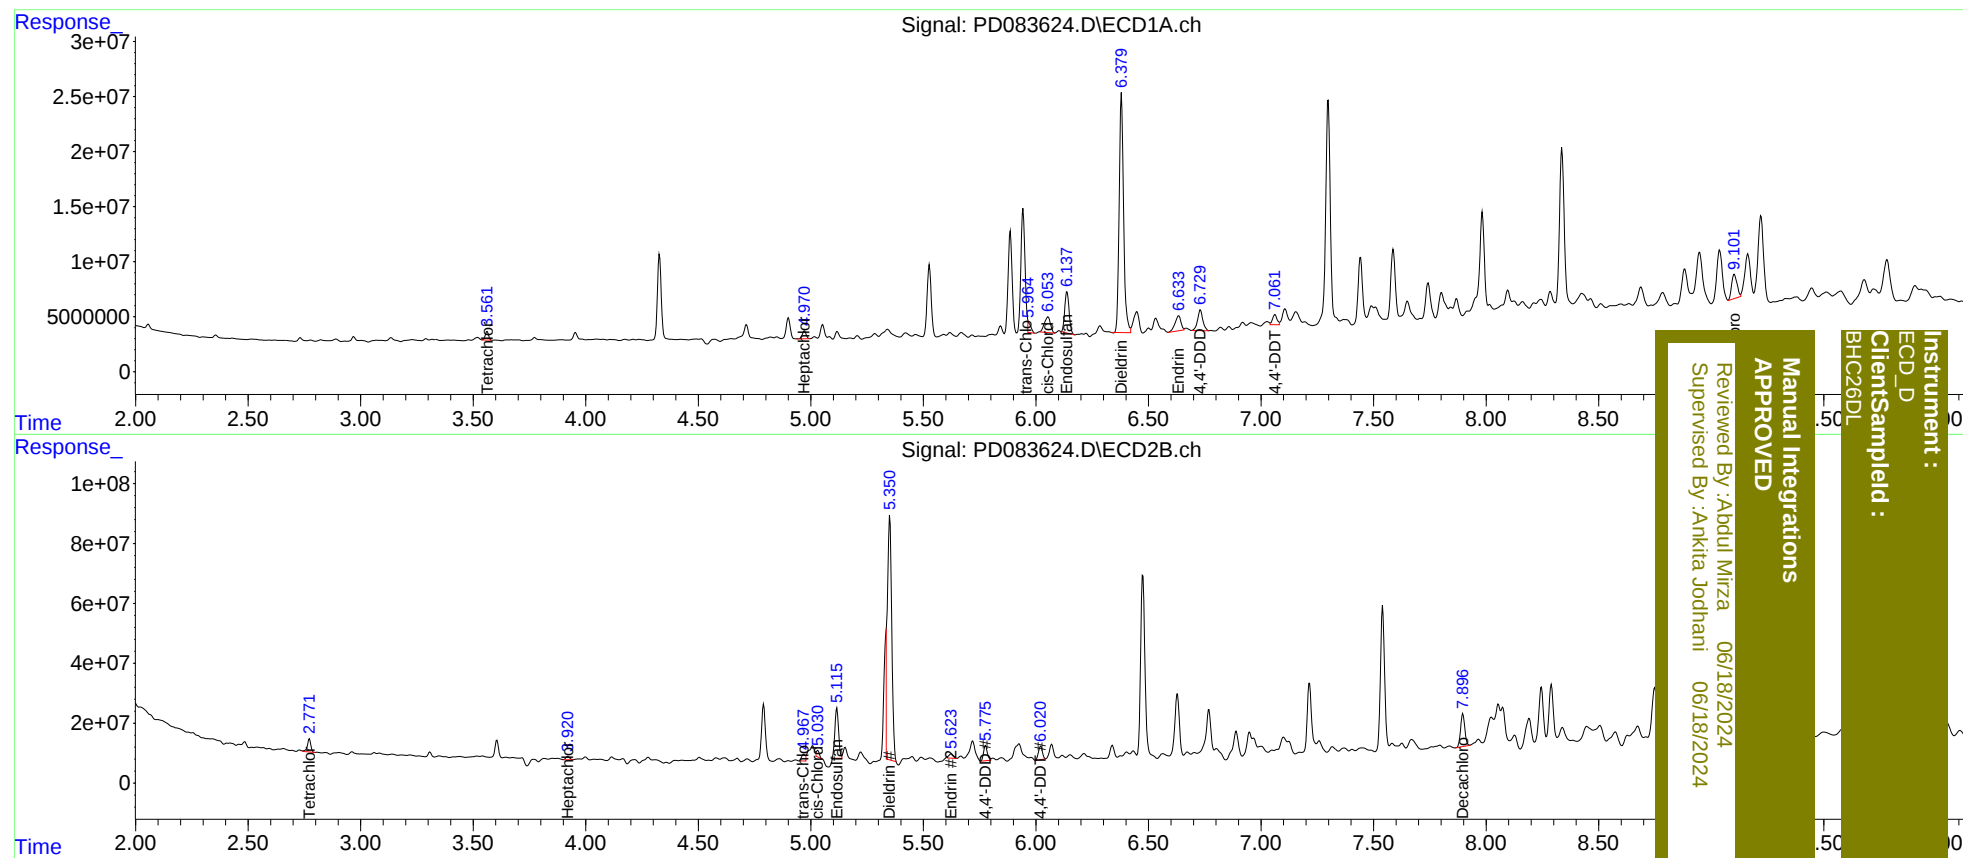

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/18/2024
Supervised By: Ankita Jodhani 06/18/2024

Instrument :
ECD_D
Client Sampled :
BHC26DL