

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061024\
 Data File : PD083586.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jun 2024 16:13
 Operator : AR\AJ
 Sample : P2648-09DL2 40X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 BHBZ8DL2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/12/2024
 Supervised By : mohammad ahmed 06/13/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 22:11:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 07 04:03:14 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
10) B	trans-Chl...	5.974	4.968	6226689	18330804	3.058m 2.524m
11) B	cis-Chlor...	6.057	5.031	7090706	15818397	3.405 2.149m#
12) B	4,4'-DDE	6.226	5.219	20285611	84287286	9.780m 11.860m
13) MA	Dieldrin	6.381	5.347	5270721	18327172	2.549m 2.516m
17) MA	4,4'-DDT	7.060	6.024	137.3E6	507.0E6	91.127m 89.565m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061024\
Data File : PD083586.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jun 2024 16:13
Operator : AR\AJ
Sample : P2648-09DL2 40X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 22:11:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060724CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 07 04:03:14 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

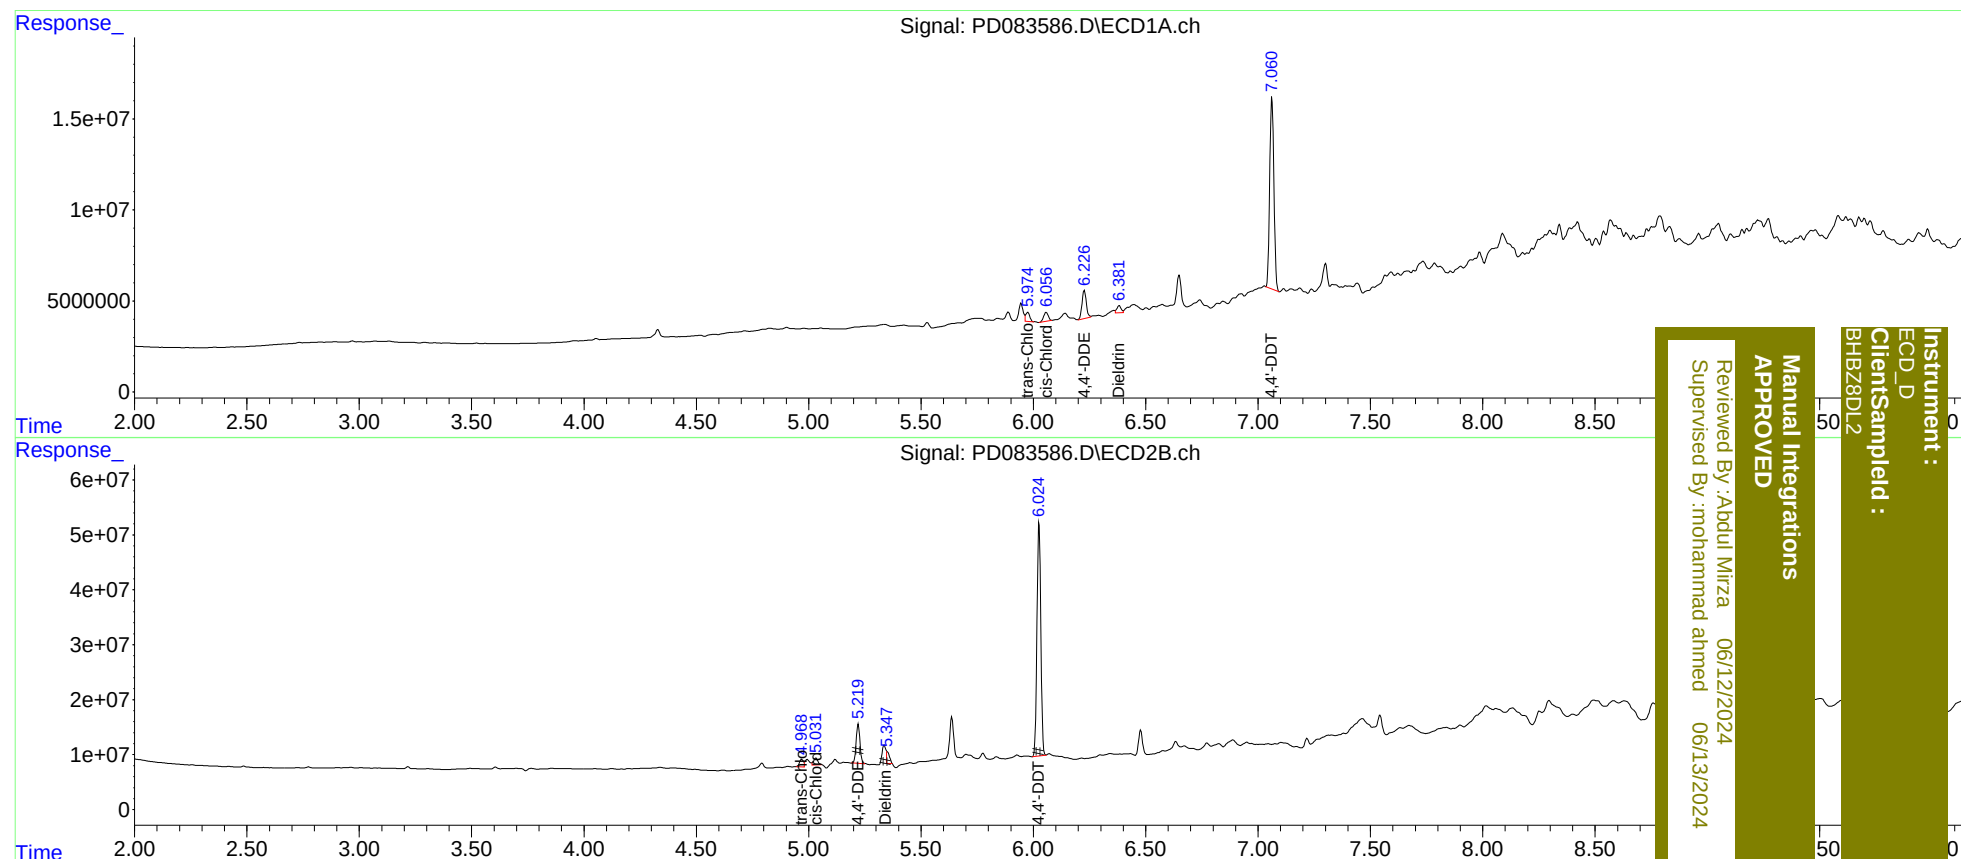

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 06/12/2024
Supervised By: mohammad ahmed 06/13/2024

Instrument :
ECD_D
Client Sampled :
BHBZ8DL2