

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD061024\  
 Data File : PD083627.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 11 Jun 2024 11:14  
 Operator : AR\AJ  
 Sample : P2659-13DL 5X  
 Misc :  
 ALS Vial : 50 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 BHC34DL

Manual Integrations  
 APPROVED

Reviewed By : Abdul Mirza 06/14/2024  
 Supervised By : Ankita Jodhani 06/17/2024

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jun 12 17:55:21 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD060724CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Jun 07 04:03:14 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml    |
|-----------------------------|-----------------|-------|-------|----------|----------|---------|----------|
| -----                       |                 |       |       |          |          |         |          |
| System Monitoring Compounds |                 |       |       |          |          |         |          |
| 1)                          | SA Tetrachlo... | 3.561 | 2.771 | 1629144  | 9254852  | 1.248m  | 1.698m#  |
| 27)                         | SA Decachlor... | 9.105 | 7.897 | 4481859  | 28758498 | 2.305m  | 4.736m#  |
| Target Compounds            |                 |       |       |          |          |         |          |
| 9)                          | A Endosulfan I  | 6.139 | 5.116 | 7074698  | 23766506 | 3.618m  | 3.595m   |
| 10)                         | B trans-Chl...  | 5.974 | 4.967 | 5897211  | 11737394 | 2.896m  | 1.616m#  |
| 11)                         | B cis-Chlor...  | 6.057 | 5.030 | 12911642 | 24969757 | 6.200   | 3.392m#  |
| 12)                         | B 4,4'-DDE      | 6.226 | 5.219 | 20184812 | 97325217 | 9.732   | 13.695m# |
| 13)                         | MA Dieldrin     | 6.382 | 5.351 | 122.0E6  | 465.9E6  | 58.985  | 63.953m  |
| 14)                         | MA Endrin       | 6.644 | 5.635 | 6048322  | 14426288 | 3.580m  | 2.231m#  |
| 16)                         | A 4,4'-DDD      | 6.738 | 5.774 | 3226911  | 6754091  | 2.202   | 1.198m#  |
| 17)                         | MA 4,4'-DDT     | 7.061 | 6.024 | 15590596 | 66373936 | 10.349m | 11.726   |
| -----                       |                 |       |       |          |          |         |          |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD061024\  
Data File : PD083627.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 11 Jun 2024 11:14  
Operator : AR\AJ  
Sample : P2659-13DL 5X  
Misc :  
ALS Vial : 50 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jun 12 17:55:21 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD060724CLP.M  
Quant Title : GC Extractables  
QLast Update : Fri Jun 07 04:03:14 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

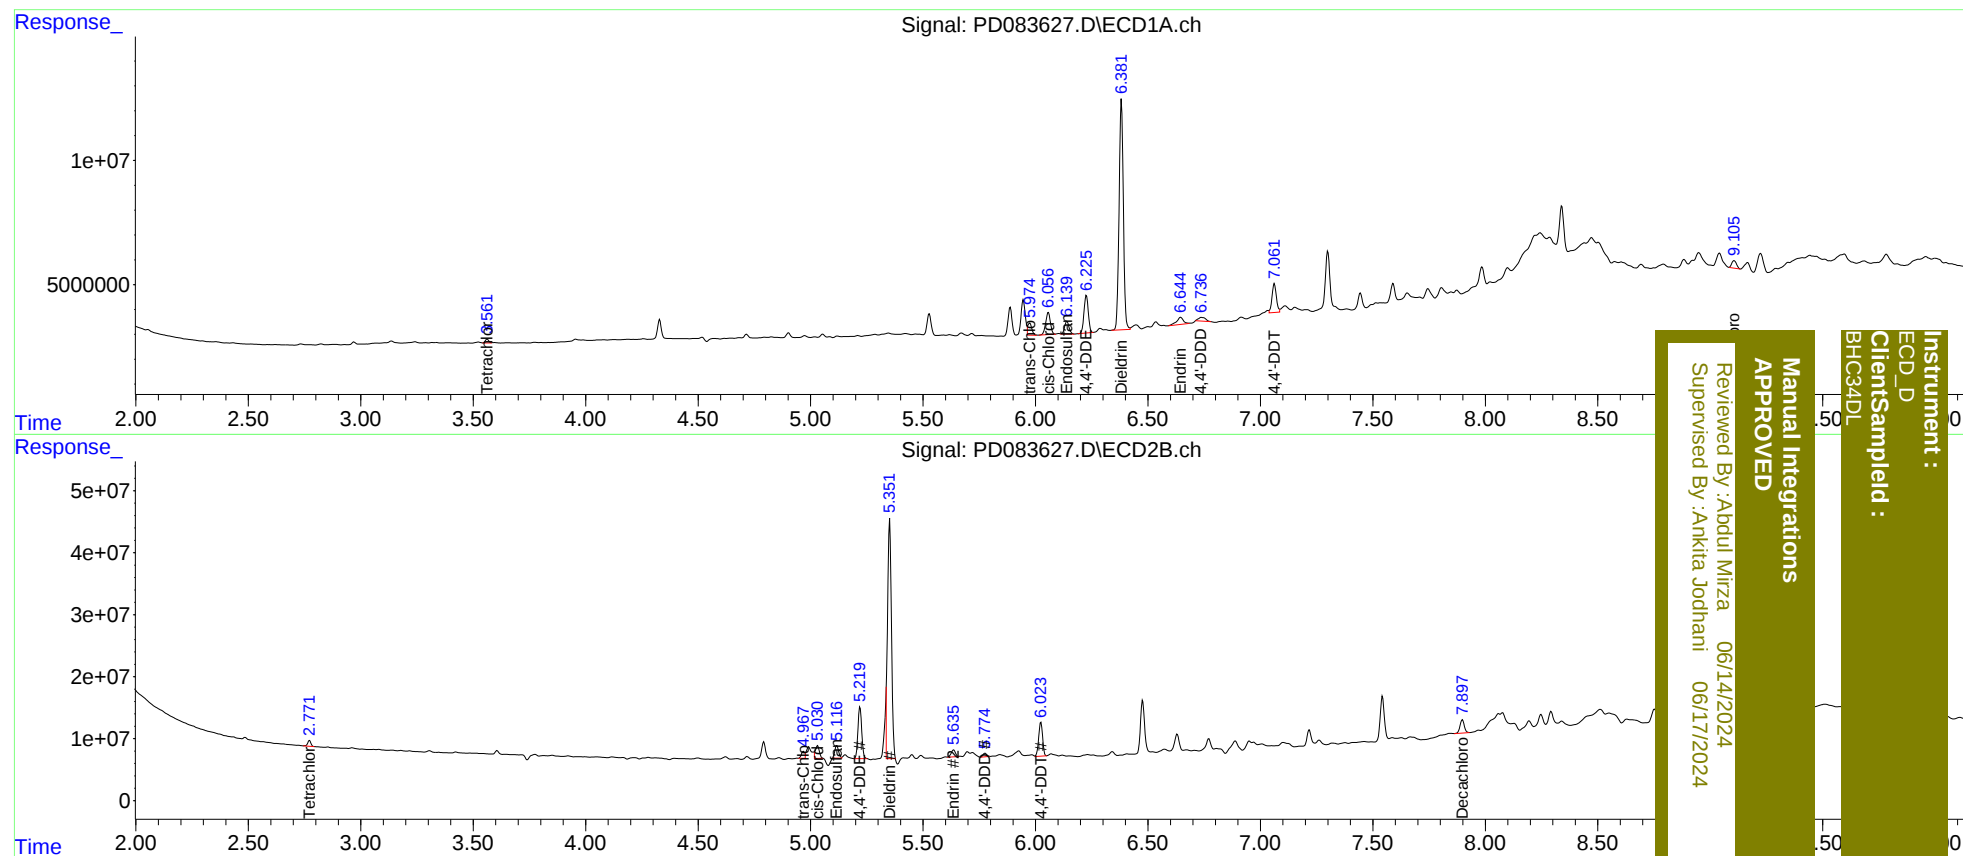

Manual Integrations  
APPROVED  
Reviewed By: Abdul Mirza 06/14/2024  
Supervised By: Ankita Jodhani 06/17/2024

Instrument :  
ECD\_D  
Client Sampled :  
BHC34DL