

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061423\
 Data File : PD075785.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2023 10:23
 Operator : AR\AJ
 Sample : 03062-04MS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZEL1MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/15/2023
 Supervised By : Ankita Jodhani 06/15/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 22:14:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.768	38383060	18739505	19.200	18.483
27)	SA Decachlor...	9.105	7.919	75879964	30973099	33.084	32.982
Target Compounds							
2)	A alpha-BHC	4.013	3.271	198.6E6	83228993	59.614	55.643
3)	MA gamma-BHC...	4.347	3.601	176.4E6	73697781	56.425	53.092
4)	MA Heptachlor	4.939	3.942	177.4E6	71839799	54.695	52.475
5)	MB Aldrin	5.282	4.222	189.8E6	78042359	58.582	55.224
6)	B beta-BHC	4.543	3.897	72984204	32601438	51.646	47.473m
7)	B delta-BHC	4.791	4.129	174.5E6	72361406	55.029m	49.916
8)	B Heptachlo...	5.709	4.725	161.3E6	65658093	52.780	49.902
9)	A Endosulfan I	6.097	5.096	148.3E6	61071948	55.948	52.883
10)	B trans-Chl...	5.967	4.977	159.0E6	66024545	54.405	51.921
11)	B cis-Chlor...	6.046	5.041	162.9E6	66952201	54.094	51.368
12)	B 4,4'-DDE	6.219	5.230	310.5E6	118.6E6	110.891	104.269
13)	MA Dieldrin	6.373	5.361	347.9E6	141.3E6	116.886	108.354
14)	MA Endrin	6.604	5.638	284.6E6	118.7E6	113.282	103.410
15)	B Endosulfa...	6.823	5.932	278.2E6	116.4E6	108.707	103.598
16)	A 4,4'-DDD	6.737	5.785	247.3E6	92657955	116.507	105.448
17)	MA 4,4'-DDT	7.052	6.038	260.3E6	96799795	126.798	118.972
18)	B Endrin al...	6.953	6.112	196.5E6	81865503	95.007	90.582
19)	B Endosulfa...	7.188	6.335	250.7E6	107.2E6	104.946	102.215
20)	A Methoxychlor	7.528	6.613	658.8E6	229.0E6	528.291	474.415
21)	B Endrin ke...	7.675	6.842	283.2E6	127.2E6	106.995	108.777

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061423\
Data File : PD075785.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2023 10:23
Operator : AR\AJ
Sample : 03062-04MS
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 22:14:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

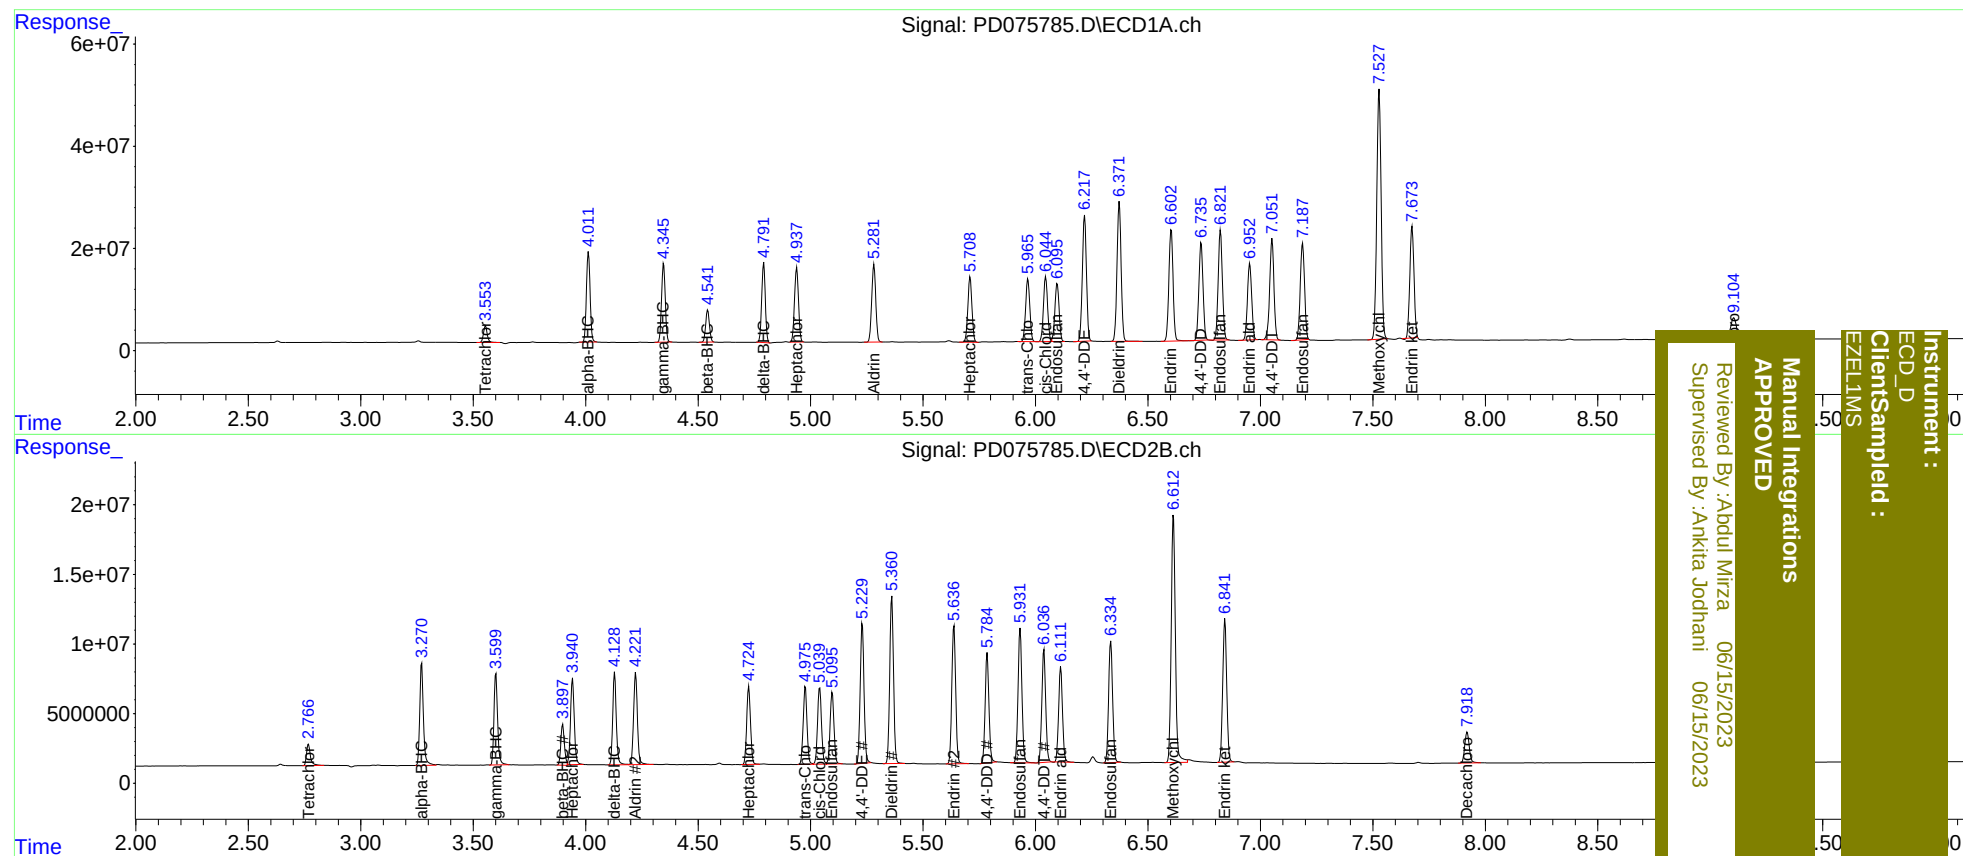

Instrument :
ECD_D
Client Sampled :
EZELIMS

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 06/15/2023
Supervised By: Ankita Jodhani 06/15/2023