

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061423\
 Data File : PD075786.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Jun 2023 10:36
 Operator : AR\AJ
 Sample : 03062-05MSD
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZEL1MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/16/2023
 Supervised By :Ankita Jodhani 06/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 14 22:15:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 02 04:01:43 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.768	40157317	19441859	20.088	19.176
27)	SA Decachlor...	9.093	7.915	77350658	32359917	33.725	34.458
Target Compounds							
2)	A alpha-BHC	4.005	3.271	204.0E6	85688547	61.225	57.288
3)	MA gamma-BHC...	4.338	3.601	181.5E6	75968969	58.047	54.728
4)	MA Heptachlor	4.930	3.941	183.2E6	73902252	56.478	53.982
5)	MB Aldrin	5.273	4.221	194.2E6	80246547	59.953	56.784
6)	B beta-BHC	4.535	3.896	76213922	32949912	53.932	47.981m
7)	B delta-BHC	4.782	4.128	178.8E6	75722603	56.386m	52.235
8)	B Heptachlo...	5.701	4.724	163.6E6	67888808	53.521	51.598
9)	A Endosulfan I	6.088	5.095	150.7E6	62830520	56.874	54.406
10)	B trans-Chl...	5.958	4.975	162.1E6	68140369	55.456	53.585
11)	B cis-Chlor...	6.037	5.039	165.3E6	69080689	54.917	53.001
12)	B 4,4'-DDE	6.210	5.229	318.4E6	126.3E6	113.718	110.999
13)	MA Dieldrin	6.364	5.360	350.2E6	145.6E6	117.668	111.696
14)	MA Endrin	6.595	5.636	286.2E6	122.5E6	113.920	106.703
15)	B Endosulfa...	6.814	5.930	280.7E6	120.0E6	109.712	106.804
16)	A 4,4'-DDD	6.728	5.784	252.7E6	100.1E6	119.043	113.892
17)	MA 4,4'-DDT	7.043	6.035	262.9E6	102.0E6	128.090	125.423
18)	B Endrin al...	6.944	6.109	199.6E6	85699784	96.547	94.825
19)	B Endosulfa...	7.179	6.332	257.5E6	111.2E6	107.801	106.070
20)	A Methoxychlor	7.520	6.610	670.2E6	246.1E6	537.420	509.831
21)	B Endrin ke...	7.666	6.839	294.2E6	132.2E6	111.157	113.024

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061423\
Data File : PD075786.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Jun 2023 10:36
Operator : AR\AJ
Sample : 03062-05MSD
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 14 22:15:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD060223CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jun 02 04:01:43 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

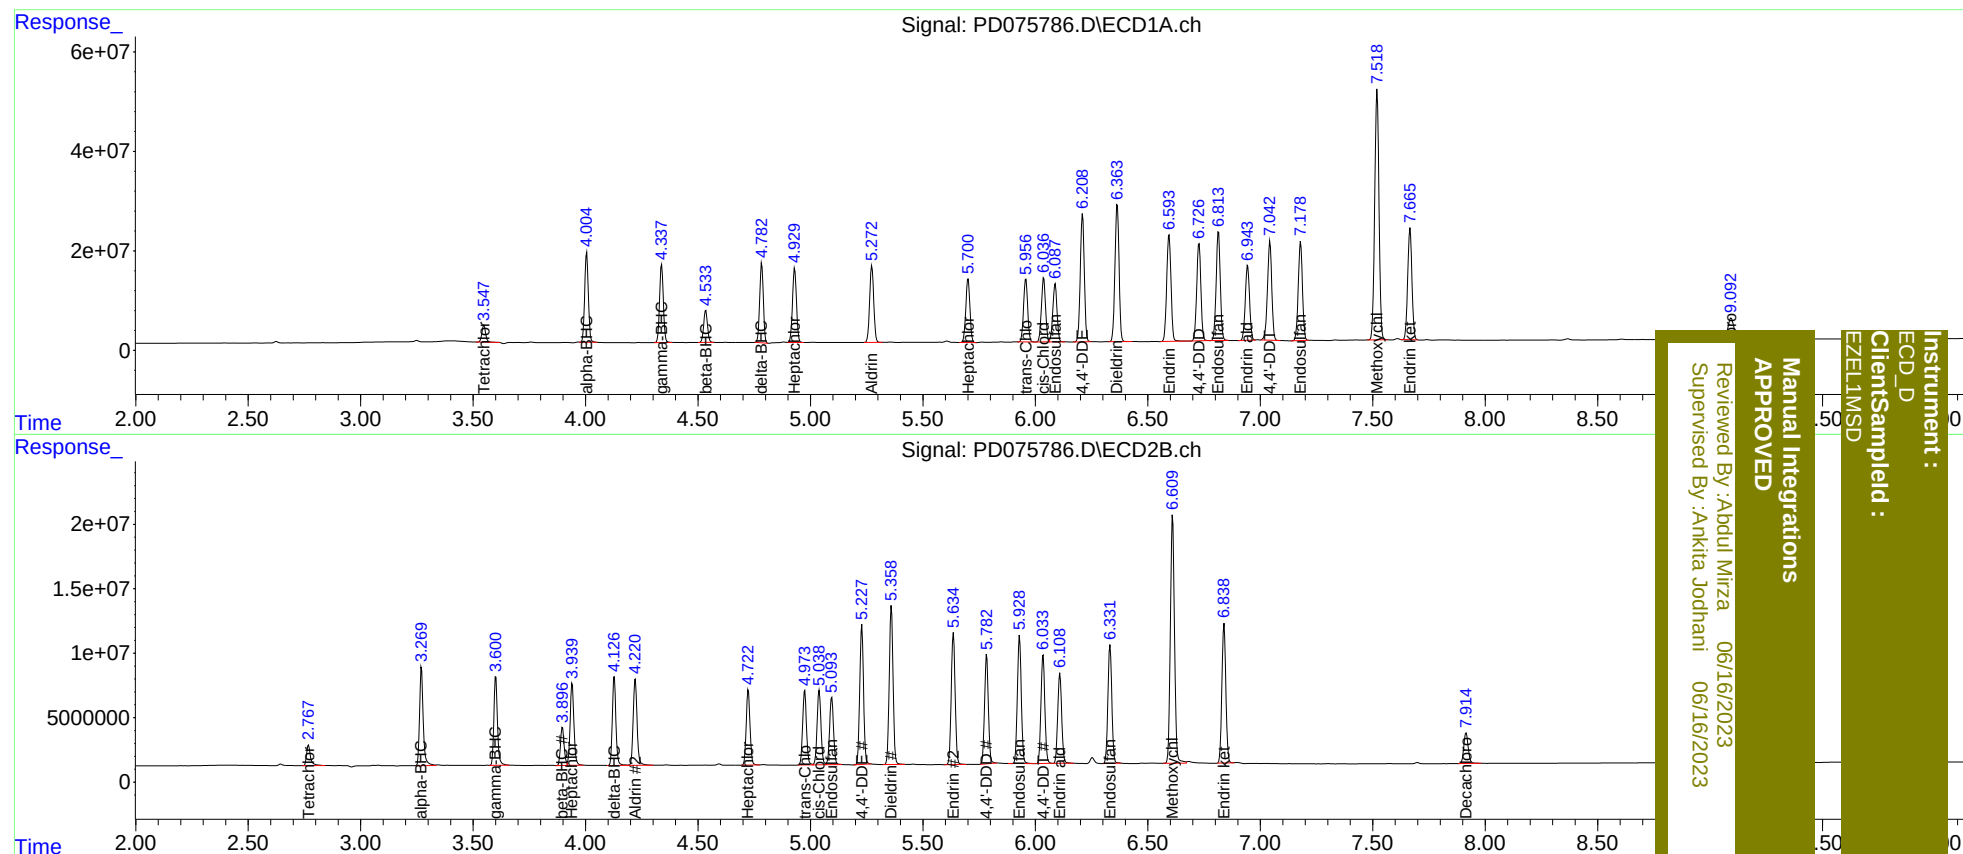

Instrument :
ECD_D
Client Sampled :
EZELMSD

Manual Integrations
APPROVED

Reviewed By: Abdul Mirza 06/16/2023
Supervised By: Ankita Jodhani 06/16/2023