

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061622\
 Data File : PD070361.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jun 2022 20:10
 Operator : AR\AJ
 Sample : N3358-09MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4R7MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/17/2022
 Supervised By : Ankita Jodhani 06/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 01:46:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 16:58:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.401	4.122	28595457	229.3E6	19.717	16.976
27)	SA Decachlor...	8.129	9.280	61658818	263.4E6	38.496	36.502
Target Compounds							
2)	A alpha-BHC	3.836	4.515	124.8E6	890.3E6	59.041	45.479
3)	MA gamma-BHC...	4.117	4.803	117.8E6	822.0E6	58.666	45.080
4)	MA Heptachlor	4.410	5.327	106.1E6	744.1E6	53.907	41.532
5)	MB Aldrin	4.655	5.637	112.4E6	757.8E6	58.917	45.592
6)	B beta-BHC	4.366	4.968	47377671	346.0E6	52.932	43.735
7)	B delta-BHC	4.567	5.190	122.8E6	727.6E6	60.856	56.394m
8)	B Heptachlo...	5.096	6.024	104.3E6	613.3E6	59.567	52.561
9)	A Endosulfan I	5.432	6.386	95862869	620.4E6	56.992	46.006
10)	B trans-Chl...	5.321	6.261	106.2E6	672.3E6	59.032	46.519
11)	B cis-Chlor...	5.379	6.335	102.2E6	650.9E6	57.760	46.354
12)	B 4,4'-DDE	5.545	6.486	210.9E6	1245.8E6	124.952	95.806
13)	MA Dieldrin	5.675	6.643	230.5E6	1296.4E6	121.511	94.654
14)	MA Endrin	5.931	6.863	202.1E6	1073.4E6	118.774	93.286
15)	B Endosulfa...	6.205	7.068	191.0E6	1031.2E6	117.718	93.755
16)	A 4,4'-DDD	6.060	6.975	180.8E6	1001.9E6	119.418	90.745m
17)	MA 4,4'-DDT	6.298	7.278	182.3E6	1001.3E6	125.254	97.385
18)	B Endrin al...	6.374	7.191	140.6E6	759.0E6	113.018	90.233m
19)	B Endosulfa...	6.586	7.417	184.2E6	941.0E6	116.279	95.205
20)	A Methoxychlor	6.848	7.733	478.4E6	2180.3E6	565.242	461.834
21)	B Endrin ke...	7.077	7.890	224.7E6	1014.2E6	125.989	99.557

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061622\
Data File : PD070361.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jun 2022 20:10
Operator : AR\AJ
Sample : N3358-09MSD
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 01:46:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 16:58:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

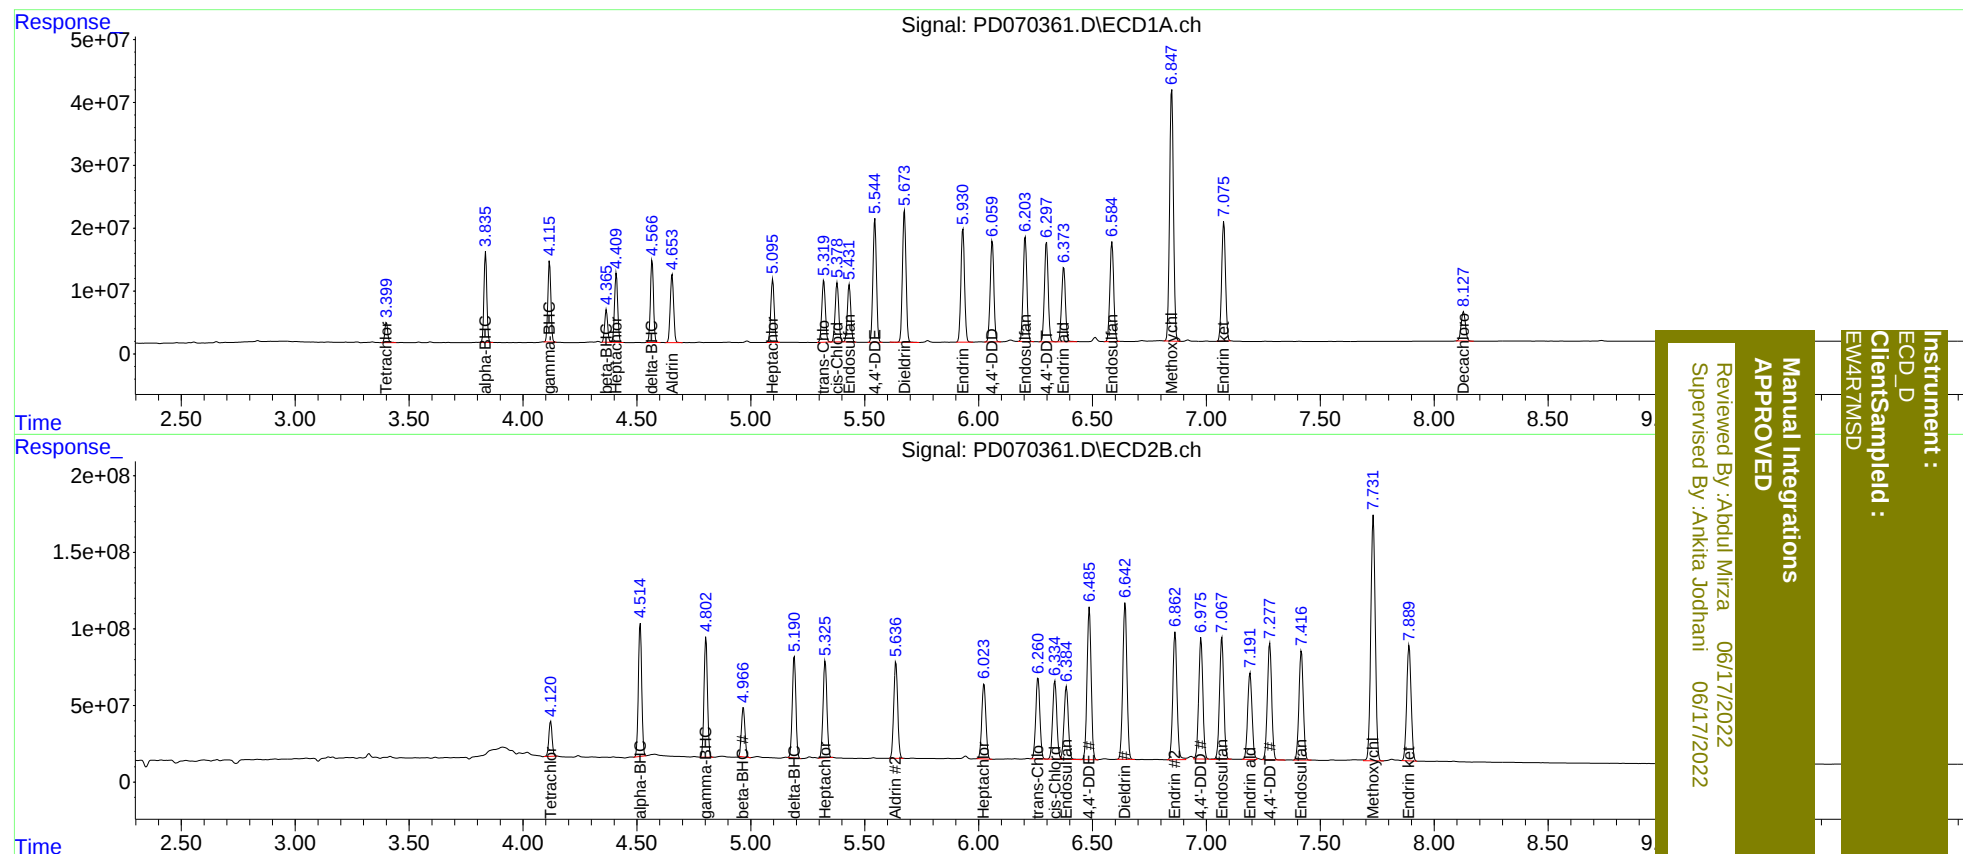

Reviewed By: Abdul Mirza 06/17/2022
Supervised By: Ankita Jodhani 06/17/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
EM4R7MSD