

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061622\
 Data File : PD070372.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jun 2022 22:46
 Operator : AR\AJ
 Sample : PB145615BS
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS615

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 06/17/2022
 Supervised By :Ankita Jodhani 06/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 01:52:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 16:58:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.401	4.122	30934800	262.0E6	21.329	19.392
27)	SA Decachlor...	8.128	9.279	68403261	285.5E6	42.707	39.553
Target Compounds							
2)	A alpha-BHC	3.836	4.515	10331474	89748705	4.889	4.585
3)	MA gamma-BHC...	4.117	4.803	10740878	92284089	5.349	5.061
4)	MA Heptachlor	4.410	5.327	10223418	90379516	5.195	5.045
5)	MB Aldrin	4.654	5.637	10624338	88134631	5.570m	5.303
6)	B beta-BHC	4.366	4.968	4942376	42767230	5.522	5.406
7)	B delta-BHC	4.566	5.190	8127762	48034261	4.027m	3.723m
8)	B Heptachlo...	5.096	6.022	10348193	71893157	5.907	6.161m
9)	A Endosulfan I	5.433	6.385	9730706	73297611	5.785	5.435
10)	B trans-Chl...	5.321	6.261	10487338	77445558	5.831	5.359
11)	B cis-Chlor...	5.380	6.335	10869446	76944060	6.145	5.480
12)	B 4,4'-DDE	5.545	6.486	19338984	141.2E6	11.456	10.860
13)	MA Dieldrin	5.673	6.642	20414840	145.0E6	10.762m	10.587m
14)	MA Endrin	5.932	6.862	18573432	114.7E6	10.914	9.972
15)	B Endosulfa...	6.205	7.067	17822960	115.9E6	10.983	10.535m
16)	A 4,4'-DDD	6.060	6.975	16938626	117.3E6	11.187	10.623m
17)	MA 4,4'-DDT	6.299	7.279	13103312	96059311	9.004	9.343
18)	B Endrin al...	6.374	7.192	16024775	101.5E6	12.882	12.071
19)	B Endosulfa...	6.586	7.416	16092555	98822477	10.160	9.998
20)	A Methoxychlor	6.849	7.733	44474248	243.9E6	52.547	51.661
21)	B Endrin ke...	7.076	7.890	20614332	114.9E6	11.560m	11.281

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061622\
Data File : PD070372.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jun 2022 22:46
Operator : AR\AJ
Sample : PB145615BS
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 01:52:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 16:58:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

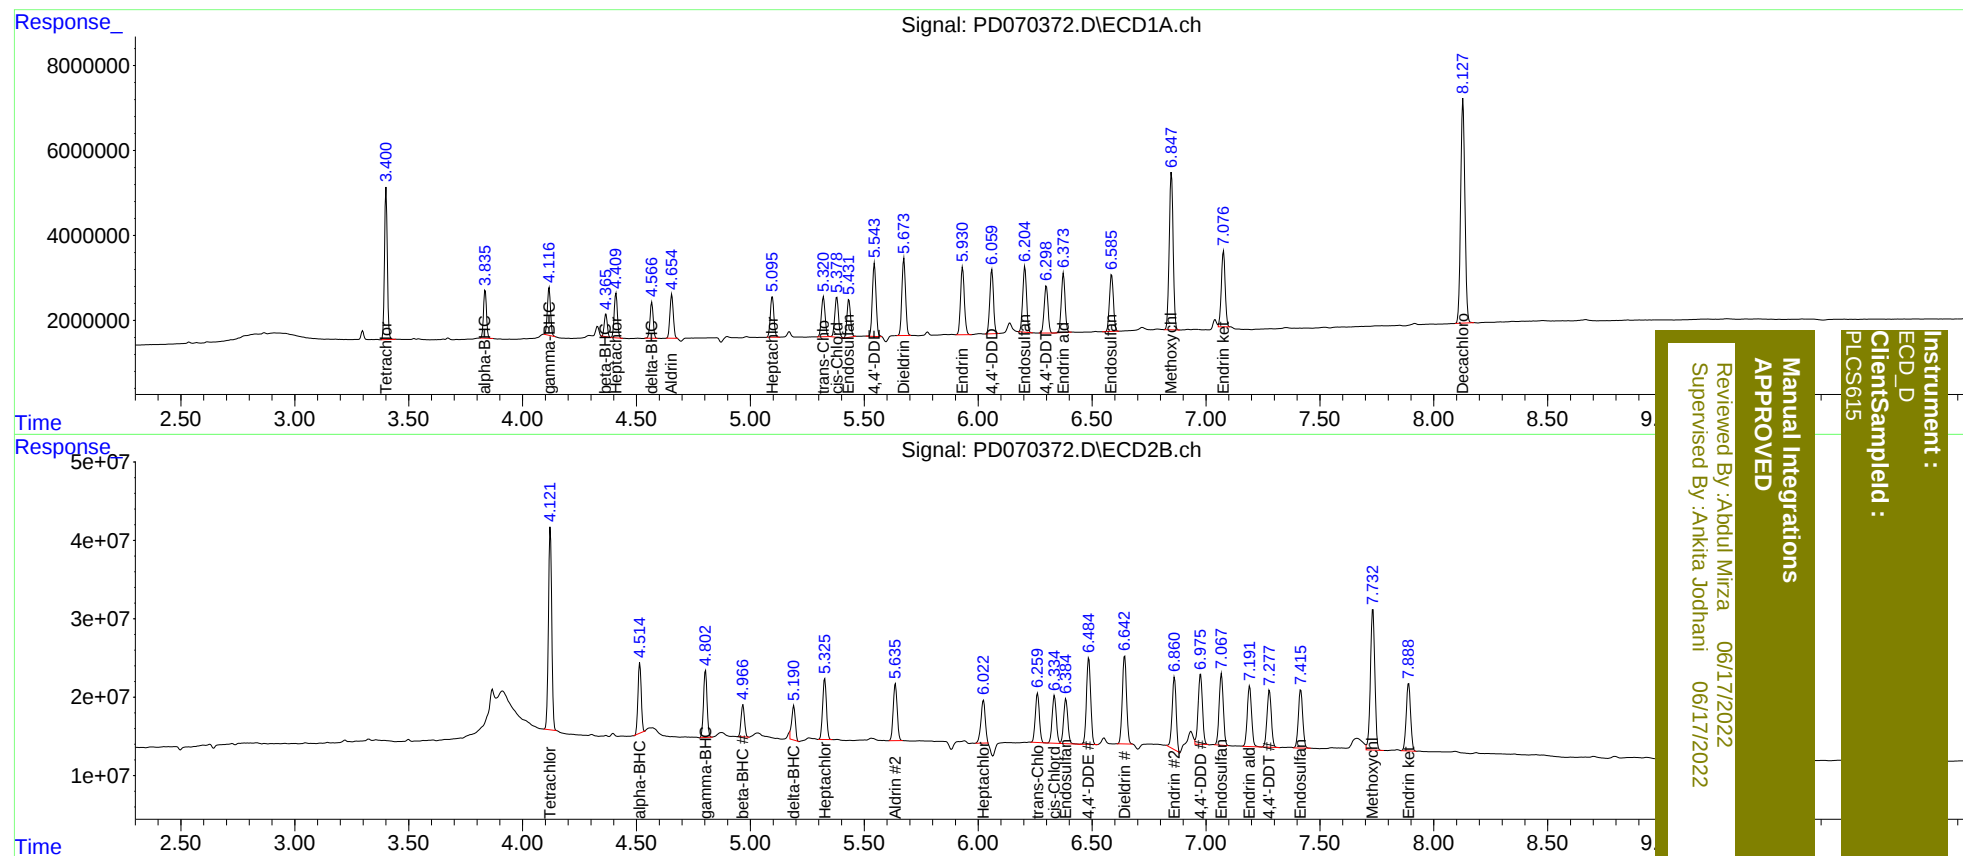

Reviewed By: Abdul Mirza 06/17/2022
Supervised By: Ankita Jodhani 06/17/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
PLCS615