

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061622\
 Data File : PD070360.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Jun 2022 19:56
 Operator : AR\AJ
 Sample : N3358-08MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EW4R7MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 06/17/2022
 Supervised By : Ankita Jodhani 06/17/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 17 01:46:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 14 16:58:30 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.401	4.123	28752777	232.5E6	19.825	17.208
27)	SA Decachlor...	8.128	9.280	61735068	264.6E6	38.544	36.662
Target Compounds							
2)	A alpha-BHC	3.835	4.516	125.4E6	898.6E6	59.344	45.902
3)	MA gamma-BHC...	4.117	4.804	118.3E6	830.6E6	58.927	45.550
4)	MA Heptachlor	4.410	5.327	105.6E6	747.8E6	53.661	41.741
5)	MB Aldrin	4.655	5.638	112.8E6	761.1E6	59.111	45.791
6)	B beta-BHC	4.365	4.968	46904820	355.7E6	52.404	44.964
7)	B delta-BHC	4.567	5.190	122.8E6	715.7E6	60.865	55.468m
8)	B Heptachlo...	5.096	6.025	104.6E6	598.2E6	59.703	51.265
9)	A Endosulfan I	5.432	6.386	96033180	620.7E6	57.093	46.029
10)	B trans-Chl...	5.320	6.262	106.5E6	673.7E6	59.234	46.612
11)	B cis-Chlor...	5.378	6.336	102.8E6	652.8E6	58.112	46.493
12)	B 4,4'-DDE	5.544	6.487	211.3E6	1246.9E6	125.153	95.894
13)	MA Dieldrin	5.674	6.644	230.5E6	1297.7E6	121.520	94.749
14)	MA Endrin	5.931	6.863	202.3E6	1074.5E6	118.849	93.386
15)	B Endosulfa...	6.204	7.069	191.5E6	1033.0E6	118.006	93.921
16)	A 4,4'-DDD	6.059	6.977	181.3E6	1013.9E6	119.727	91.826
17)	MA 4,4'-DDT	6.298	7.279	182.3E6	1002.8E6	125.299	97.528
18)	B Endrin al...	6.374	7.191	140.7E6	759.0E6	113.082	90.237m
19)	B Endosulfa...	6.585	7.417	184.6E6	939.8E6	116.523	95.078
20)	A Methoxychlor	6.847	7.733	477.8E6	2177.4E6	564.556	461.210
21)	B Endrin ke...	7.076	7.890	224.3E6	1015.6E6	125.798	99.696

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD061622\
Data File : PD070360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Jun 2022 19:56
Operator : AR\AJ
Sample : N3358-08MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 17 01:46:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061422CLP.M
Quant Title : GC Extractables
QLast Update : Tue Jun 14 16:58:30 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

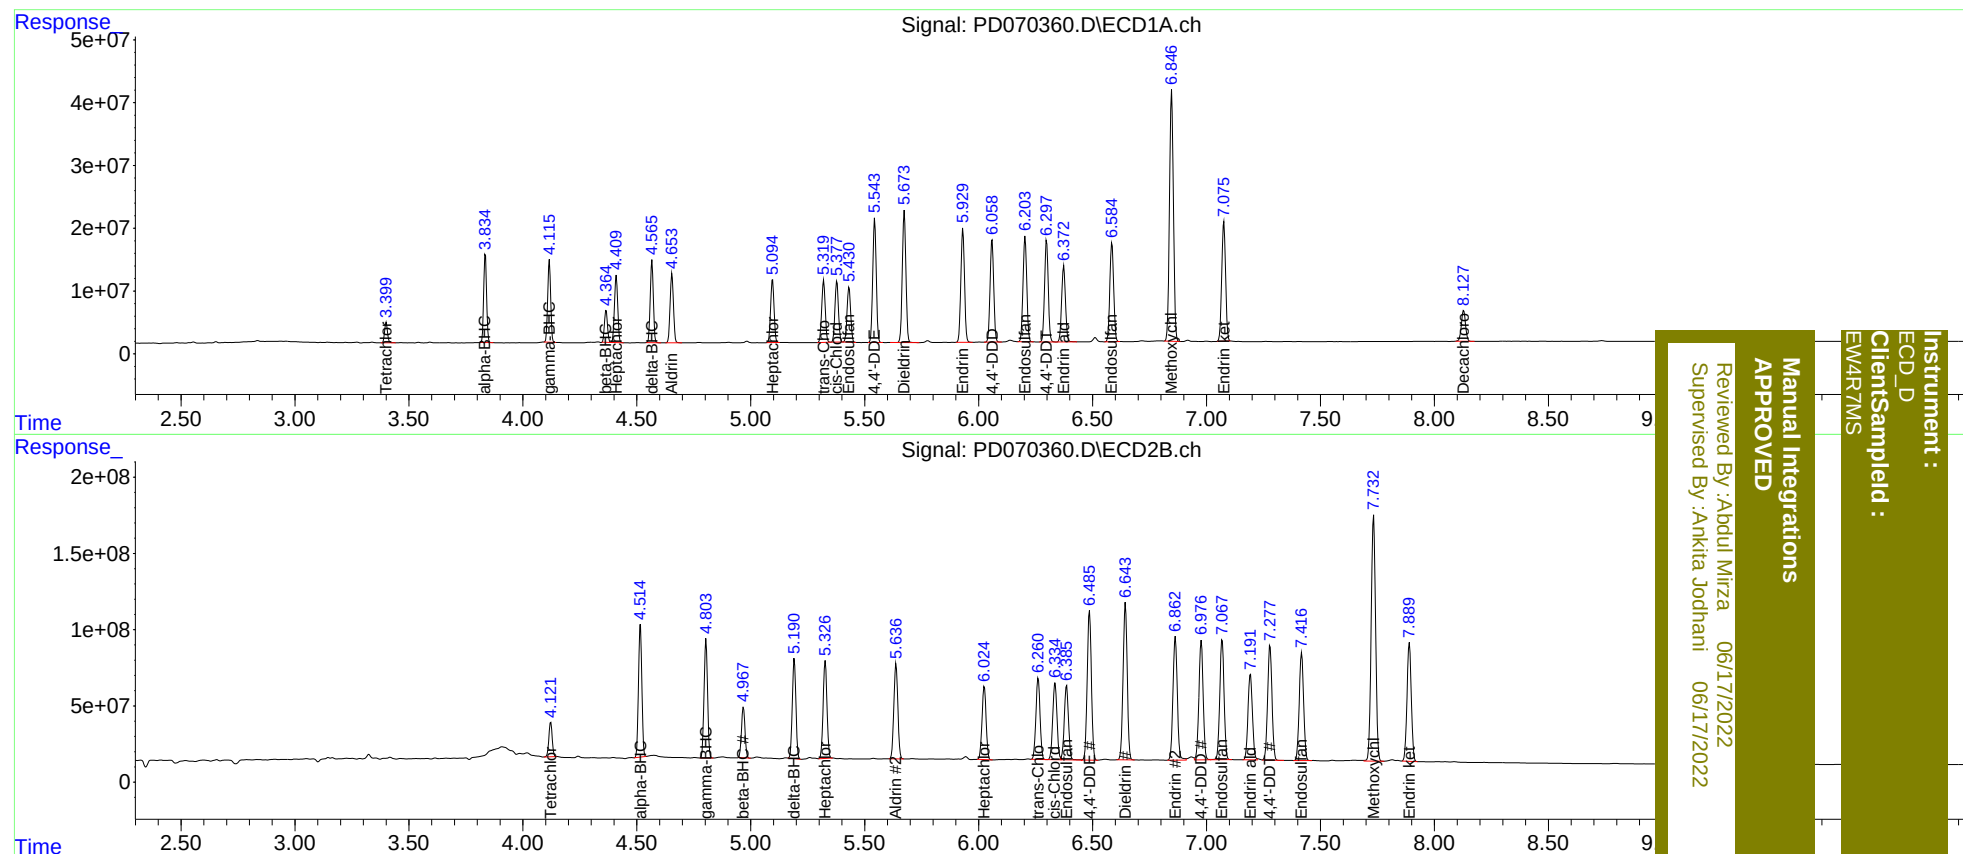

Reviewed By: Abdul Mirza 06/17/2022
Supervised By: Ankita Jodhani 06/17/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
EW4R7MS