

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070122\
 Data File : PD070684.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2022 13:08
 Operator : AR\AJ
 Sample : N3425-20MS
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AE5MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/05/2022
 Supervised By : Ankita Jodhani 07/05/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 06:22:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070122CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 01 11:10:28 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	4.125	32911105	365.6E6	13.812	14.157
27)	SA Decachlor...	8.265	9.313	55772192	171.4E6	23.722	24.672
Target Compounds							
2)	A alpha-BHC	3.929	4.530	180.3E6	1767.9E6	53.683	48.303
3)	MA gamma-BHC...	4.214	4.823	171.6E6	1656.9E6	52.517	49.791
4)	MA Heptachlor	4.516	5.338	166.8E6	1524.3E6	51.283	48.477
5)	MB Aldrin	4.765	5.650	175.1E6	1421.5E6	53.732	50.920
6)	B beta-BHC	4.464	4.999	72640724	673.4E6	48.425	43.022
7)	B delta-BHC	4.670	5.223	179.8E6	1603.2E6	55.246	52.109
8)	B Heptachlo...	5.211	6.045	156.8E6	1184.1E6	52.176	50.120
9)	A Endosulfan I	5.551	6.410	144.1E6	999.2E6	51.342	49.909
10)	B trans-Chl...	5.438	6.281	164.0E6	1134.5E6	52.034	49.544
11)	B cis-Chlor...	5.497	6.354	158.0E6	1075.9E6	51.409	49.662
12)	B 4,4'-DDE	5.663	6.509	318.6E6	2013.9E6	107.344	102.830
13)	MA Dieldrin	5.796	6.671	338.0E6	2037.7E6	108.197	103.516
14)	MA Endrin	6.055	6.894	287.1E6	1518.0E6	110.865	107.495
15)	B Endosulfa...	6.328	7.107	276.4E6	1468.6E6	110.152	105.163
16)	A 4,4'-DDD	6.181	7.007	261.0E6	1512.4E6	104.231	100.355m
17)	MA 4,4'-DDT	6.423	7.309	274.9E6	1449.5E6	112.658	110.780
18)	B Endrin al...	6.499	7.233	195.2E6	1056.8E6	93.255	90.870
19)	B Endosulfa...	6.711	7.456	253.4E6	1306.8E6	102.319	100.275
20)	A Methoxychlor	6.975	7.769	700.2E6	3114.2E6	535.435	534.026
21)	B Endrin ke...	7.205	7.938	300.2E6	1281.6E6	111.297	108.349

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070122\
Data File : PD070684.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2022 13:08
Operator : AR\AJ
Sample : N3425-20MS
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 06:22:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070122CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 01 11:10:28 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

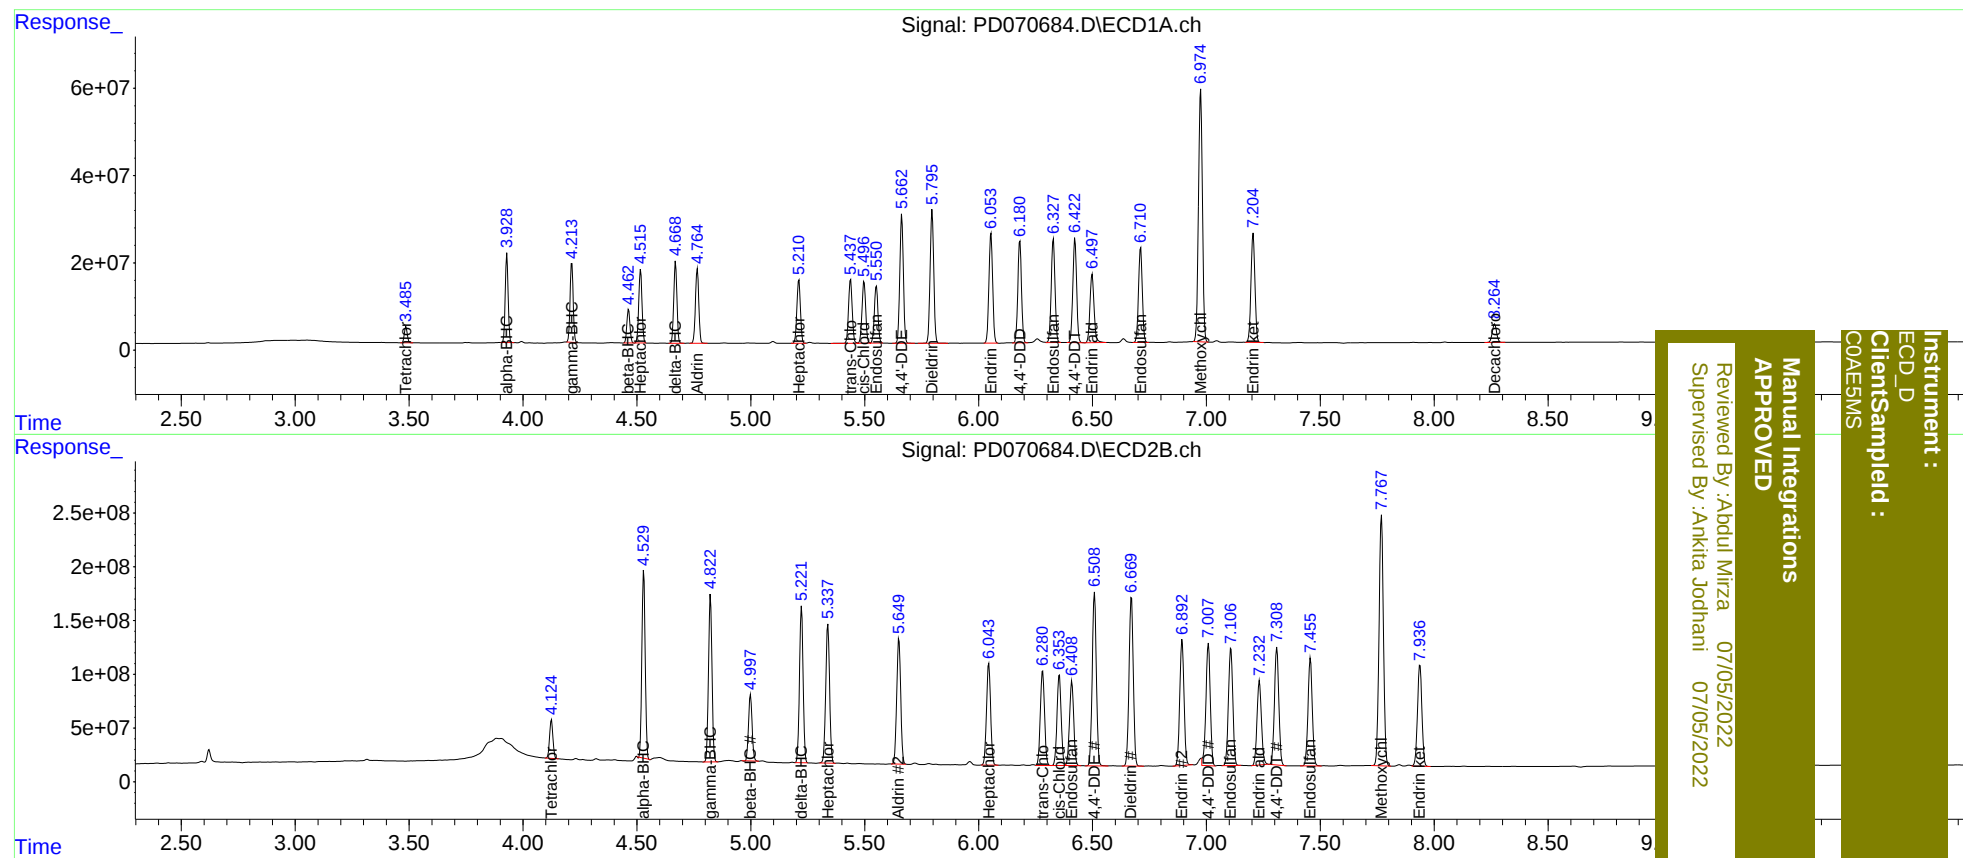

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 07/05/2022
Supervised By: Ankita Jodhani 07/05/2022

Instrument :
ECD_D
ClientSampled :
COAESMS