

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070122\
 Data File : PD070685.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2022 13:22
 Operator : AR\AJ
 Sample : N3425-21MSD
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AE5MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/05/2022
 Supervised By : Ankita Jodhani 07/05/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 06:23:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070122CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 01 11:10:28 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	4.125	32626957	361.1E6	13.693	13.982
27)	SA Decachlor...	8.266	9.314	55718885	171.6E6	23.700	24.707
Target Compounds							
2)	A alpha-BHC	3.929	4.530	178.9E6	1766.5E6	53.282	48.266
3)	MA gamma-BHC...	4.214	4.822	170.2E6	1650.6E6	52.072	49.601
4)	MA Heptachlor	4.516	5.337	167.2E6	1516.3E6	51.384	48.223
5)	MB Aldrin	4.765	5.650	174.7E6	1416.1E6	53.600	50.728
6)	B beta-BHC	4.463	4.997	72429910	674.8E6	48.284	43.116
7)	B delta-BHC	4.669	5.221	179.6E6	1599.6E6	55.189	51.992
8)	B Heptachlo...	5.211	6.045	156.6E6	1180.2E6	52.118	49.955
9)	A Endosulfan I	5.551	6.409	143.5E6	1000.0E6	51.123	49.953
10)	B trans-Chl...	5.437	6.281	164.1E6	1132.5E6	52.082	49.456
11)	B cis-Chlor...	5.497	6.354	157.8E6	1076.9E6	51.366	49.709
12)	B 4,4'-DDE	5.663	6.509	319.7E6	2018.0E6	107.707	103.039
13)	MA Dieldrin	5.796	6.670	338.5E6	2036.7E6	108.343	103.465
14)	MA Endrin	6.055	6.893	288.6E6	1525.9E6	111.464	108.048
15)	B Endosulfa...	6.328	7.106	275.7E6	1471.8E6	109.889	105.392
16)	A 4,4'-DDD	6.181	7.007	260.5E6	1521.5E6	104.007	100.962m
17)	MA 4,4'-DDT	6.423	7.309	276.0E6	1457.7E6	113.122	111.402
18)	B Endrin al...	6.498	7.233	195.2E6	1057.3E6	93.245	90.912
19)	B Endosulfa...	6.711	7.457	254.1E6	1313.1E6	102.616	100.762
20)	A Methoxychlor	6.975	7.768	707.1E6	3142.3E6	540.692	538.831
21)	B Endrin ke...	7.206	7.938	300.4E6	1282.3E6	111.373	108.411

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070122\
Data File : PD070685.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2022 13:22
Operator : AR\AJ
Sample : N3425-21MSD
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 06:23:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070122CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 01 11:10:28 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

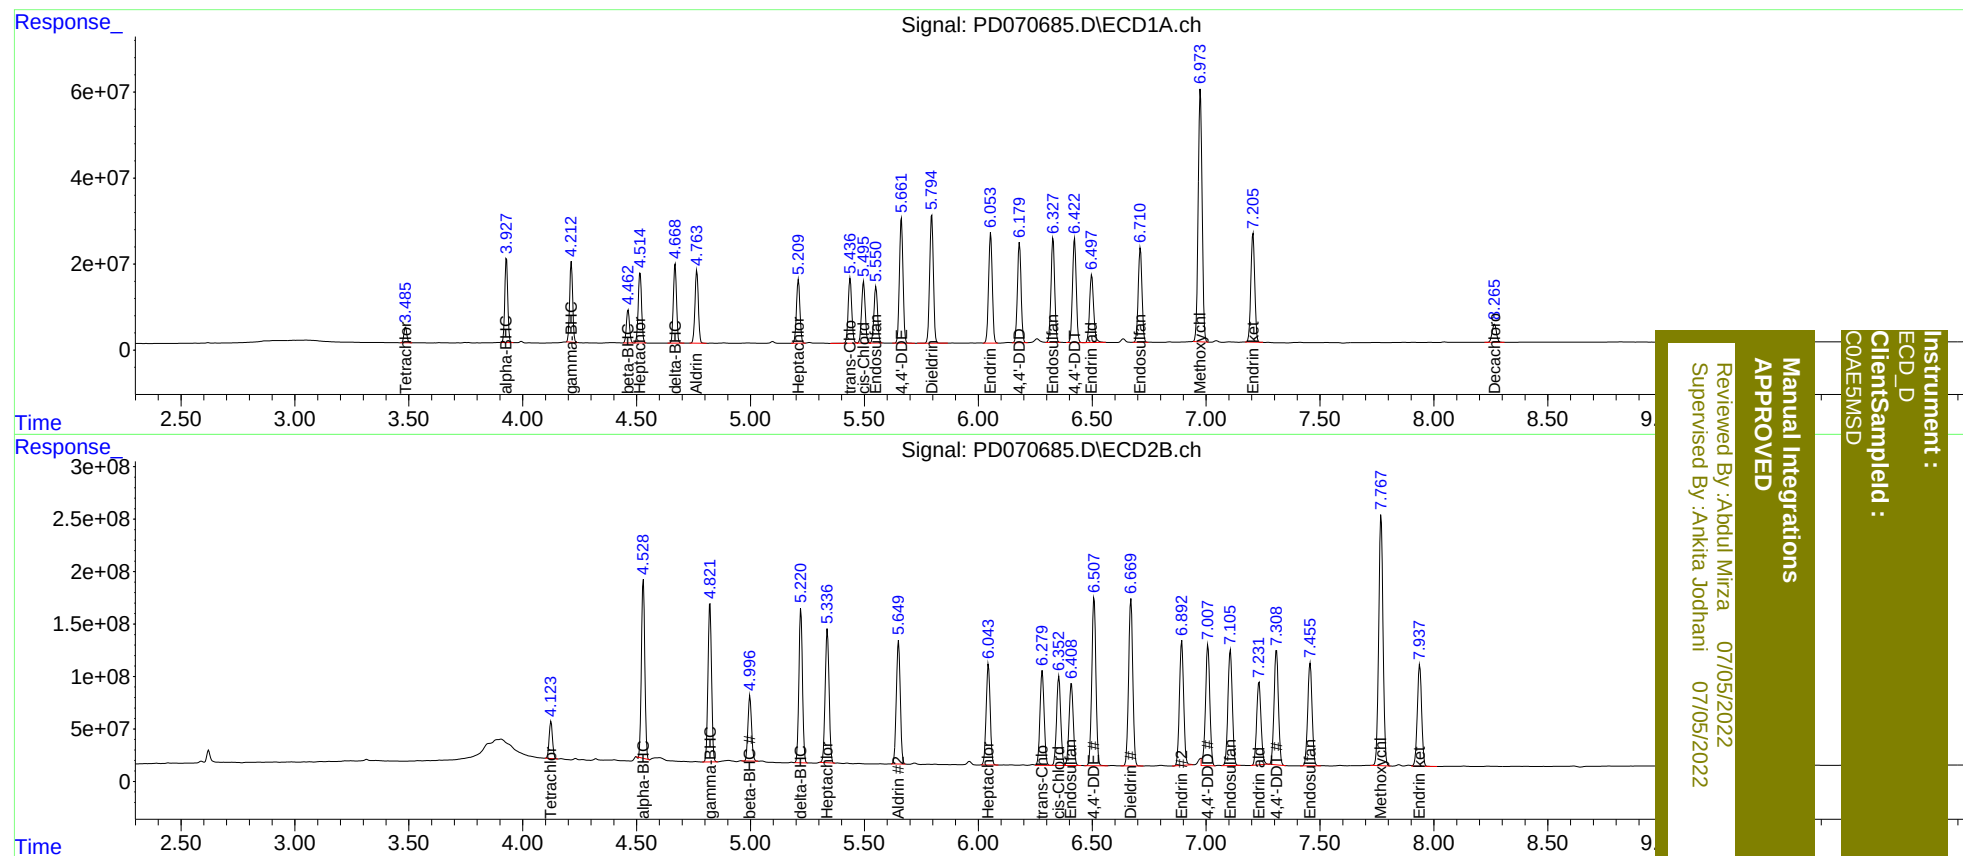

Reviewed By: Abdul Mirza 07/05/2022
Supervised By: Ankita Jodhani 07/05/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
COAESMSD