

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070122\
 Data File : PD070651.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2022 05:03
 Operator : AR\AJ
 Sample : RESC031
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC033

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 13 08:50:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070122CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Jul 01 11:10:28 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.486	4.126	49136834	527.2E6	20.621	20.415
2)	SA Decachlor...	8.266	9.317	97543331	288.8E6	41.489	41.577
Target Compounds							
2)	A alpha-BHC	3.929	4.531	35990342	405.8E6	10.717	11.089
3)	MA gamma-BHC...	4.214	4.823	35481364	373.7E6	10.858	11.230
4)	MA Heptachlor	4.516	5.338	35520835	354.8E6	10.919	11.283
5)	MB Aldrin	4.766	5.651	33221979	292.3E6	10.194	10.469
6)	B beta-BHC	4.464	4.999	15684966	168.6E6	10.456	10.775
7)	B delta-BHC	4.670	5.222	32274910	313.7E6	9.915	10.198
8)	B Heptachlo...	5.212	6.045	30569271	247.6E6	10.174	10.479
9)	A Endosulfan I	5.552	6.409	31006401	224.5E6	11.049	11.215
10)	B trans-Chl...	5.439	6.282	31755251	236.4E6	10.078	10.324
11)	B cis-Chlor...	5.498	6.355	31079329	223.8E6	10.114	10.332
12)	B 4,4'-DDE	5.664	6.509	58491869	399.8E6	19.706	20.412
13)	MA Dieldrin	5.797	6.671	67554294	433.3E6	21.623	22.012
14)	MA Endrin	6.056	6.894	57824465	318.5E6	22.332	22.551
15)	B Endosulfa...	6.329	7.107	50813631	286.6E6	20.250	20.524
16)	A 4,4'-DDD	6.182	7.009	54655733	334.4E6	21.823	22.186
17)	MA 4,4'-DDT	6.424	7.310	53002052	289.0E6	21.722	22.084
18)	B Endrin al...	6.500	7.234	43795923	239.2E6	20.922	20.565
19)	B Endosulfa...	6.712	7.457	50174020	267.5E6	20.263	20.524
20)	A Methoxychlor	6.976	7.769	147.4E6	654.7E6	112.695	112.262
21)	B Endrin ke...	7.207	7.939	56801775	252.9E6	21.056	21.384

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070122\
Data File : PD070651.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2022 05:03
Operator : AR\AJ
Sample : RESC031
Misc :
ALS Vial : 30 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 08:50:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070122CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 01 11:10:28 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

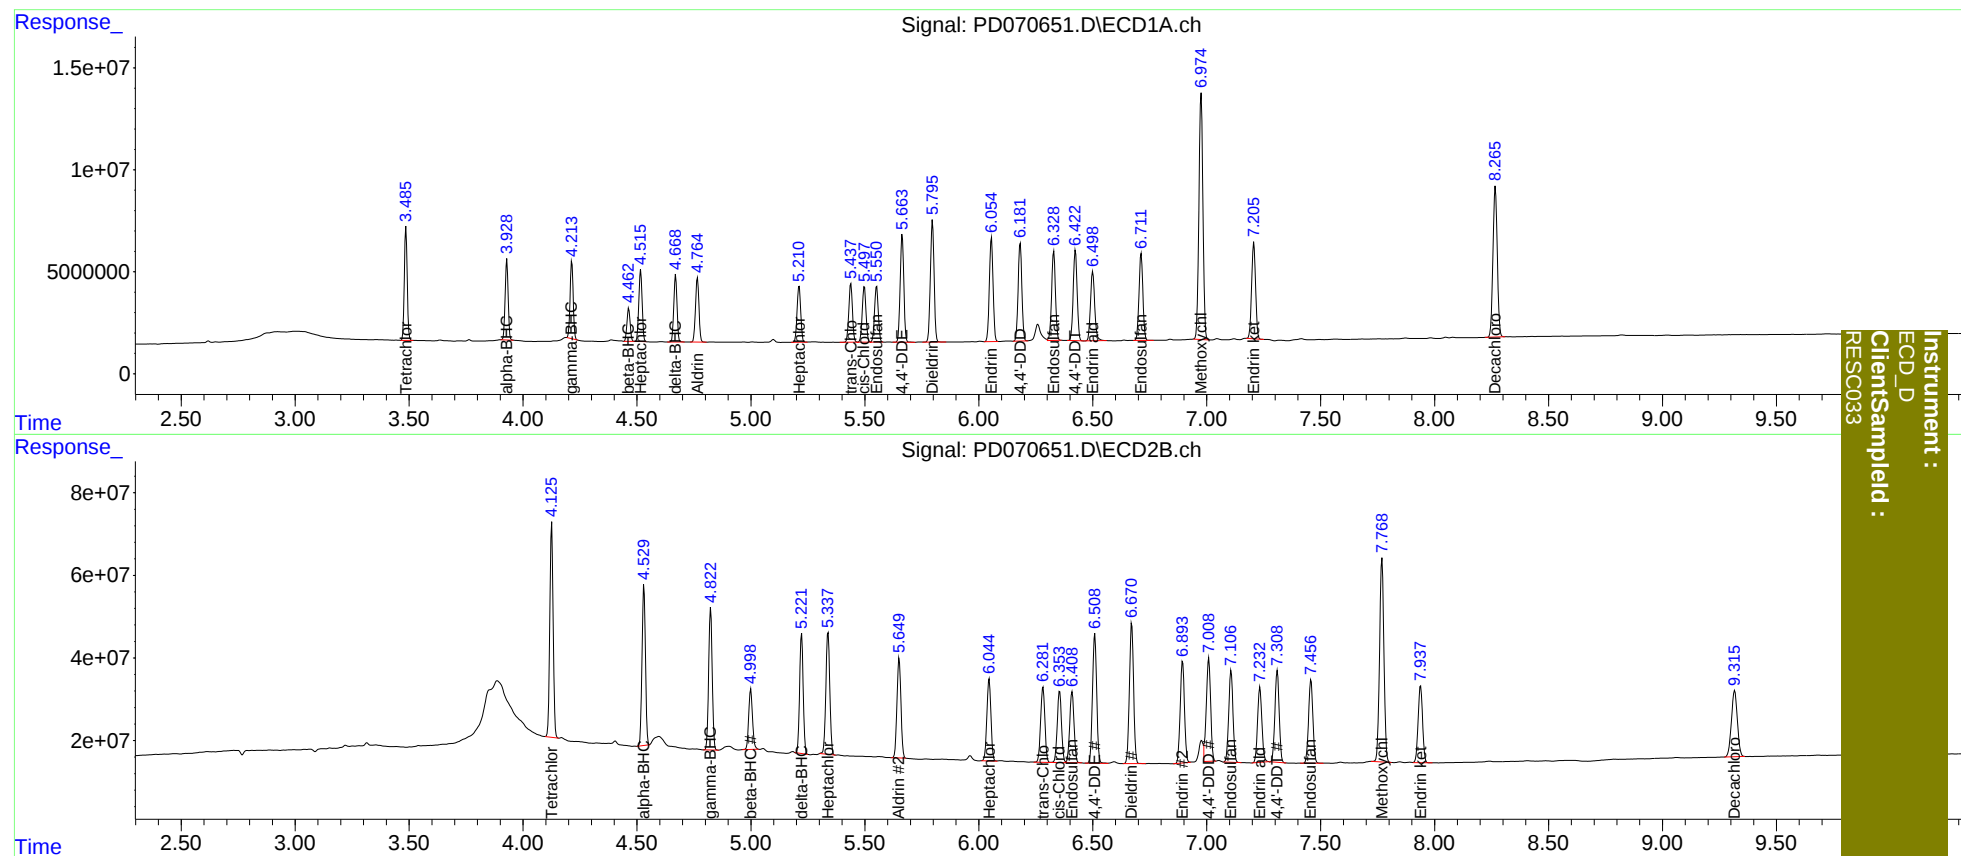

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070122\
Data File : PD070651.D
Acq On : 01 Jul 2022 05:03
Operator : AR\AJ
Sample : RESC031
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC033

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070122CLP.M
Title : GC Extractables
Last Update : Fri Jul 01 11:10:28 2022
Integrator: ChemStation

RT#1	RT#2	Resolution
3.486	3.929	100.00%
3.929	4.214	100.00%
4.214	4.464	100.00%
4.464	4.516	100.00%
4.516	4.670	100.00%
4.670	4.766	100.00%
4.766	5.212	100.00%
5.212	5.439	100.00%
5.439	5.498	99.32%
5.498	5.552	99.19%
5.552	5.664	100.00%
5.664	5.797	100.00%
5.797	6.056	100.00%
6.056	6.182	100.00%
6.182	6.329	100.00%
6.329	6.424	100.00%
6.424	6.500	100.00%
6.500	6.712	100.00%
6.712	6.976	100.00%
6.976	7.207	100.00%
7.207	8.266	100.00%

Signal #2


4.126	4.531	100.00%
4.531	4.823	100.00%
4.823	4.999	100.00%
4.999	5.222	100.00%
5.222	5.339	100.00%
5.339	5.651	100.00%
5.651	6.045	100.00%
6.045	6.282	100.00%
6.282	6.355	99.31%
6.355	6.409	99.62%
6.409	6.509	100.00%
6.509	6.671	100.00%
6.671	6.894	100.00%
6.894	7.009	100.00%
7.009	7.107	100.00%
7.107	7.234	100.00%
7.234	7.310	100.00%
7.310	7.457	100.00%
7.457	7.769	100.00%
7.769	7.939	100.00%
7.939	9.317	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070122\
Data File : PD070651.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2022 05:03
Operator : AR\AJ
Sample : RESC031
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC033

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 08:50:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070122CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 01 11:10:28 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

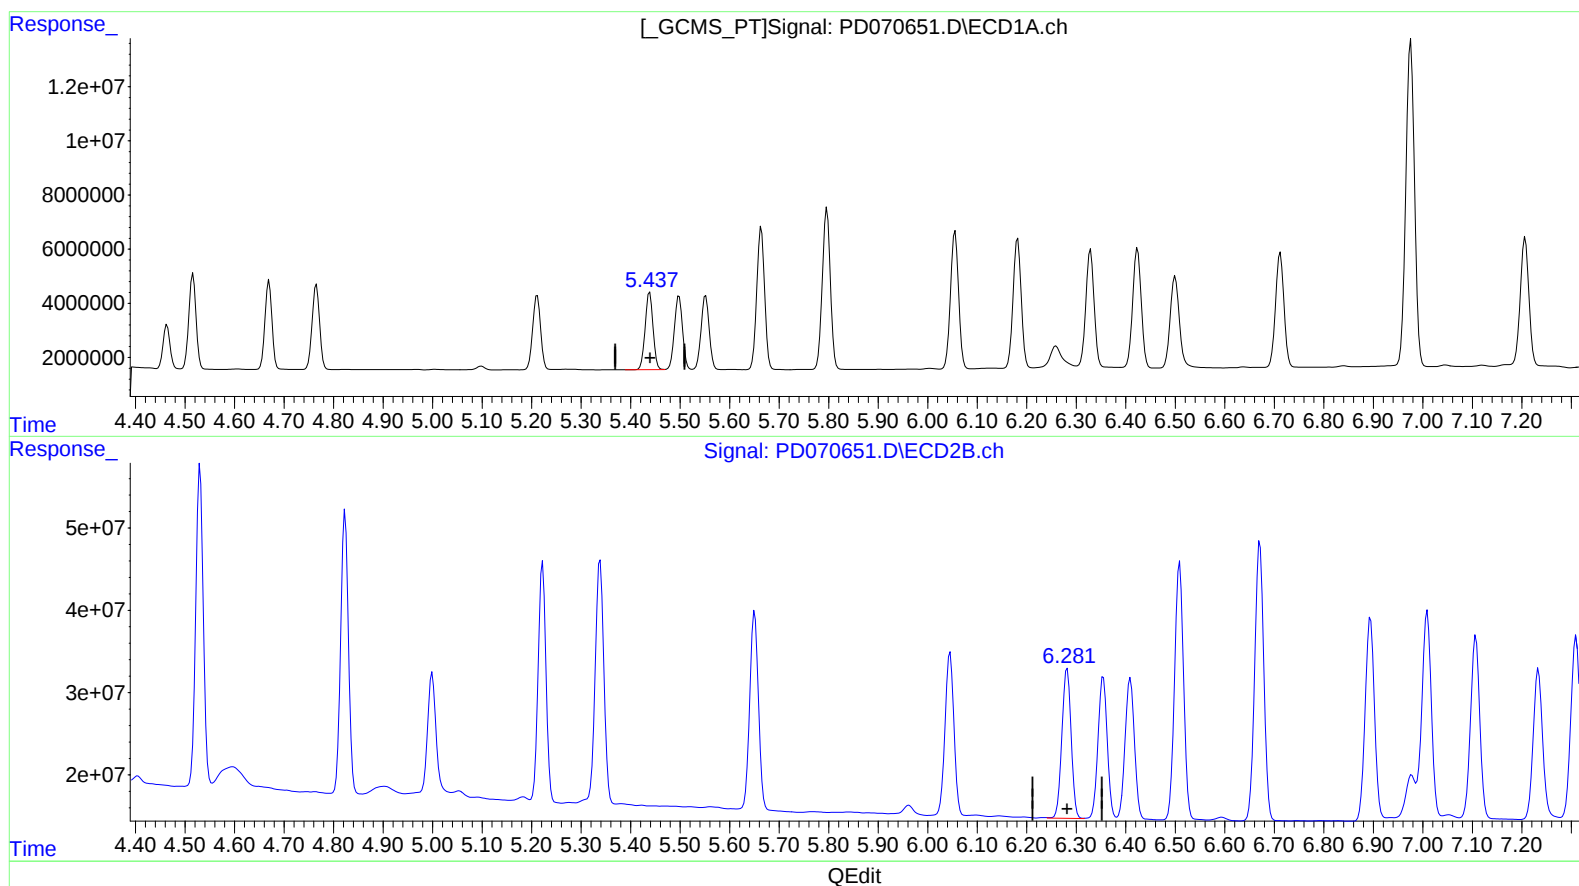

(10) trans-Chlordane (B)

5.439min 10.078 ng/ml

response 31755251

(10) trans-Chlordane #2 (B)

6.282min 10.324 ng/ml


response 236400277

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070122\
Data File : PD070651.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2022 05:03
Operator : AR\AJ
Sample : RESC031
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC033

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 13 08:50:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070122CLP.M
Quant Title : GC Extractables
QLast Update : Fri Jul 01 11:10:28 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

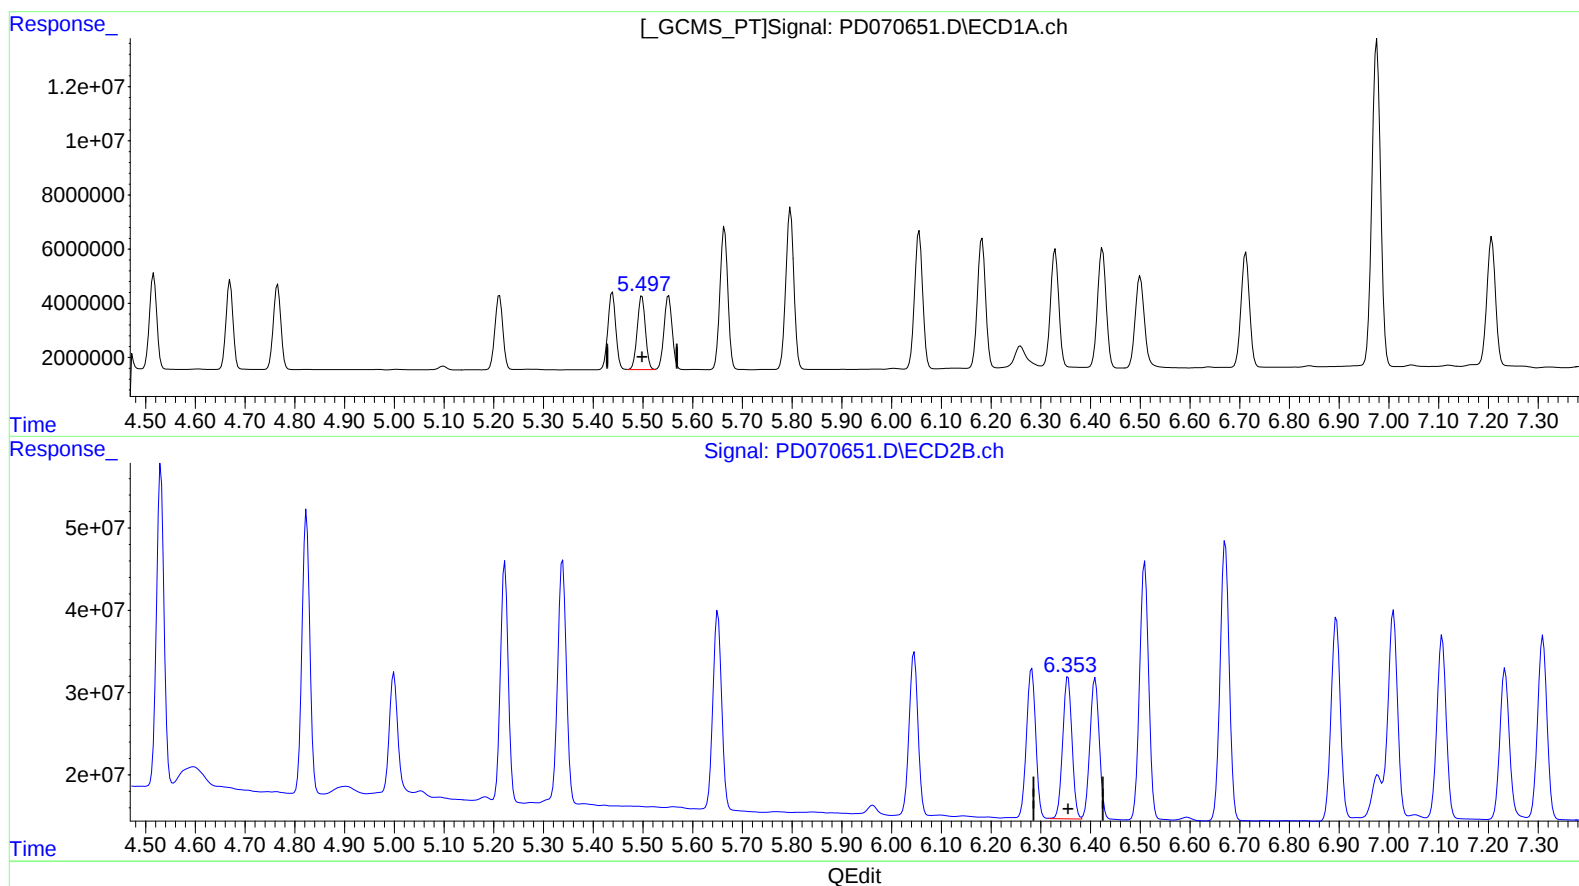

(11) cis-Chlordane (B)

5.498min 10.114 ng/ml

response 31079329

(11) cis-Chlordane #2 (B)

6.355min 10.332 ng/ml

response 223820117