

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070323\
 Data File : PD076283.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2023 08:36
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 21:33:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
6)	B	beta-BHC	4.561f	0.000	121300	0	0.084 N.D. #
8)	B	Heptachlo...	5.696	0.000	750317	0	0.233 N.D. #
9)	A	Endosulfan I	6.107f	0.000	439109	0	0.146 N.D. #
10)	B	gamma-Chl...	5.954	0.000	291470	0	0.090 N.D. #
11)	B	alpha-Chl...	6.018f	0.000	777226	0	0.240 N.D. #
15)	B	Endosulfa...	6.839f	0.000	216677	0	0.084 N.D. #
21)	B	Endrin ke...	7.638f	0.000	100787	0	0.036 N.D. #
22)		Mirex	8.163f	0.000	310380	0	0.145 N.D. #
25)		Chlordane-3	5.954	0.000	291470	0	0.561 N.D. #
26)		Chlordane-4	6.018f	0.000	777226	0	1.233 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070323\
Data File : PD076283.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2023 08:36
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 21:33:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

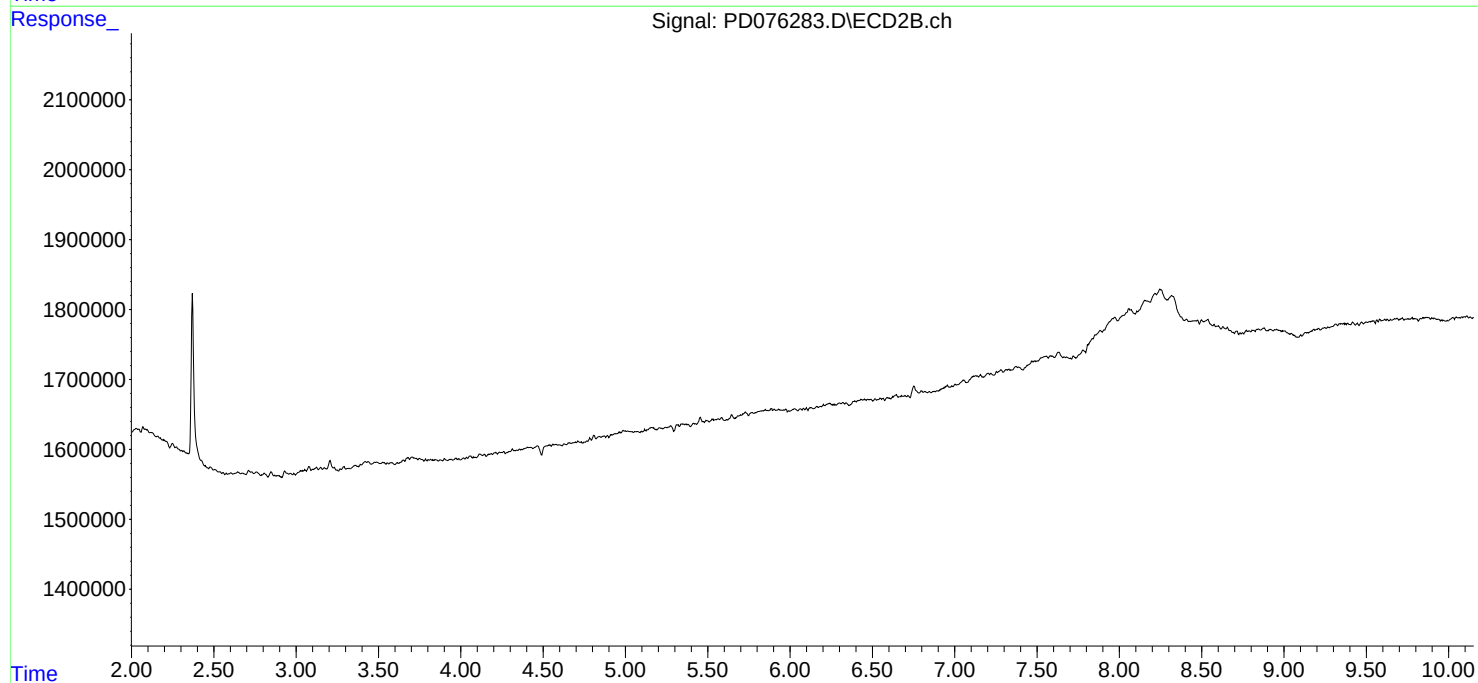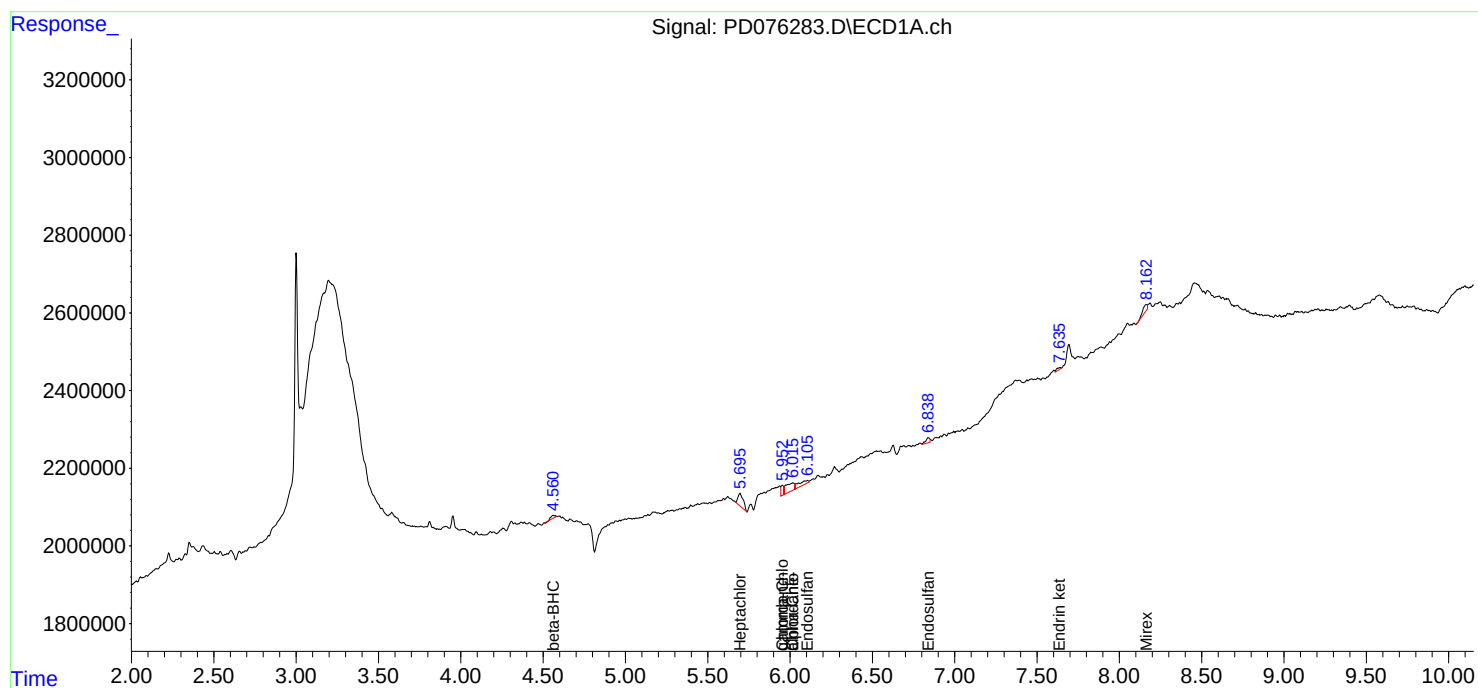


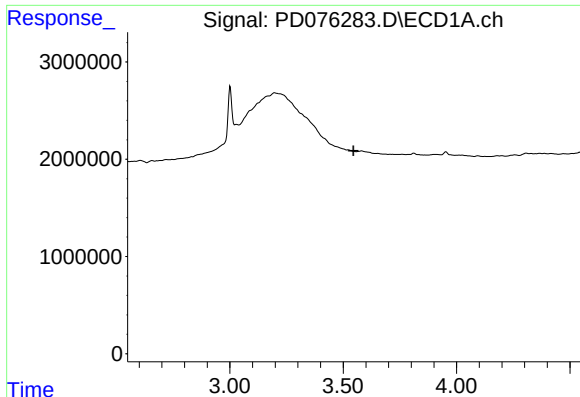

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.546 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

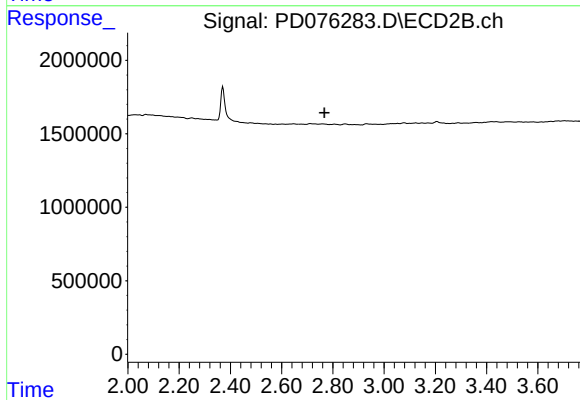


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.767 min
Response: 0
Conc: N.D.

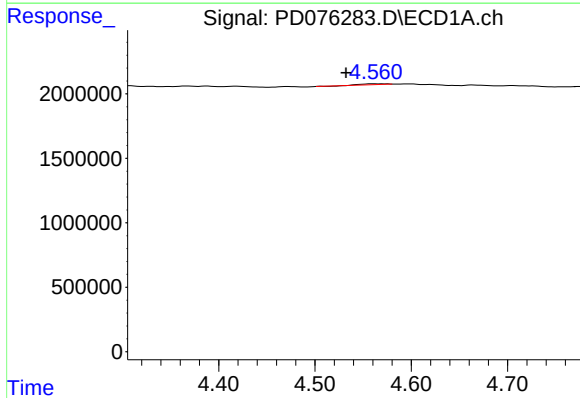


#6 beta-BHC

R.T.: 4.561 min
Delta R.T.: 0.029 min
Response: 121300
Conc: 0.08 ng/ml

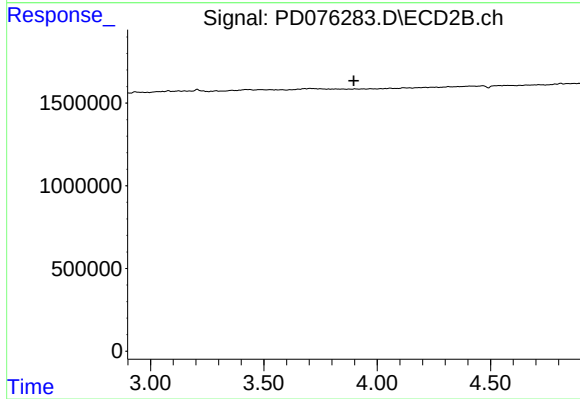

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 3.896 min
Response: 0
Conc: N.D.

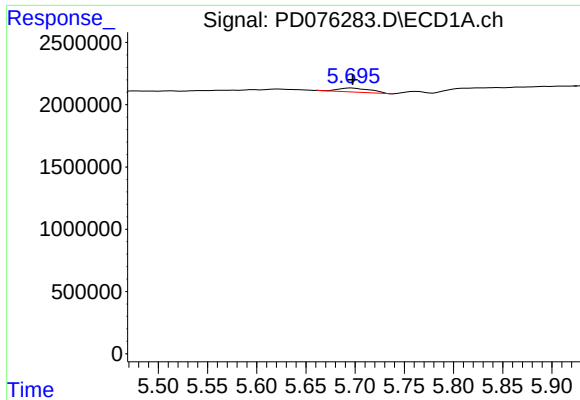

#8 Heptachlor epoxide


R.T.: 5.696 min
Delta R.T.: -0.001 min
Response: 750317
Conc: 0.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

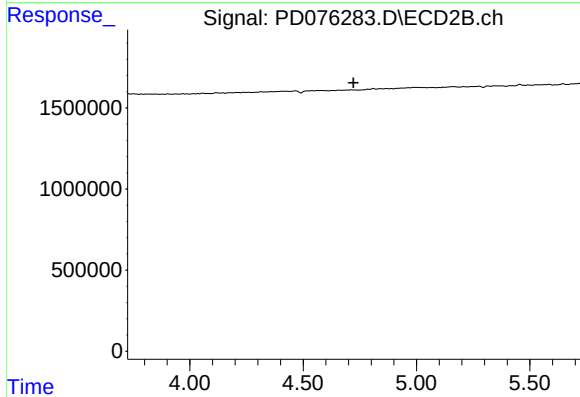


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.723 min
Response: 0
Conc: N.D.

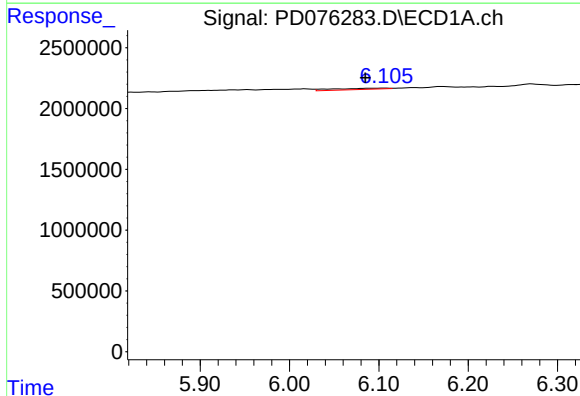


#9 Endosulfan I

R.T.: 6.107 min
Delta R.T.: 0.022 min
Response: 439109
Conc: 0.15 ng/ml

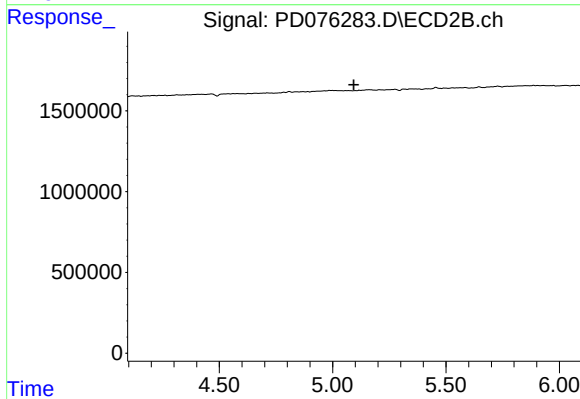

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.093 min
Response: 0
Conc: N.D.

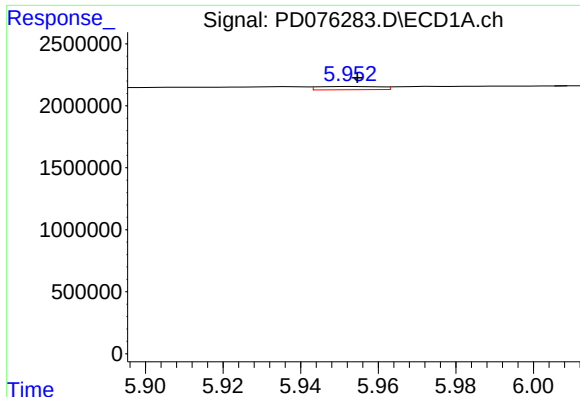

#10 gamma-Chlordane


R.T.: 5.954 min
Delta R.T.: 0.000 min
Response: 291470
Conc: 0.09 ng/ml

Instrument :
ECD_D
ClientSampleId :

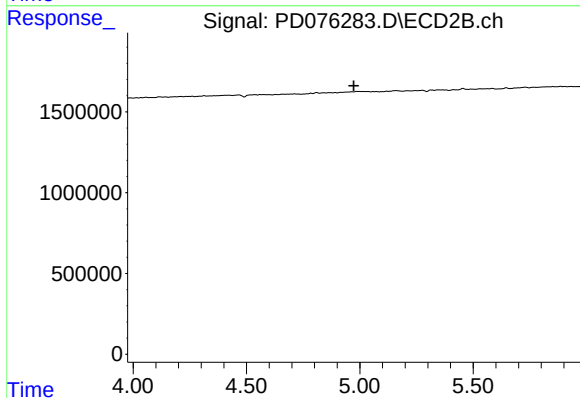


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

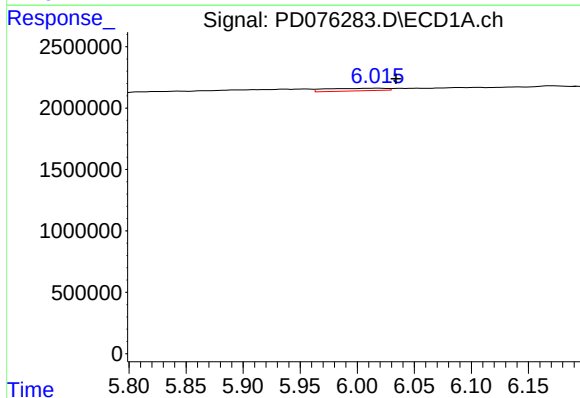


#11 alpha-Chlordane

R.T.: 6.018 min
Delta R.T.: -0.016 min
Response: 777226
Conc: 0.24 ng/ml

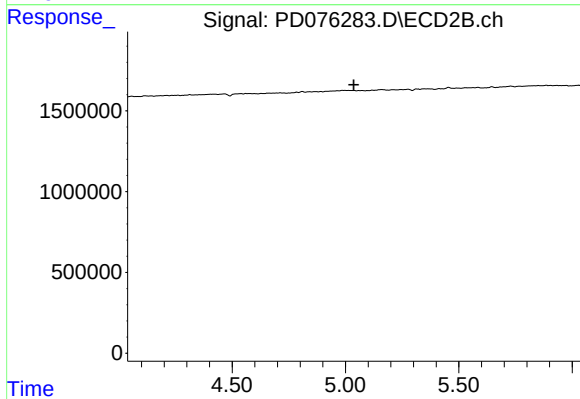

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

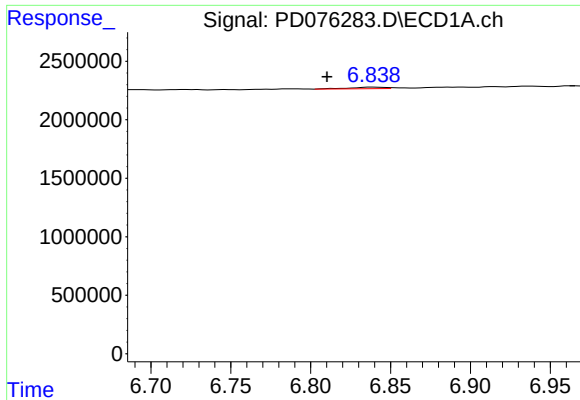

#15 Endosulfan II


R.T.: 6.839 min
Delta R.T.: 0.029 min
Response: 216677
Conc: 0.08 ng/ml

Instrument :
ECD_D
ClientSampleId :

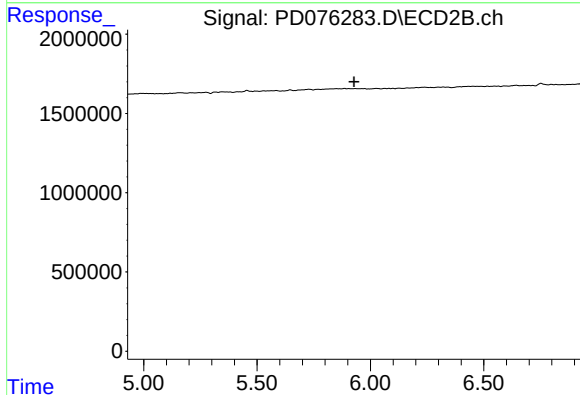


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

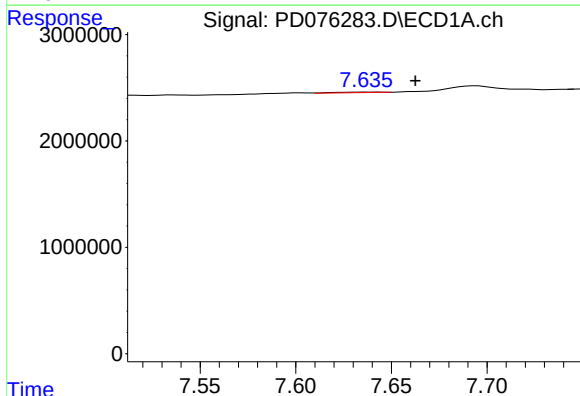


#21 Endrin ketone

R.T.: 7.638 min
Delta R.T.: -0.024 min
Response: 100787
Conc: 0.04 ng/ml

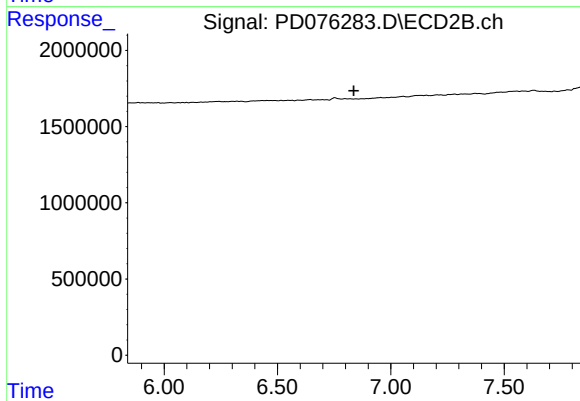

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

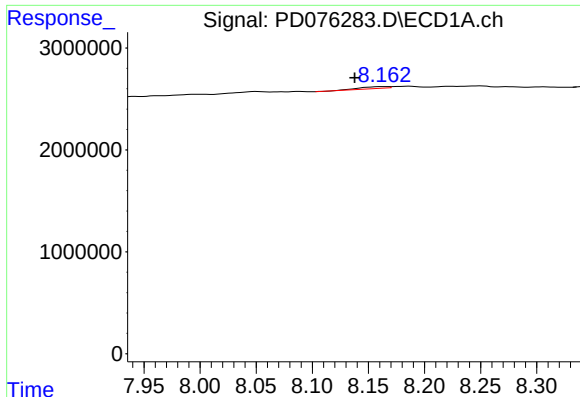

#22 Mirex


R.T.: 8.163 min
Delta R.T.: 0.026 min
Response: 310380
Conc: 0.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

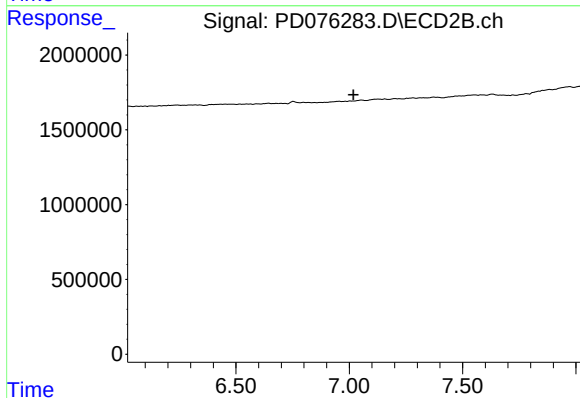


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.019 min
Response: 0
Conc: N.D.

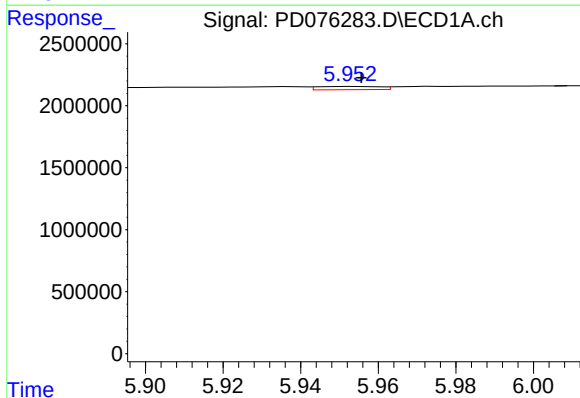


#25 Chlordane-3

R.T.: 5.954 min
Delta R.T.: -0.002 min
Response: 291470
Conc: 0.56 ng/ml

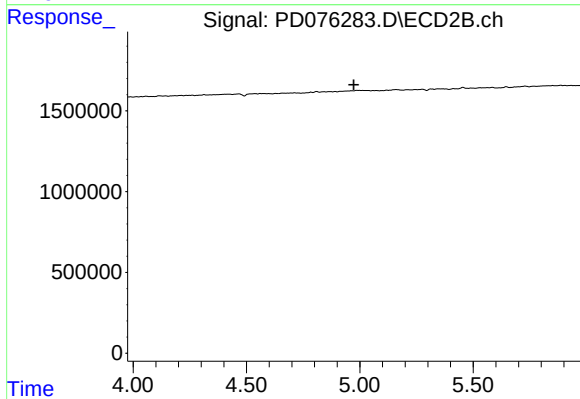

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 4.974 min
Response: 0
Conc: N.D.

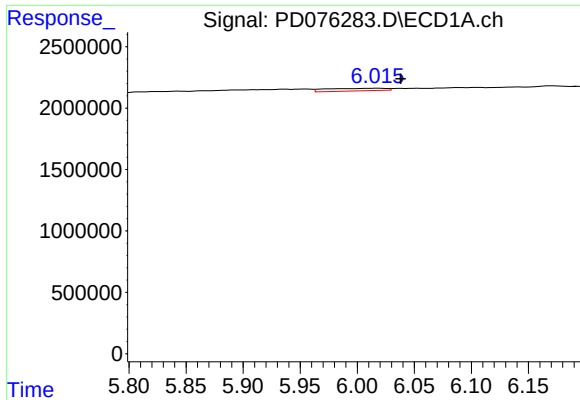

#26 Chlordane-4


R.T.: 6.018 min
Delta R.T.: -0.020 min
Response: 777226
Conc: 1.23 ng/ml

Instrument :
ECD_D
ClientSampleId :

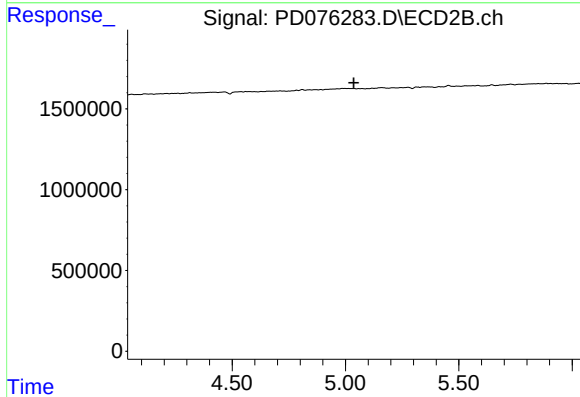


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

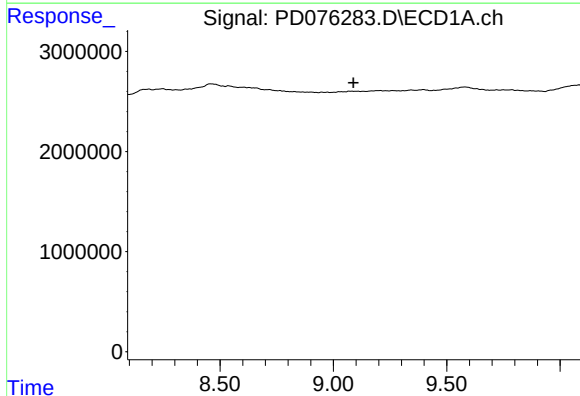

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.089 min
Response: 0
Conc: N.D.

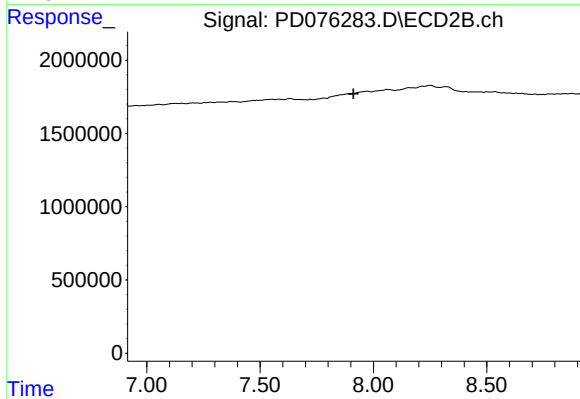

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.913 min
Response: 0
Conc: N.D.