

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070323\
 Data File : PD076287.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2023 11:34
 Operator : AR\AJ
 Sample : PB153944BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 21:37:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.766	42901770	21554413	20.140	19.867
28)	SA Decachlor...	9.100	7.916	49997911	21141701	19.736	21.622
Target Compounds							
4)	MA Heptachlor	4.953f	0.000	315437	0	0.088	N.D. #
7)	B delta-BHC	4.783	0.000	2226377	0	0.670	N.D. #
10)	B gamma-Chl...	5.942	0.000	800753	0	0.249	N.D. #
11)	B alpha-Chl...	6.036	0.000	139496	0	0.043	N.D. #
15)	B Endosulfa...	6.793f	0.000	264592	0	0.102	N.D. #
21)	B Endrin ke...	7.643f	0.000	4111414	0	1.476	N.D. #
25)	Chlordane-3	5.942	0.000	800753	0	1.542	N.D. #
26)	Chlordane-4	6.036	0.000	139496	0	0.221	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070323\
Data File : PD076287.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2023 11:34
Operator : AR\AJ
Sample : PB153944BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 21:37:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

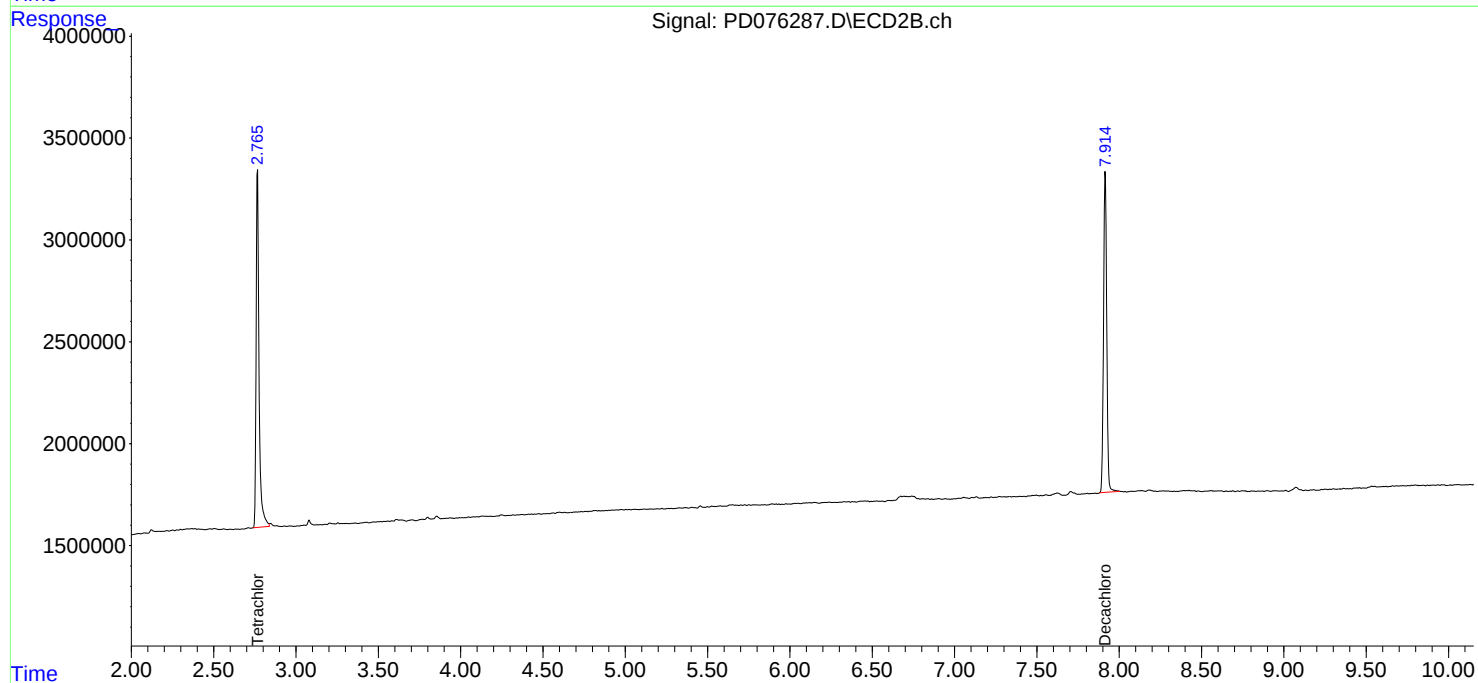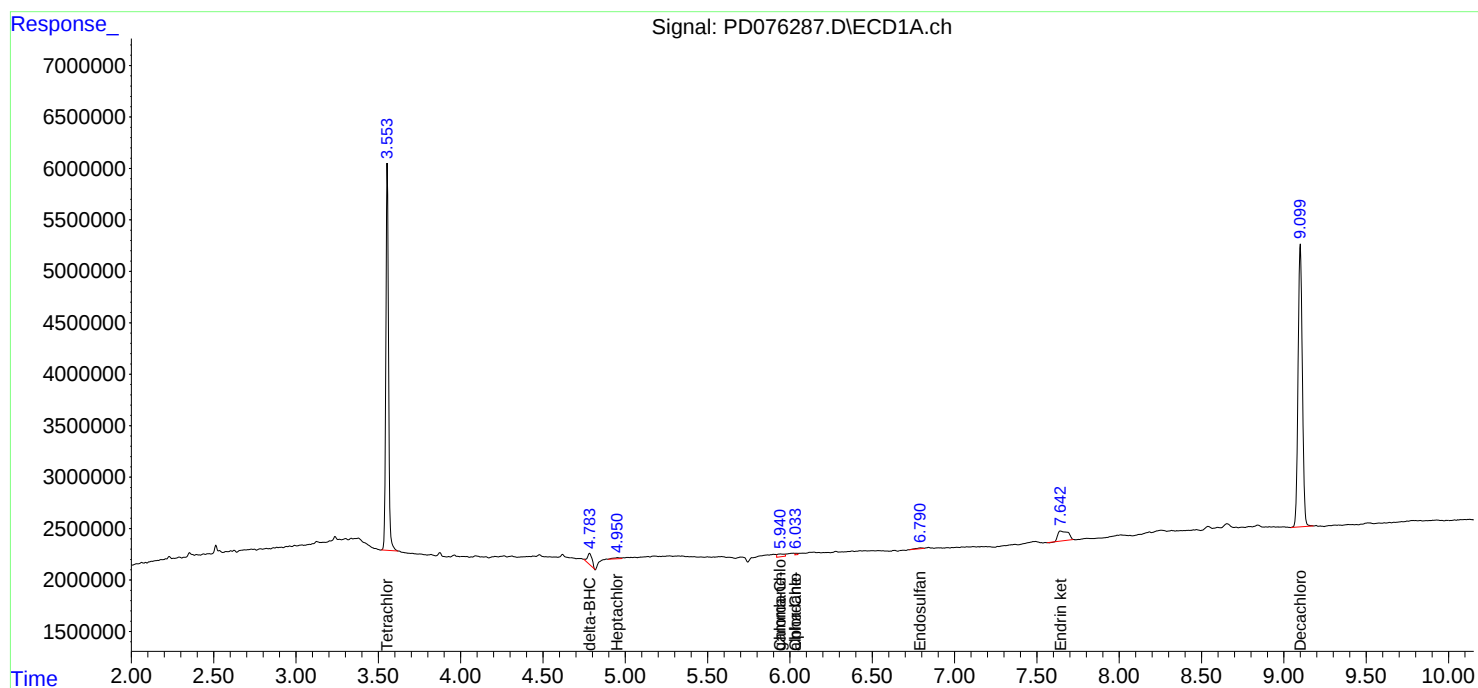


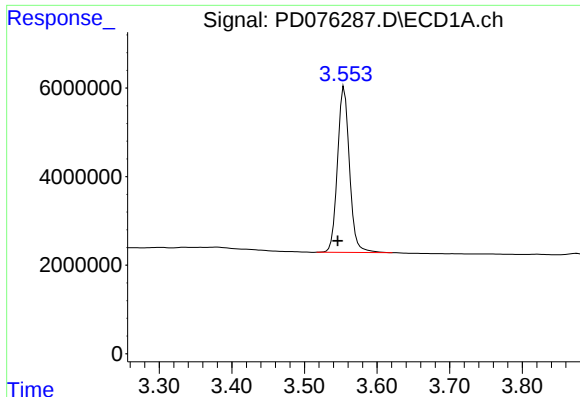

#1 Tetrachloro-m-xylene


R.T.: 3.555 min
Delta R.T.: 0.009 min
Response: 42901770
Conc: 20.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

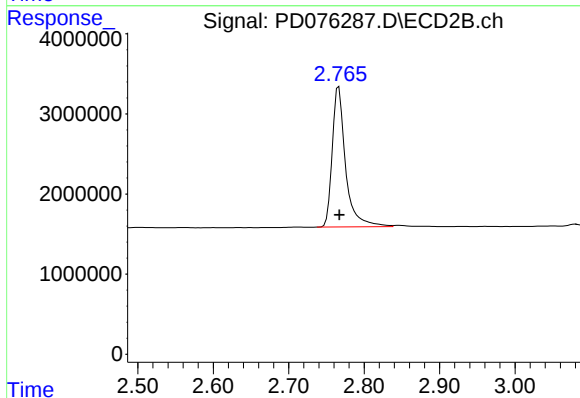


#1 Tetrachloro-m-xylene

R.T.: 2.766 min
Delta R.T.: 0.000 min
Response: 21554413
Conc: 19.87 ng/ml

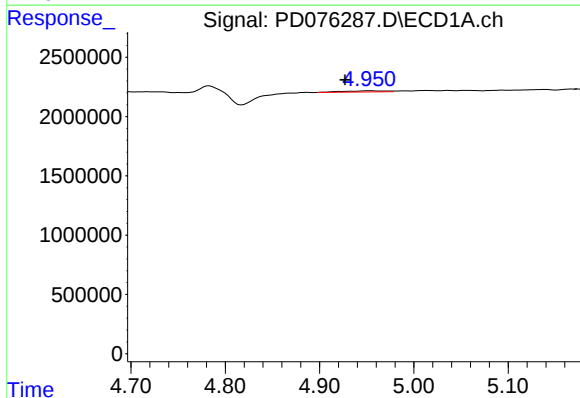


#4 Heptachlor

R.T.: 4.953 min
Delta R.T.: 0.026 min
Response: 315437
Conc: 0.09 ng/ml

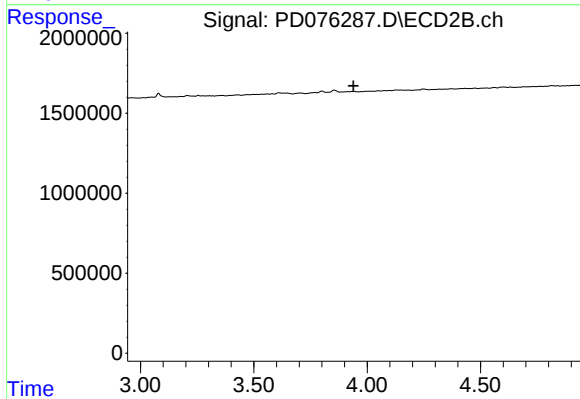

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 3.940 min
Response: 0
Conc: N.D.

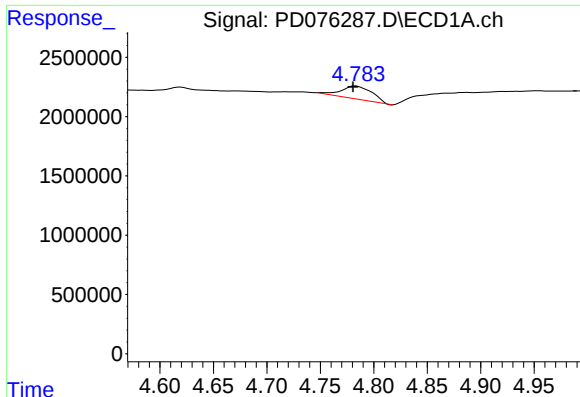

#7 delta-BHC


R.T.: 4.783 min
Delta R.T.: 0.002 min
Response: 2226377
Conc: 0.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

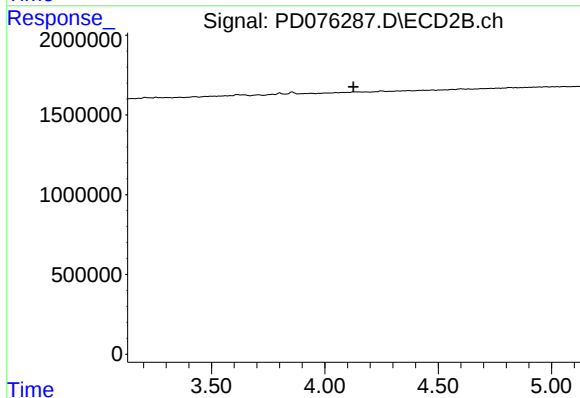


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.127 min
Response: 0
Conc: N.D.

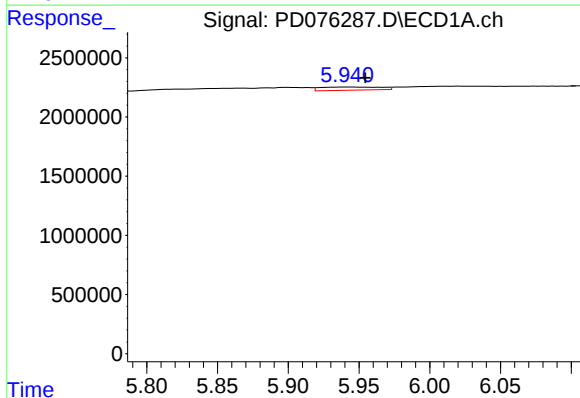


#10 gamma-Chlordane

R.T.: 5.942 min
Delta R.T.: -0.013 min
Response: 800753
Conc: 0.25 ng/ml

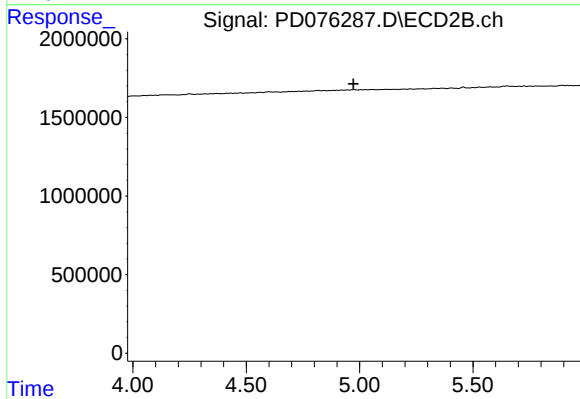

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

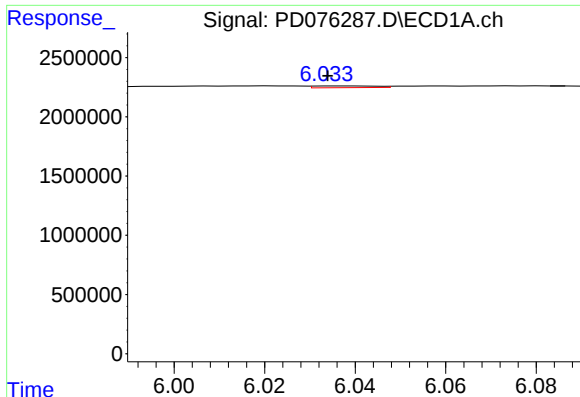

#11 alpha-Chlordane


R.T.: 6.036 min
Delta R.T.: 0.002 min
Response: 139496
Conc: 0.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

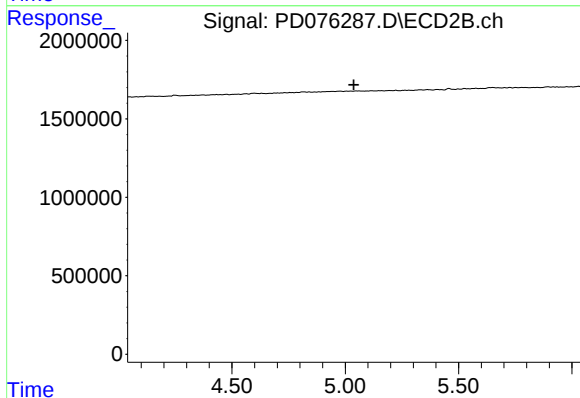


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

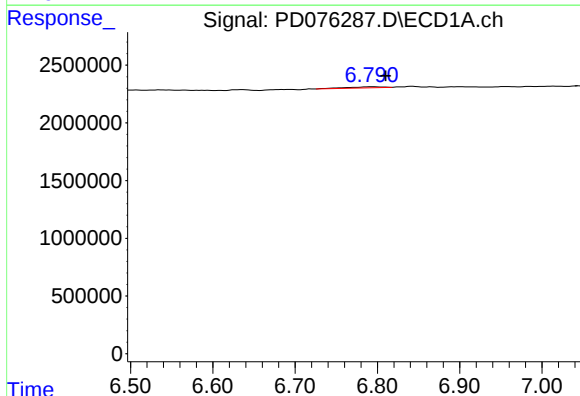


#15 Endosulfan II

R.T.: 6.793 min
Delta R.T.: -0.017 min
Response: 264592
Conc: 0.10 ng/ml

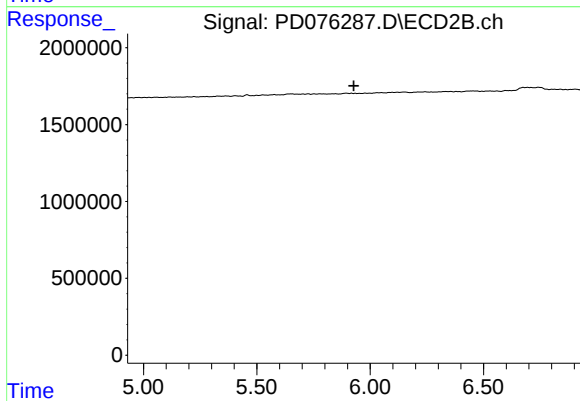

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

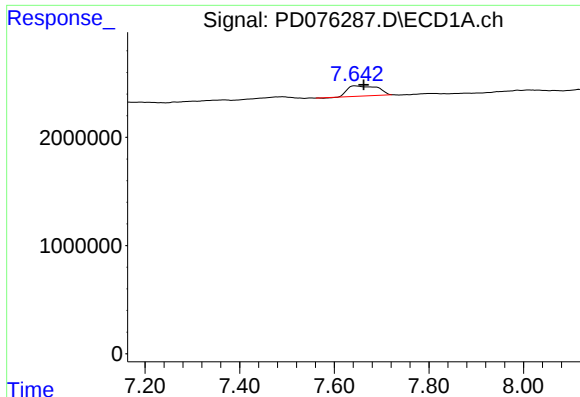

#21 Endrin ketone


R.T.: 7.643 min
Delta R.T.: -0.019 min
Response: 4111414
Conc: 1.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

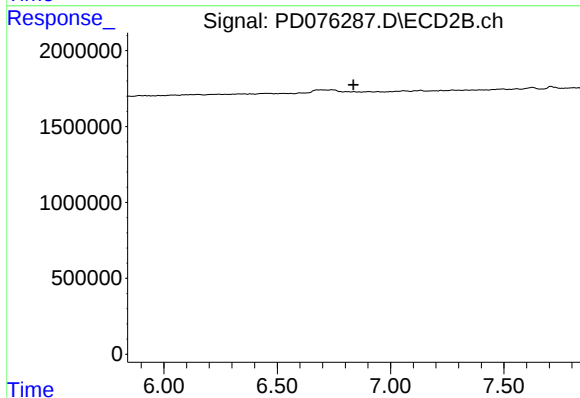


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.837 min
Response: 0
Conc: N.D.

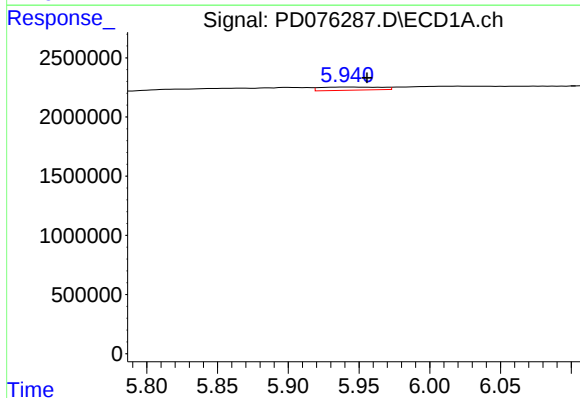


#25 Chlordane-3

R.T.: 5.942 min
Delta R.T.: -0.014 min
Response: 800753
Conc: 1.54 ng/ml

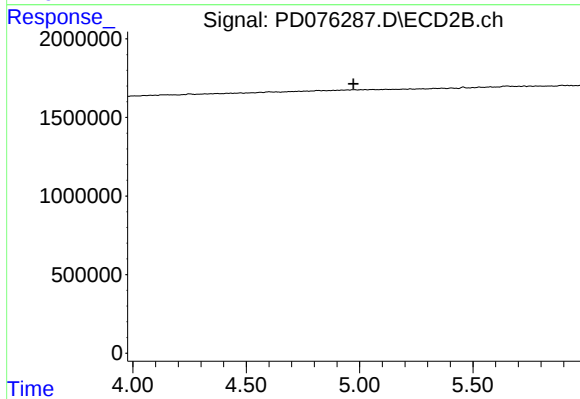

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 4.974 min
Response: 0
Conc: N.D.

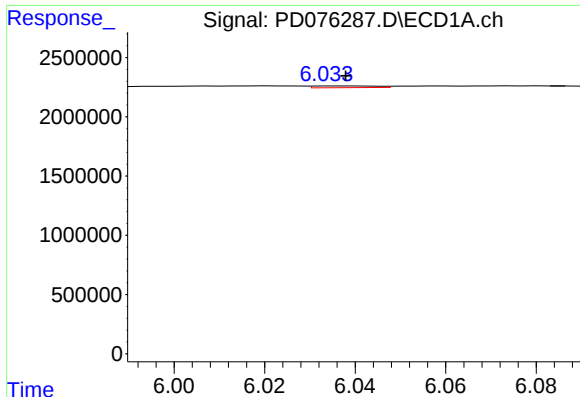

#26 Chlordane-4


R.T.: 6.036 min
Delta R.T.: -0.002 min
Response: 139496
Conc: 0.22 ng/ml

Instrument :
ECD_D
ClientSampleId :

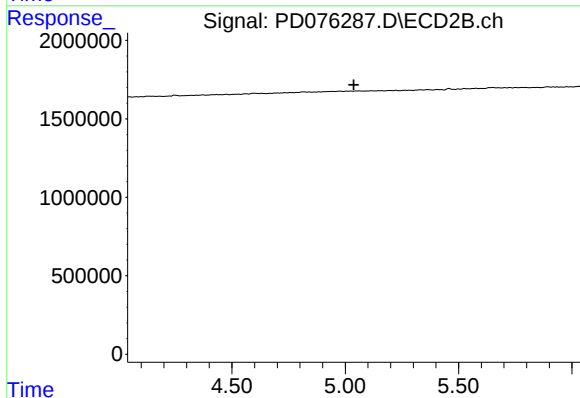


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.037 min
Response: 0
Conc: N.D.

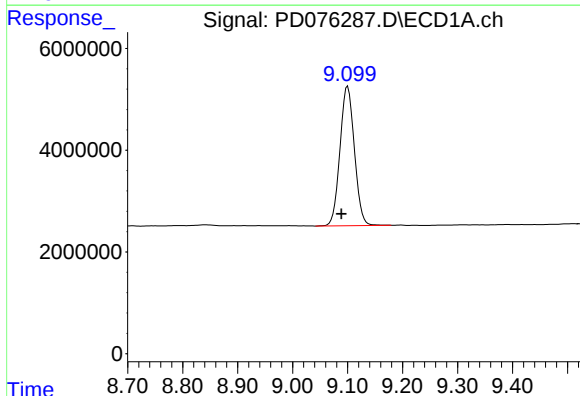

#28 Decachlorobiphenyl

R.T.: 9.100 min
Delta R.T.: 0.011 min
Response: 49997911
Conc: 19.74 ng/ml

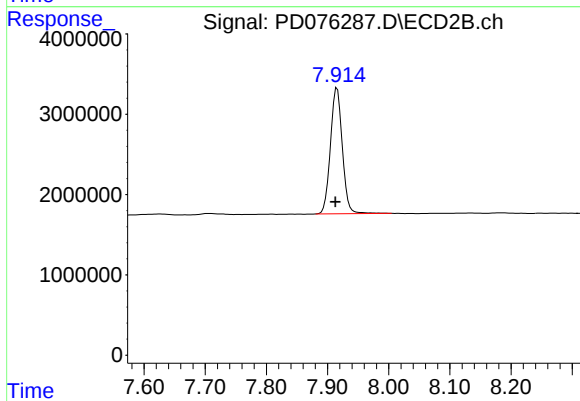

#28 Decachlorobiphenyl

R.T.: 7.916 min
Delta R.T.: 0.003 min
Response: 21141701
Conc: 21.62 ng/ml