

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070323\
 Data File : PD076297.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2023 13:53
 Operator : AR\AJ
 Sample : 03497-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 OK-2-063023

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/04/2023
 Supervised By : Ankita Jodhani 07/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 21:45:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
 Quant Title : GC Extractables
 QLast Update : Fri Jun 16 10:43:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.766	13577600	7726598	6.374m	7.122
28)	SA Decachlor...	9.090	7.911	21693961	8423540	8.563	8.615m
Target Compounds							
11)	B alpha-Chl...	6.035	5.035	3772964	985513	1.167m	0.718m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD070323\
Data File : PD076297.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2023 13:53
Operator : AR\AJ
Sample : 03497-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
OK-2-063023


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 07/04/2023
Supervised By : Ankita Jodhani 07/05/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 21:45:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD061523.M
Quant Title : GC Extractables
QLast Update : Fri Jun 16 10:43:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

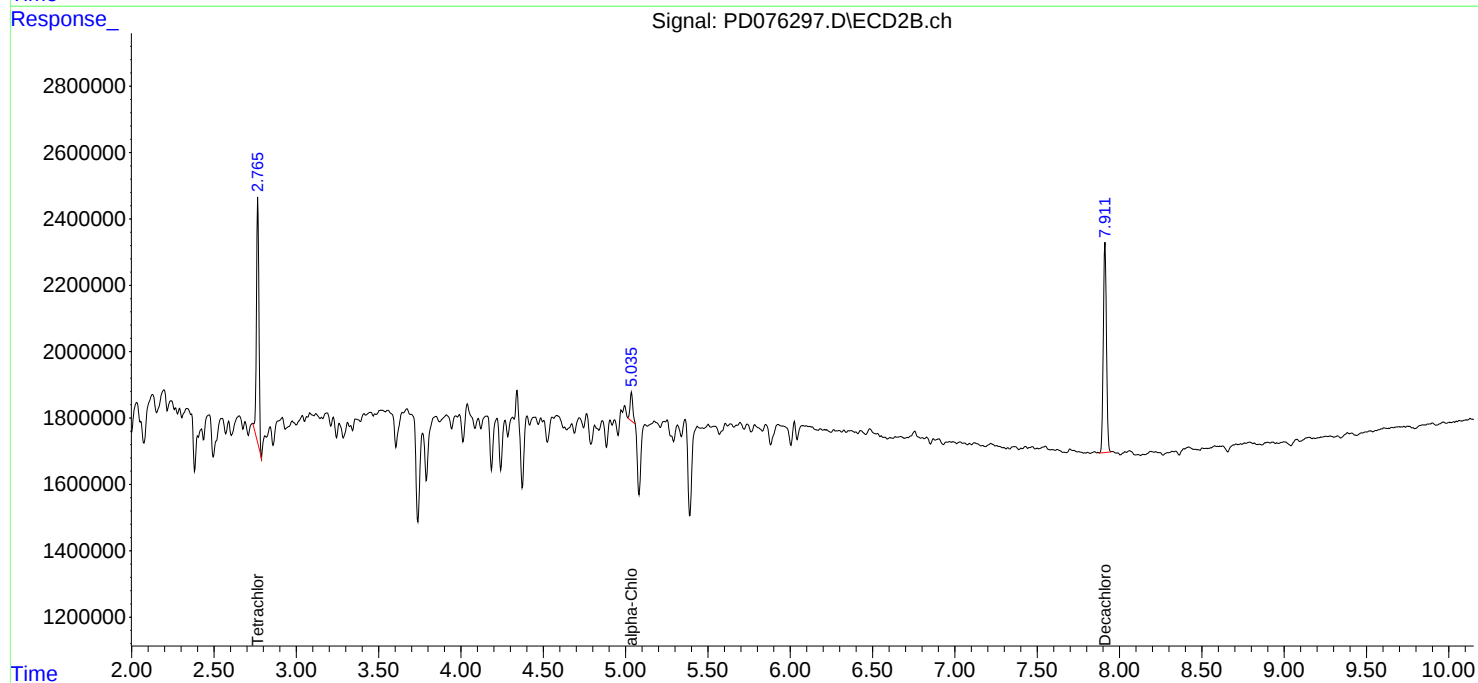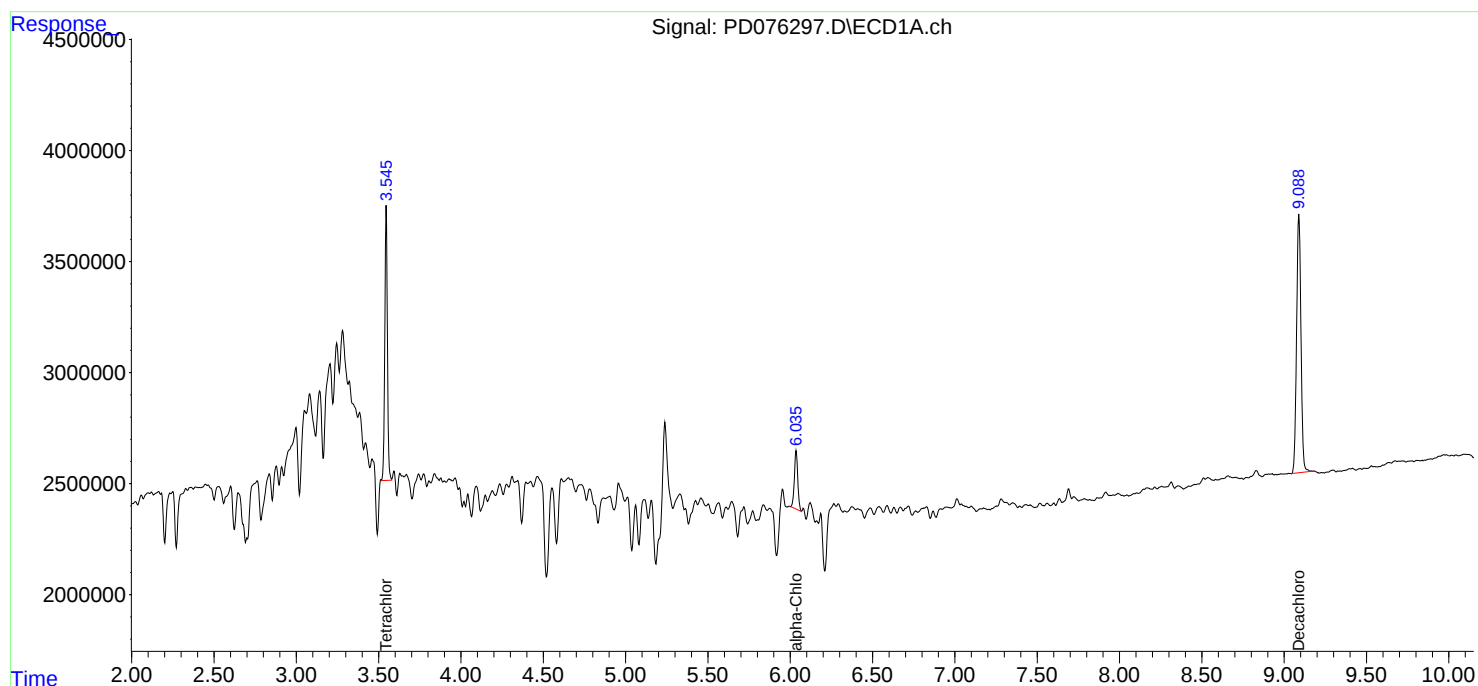

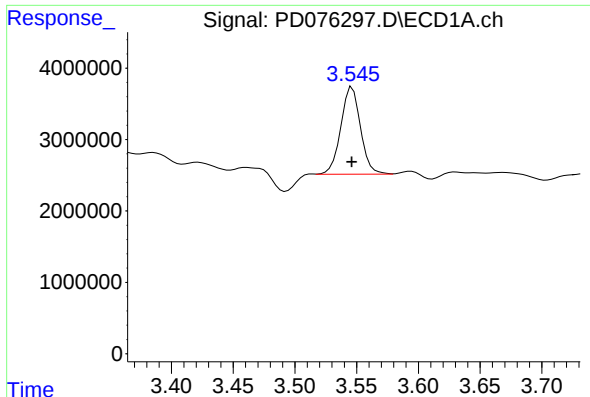


#1 Tetrachloro-m-xylene

R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 13577600
Conc: 6.37 ng/ml

Instrument :
ECD_D
ClientSampleId :
OK-2-063023


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/04/2023
Supervised By :Ankita Jodhani 07/05/2023

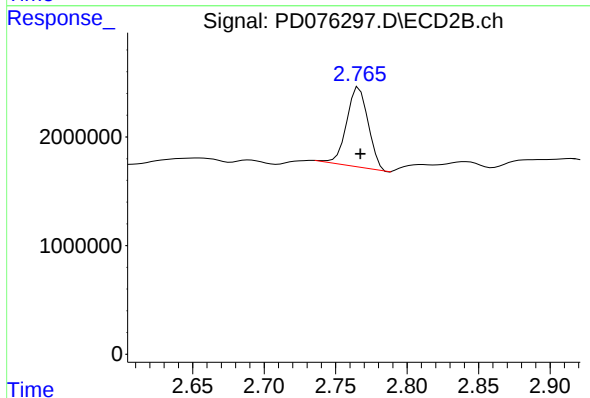


#1 Tetrachloro-m-xylene

R.T.: 2.766 min
Delta R.T.: 0.000 min
Response: 7726598
Conc: 7.12 ng/ml

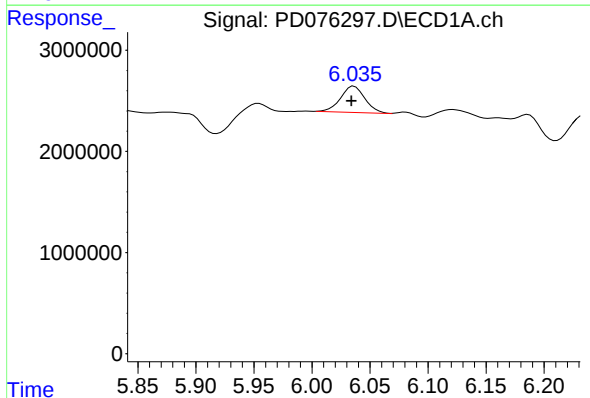


#11 alpha-Chlordane

R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 3772964
Conc: 1.17 ng/ml m

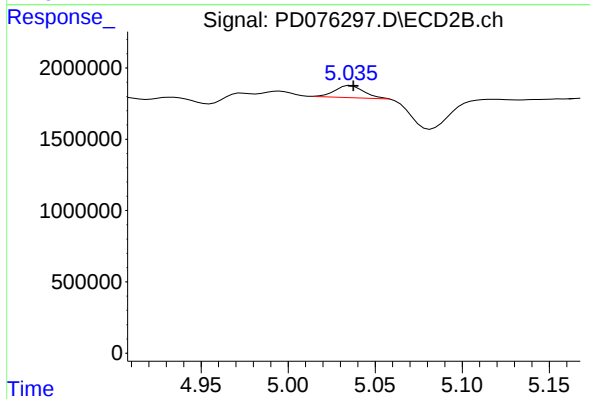

#11 alpha-Chlordane

R.T.: 5.035 min
Delta R.T.: -0.003 min
Response: 985513
Conc: 0.72 ng/ml m

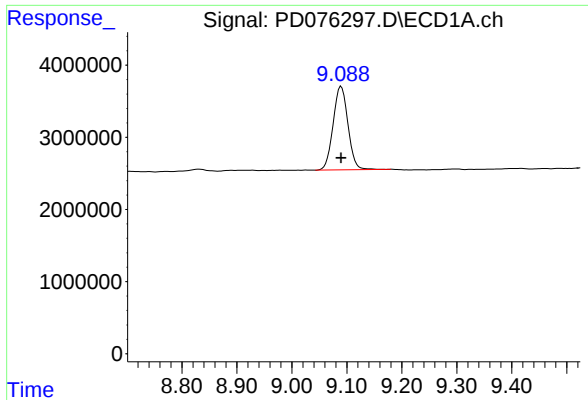


#28 Decachlorobiphenyl

R.T.: 9.090 min
Delta R.T.: 0.000 min
Response: 21693961
Conc: 8.56 ng/ml

Instrument :
ECD_D
ClientSampleId :
OK-2-063023

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 07/04/2023
Supervised By :Ankita Jodhani 07/05/2023

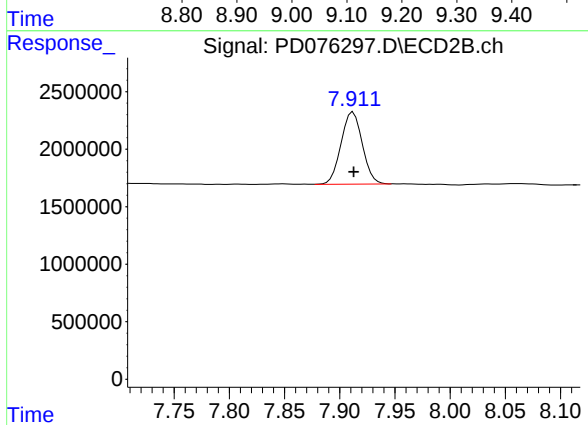

#28 Decachlorobiphenyl

R.T.: 7.911 min
Delta R.T.: -0.002 min
Response: 8423540
Conc: 8.61 ng/ml m