

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071223\
Data File : PD076568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2023 13:34
Operator : AR\AJ
Sample : 03552-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 20:41:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 14:30:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds						
15) B	Endosulfa...	0.000	5.881f	0	352961	N.D. 0.318


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071223\
Data File : PD076568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2023 13:34
Operator : AR\AJ
Sample : 03552-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 12 20:41:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 14:30:19 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

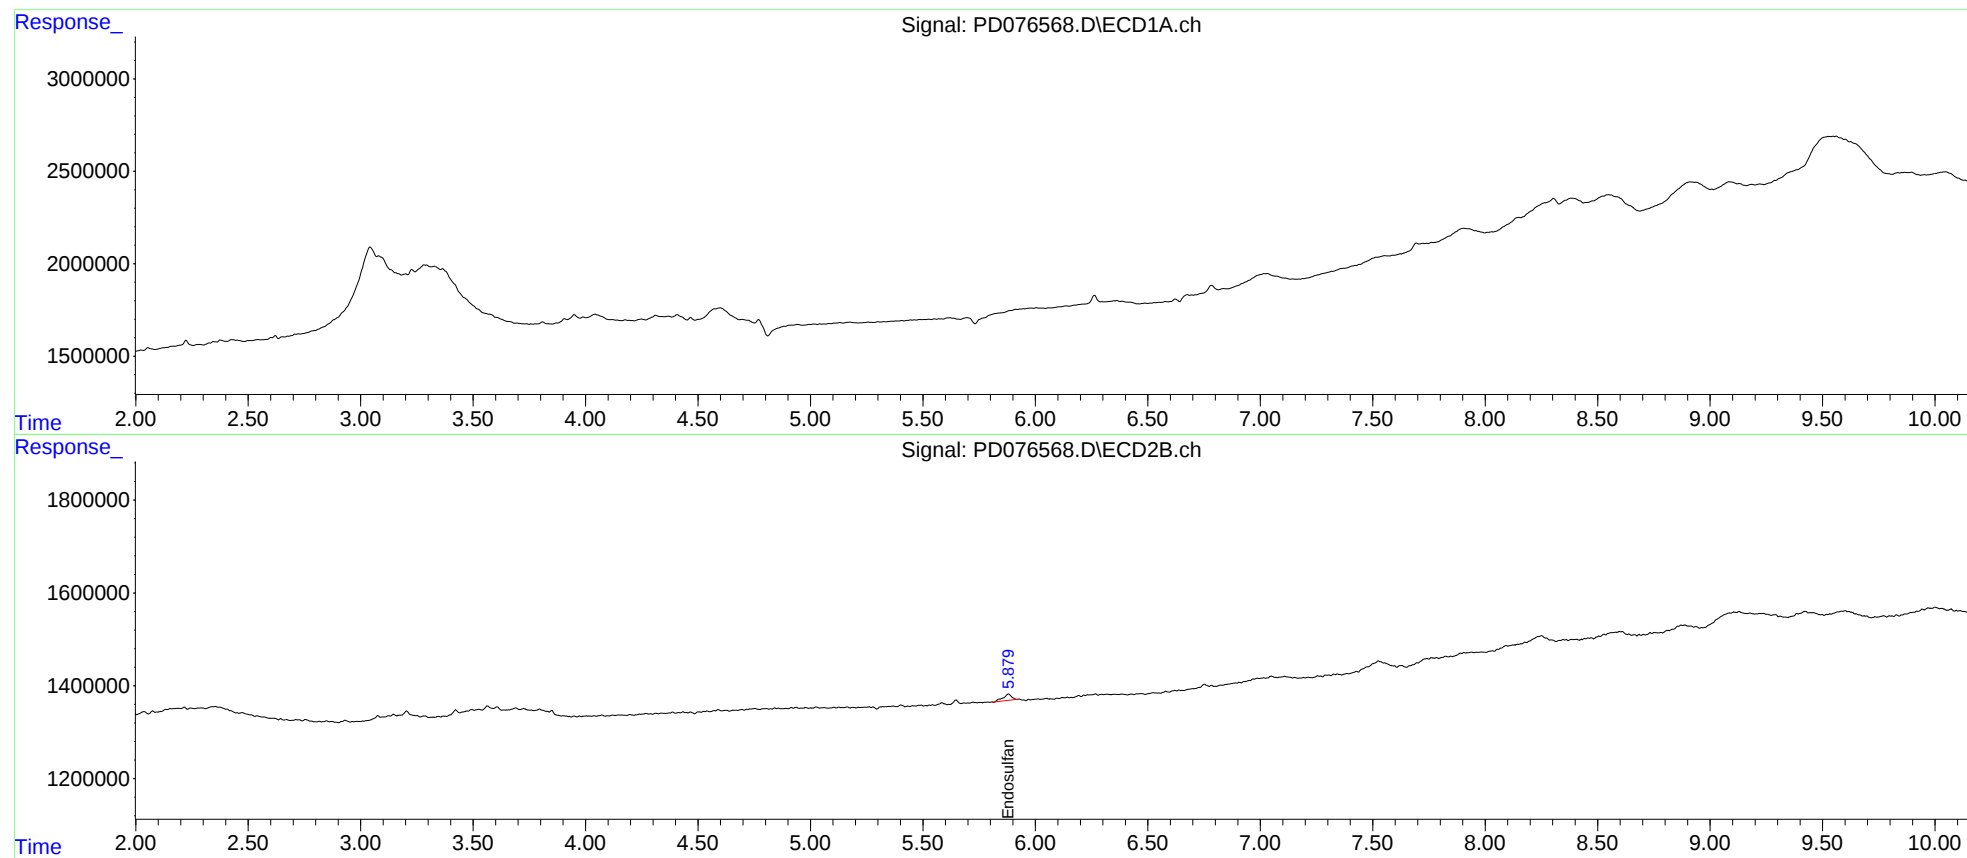

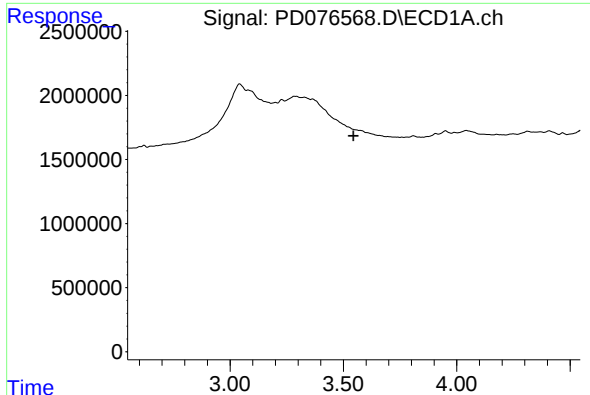


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.545 min
Response: 0
Conc: N.D.

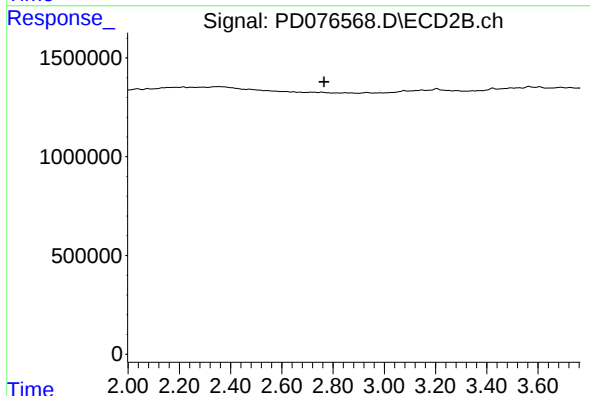


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.765 min
Response: 0
Conc: N.D.

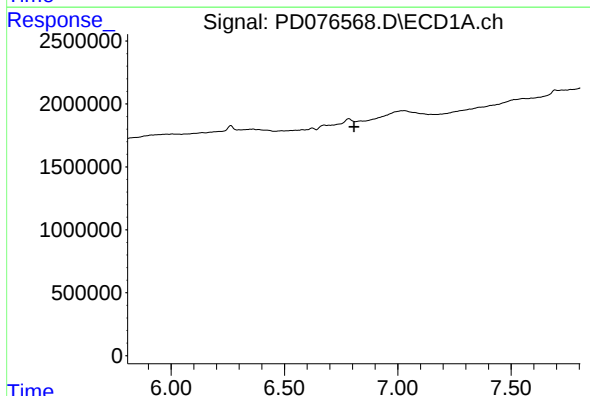


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.808 min
Response: 0
Conc: N.D.

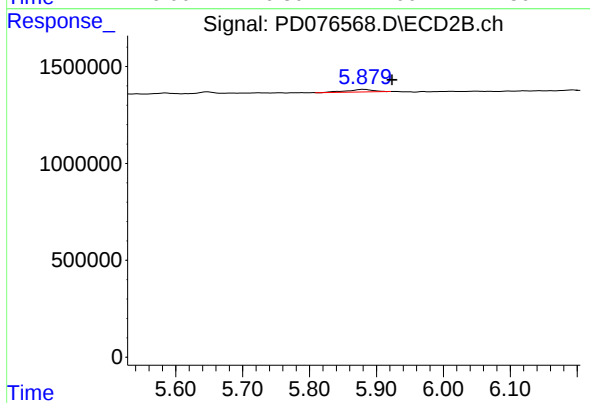


#15 Endosulfan II

R.T.: 5.881 min
Delta R.T.: -0.042 min
Response: 352961
Conc: 0.32 ng/ml

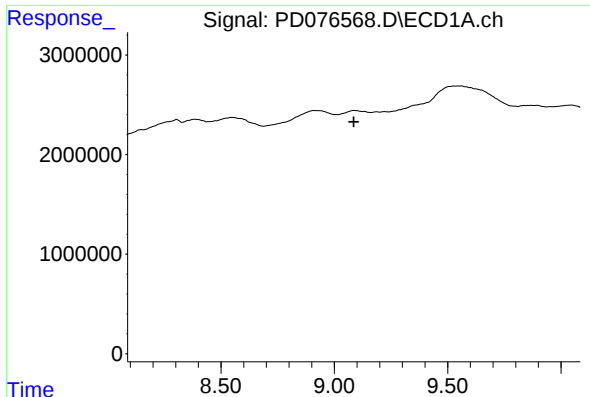

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.085 min
Response: 0
Conc: N.D.

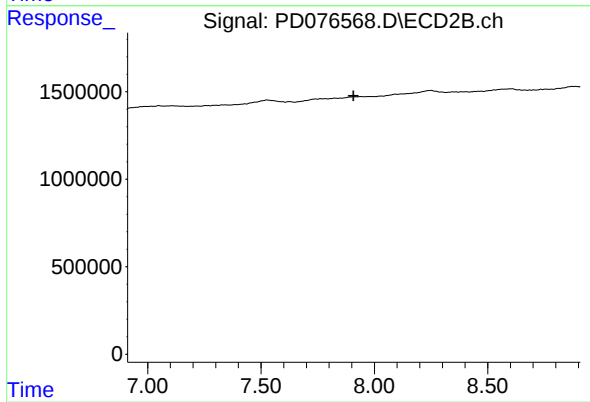

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.908 min
Response: 0
Conc: N.D.