

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071223\
 Data File : PD076578.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jul 2023 16:40
 Operator : AR\AJ
 Sample : 03418-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A46J1

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 07/14/2023
 Supervised By : Ankita Jodhani 07/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 14 02:20:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 05 14:30:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.544	2.765	21126756	9952342	9.744	9.671
27)	SA Decachlor...	9.084	7.908	37398764	15032782	14.744m	16.474
Target Compounds							
17)	MA 4,4'-DDT	7.007	6.021	3659037	1952925	1.616m	2.343 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD071223\
Data File : PD076578.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jul 2023 16:40
Operator : AR\AJ
Sample : 03418-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 14 02:20:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD070523CLP.M
Quant Title : GC Extractables
QLast Update : Wed Jul 05 14:30:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

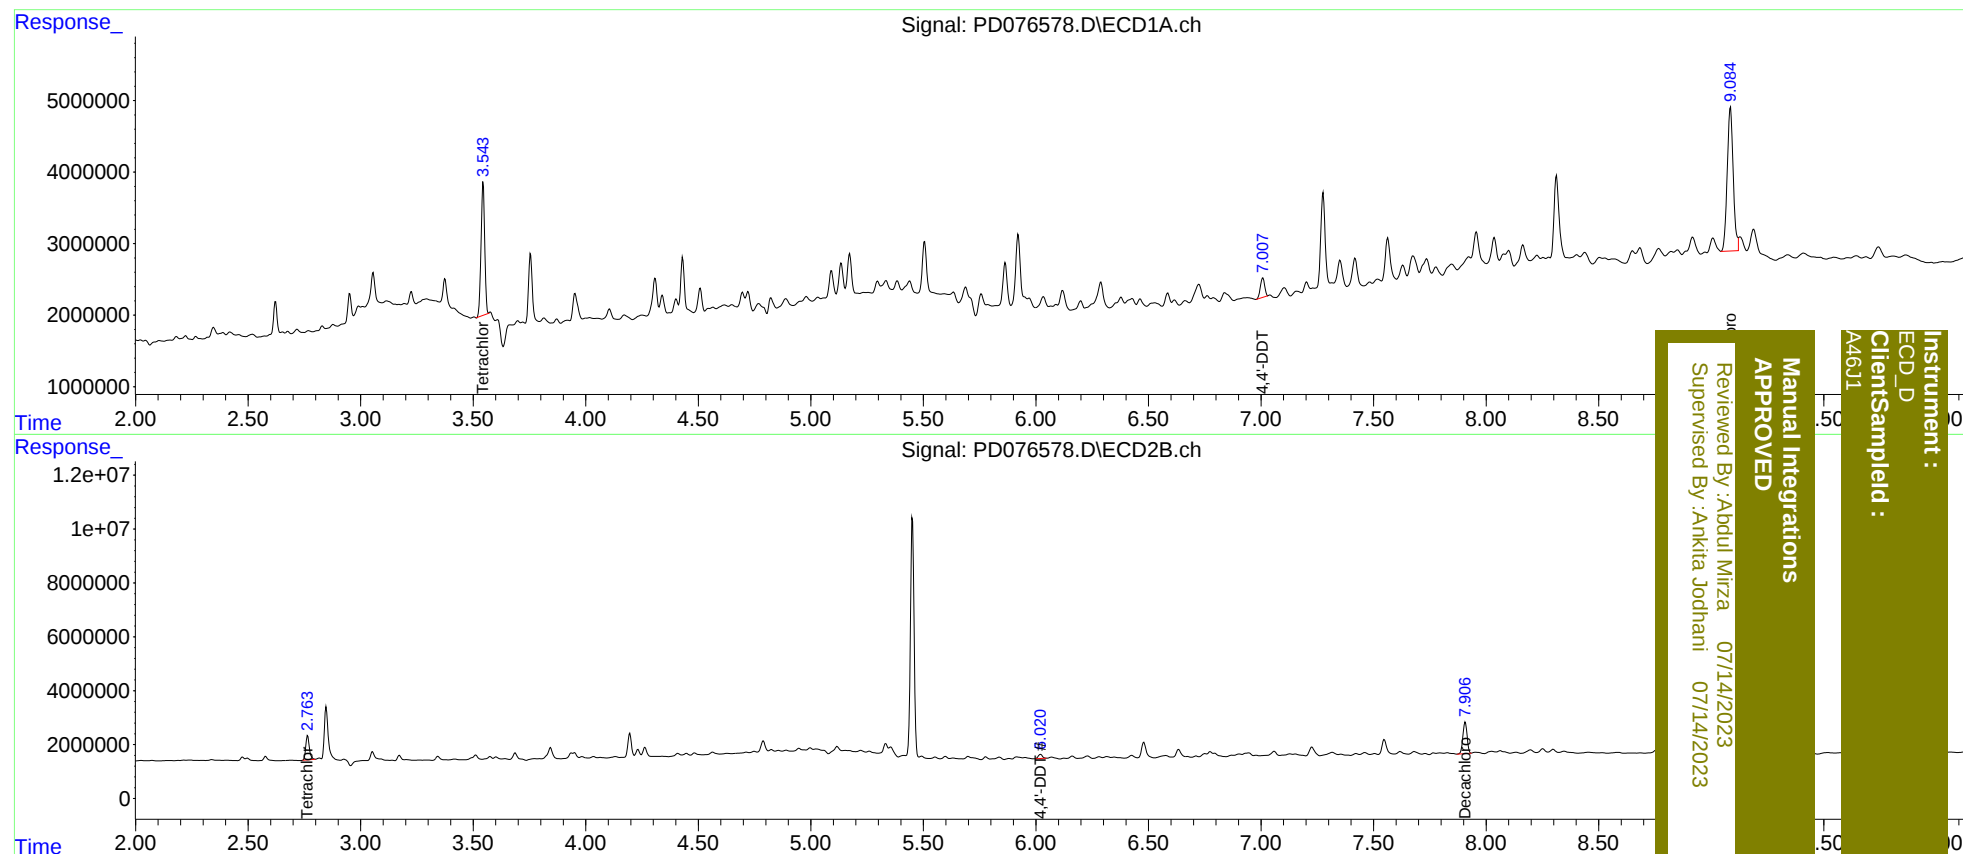

Reviewed By: Abdul Mirza 07/14/2023
Supervised By: Ankita Jodhani 07/14/2023

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
A46J1