

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081224\
 Data File : PD084294.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2024 15:01
 Operator : AR\AJ
 Sample : PB162634BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK634

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:15:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.585	2.930	17910917	109.2E6	21.364	20.742
27)	SA Decachlor...	9.117	8.143	38694486	86975800	22.247	23.145
Target Compounds							
15)	B Endosulfa...	6.803	0.000	1420778	0	0.862	N.D. #
16)	A 4,4'-DDD	6.803f	0.000	1420778	0	1.105	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081224\
Data File : PD084294.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 15:01
Operator : AR\AJ
Sample : PB162634BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 01:15:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

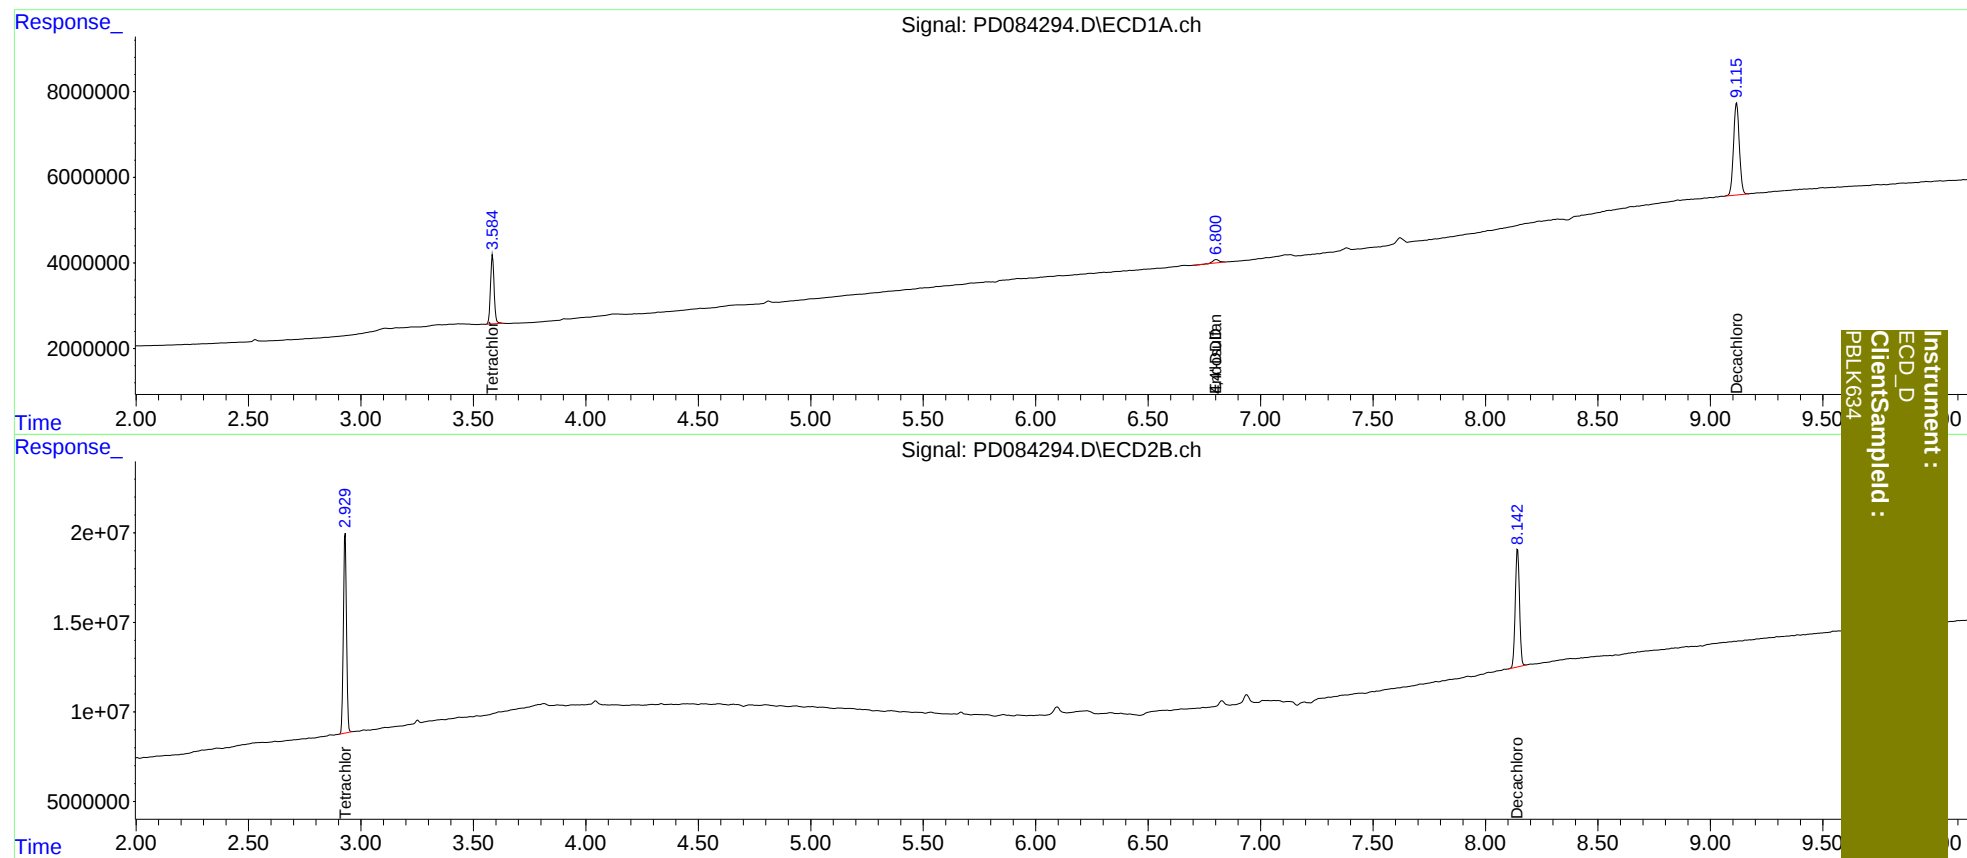


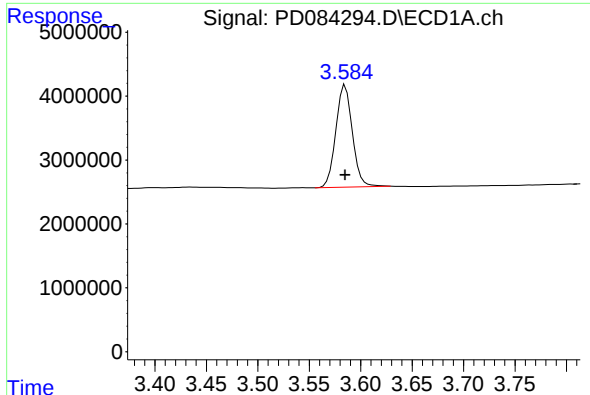

#1 Tetrachloro-m-xylene


R.T.: 3.585 min
Delta R.T.: 0.000 min
Response: 17910917
Conc: 21.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK634

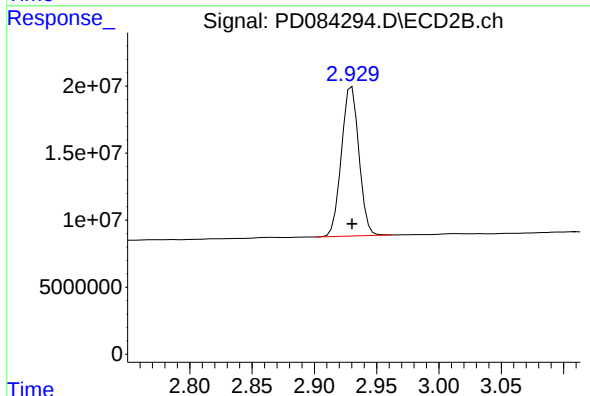


#1 Tetrachloro-m-xylene

R.T.: 2.930 min
Delta R.T.: 0.000 min
Response: 109191186
Conc: 20.74 ng/ml

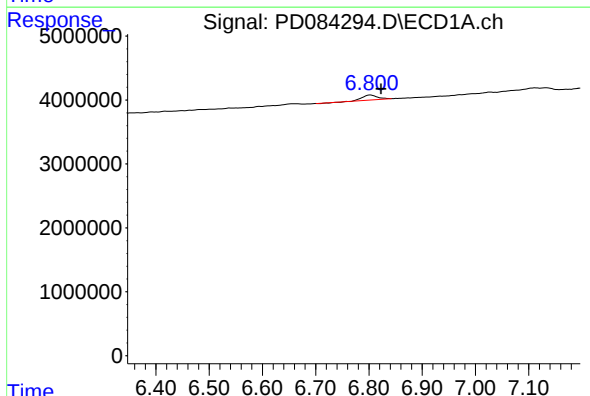


#15 Endosulfan II

R.T.: 6.803 min
Delta R.T.: -0.020 min
Response: 1420778
Conc: 0.86 ng/ml

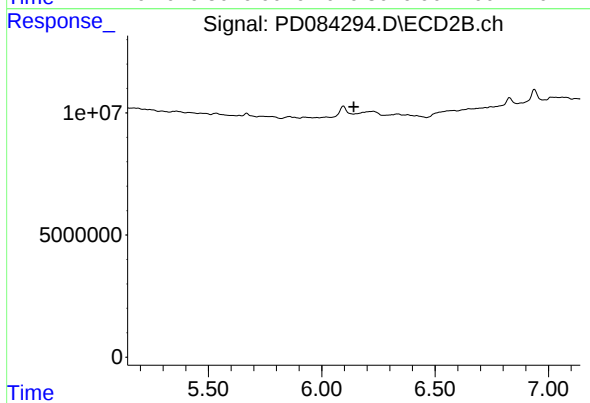

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.142 min
Response: 0
Conc: N.D.

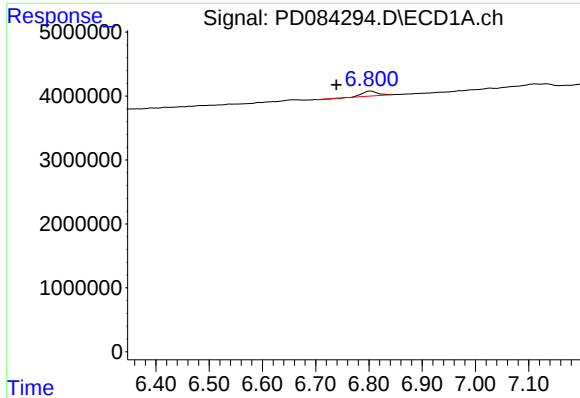

#16 4,4'-DDD


R.T.: 6.803 min
Delta R.T.: 0.064 min
Response: 1420778
Conc: 1.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK634

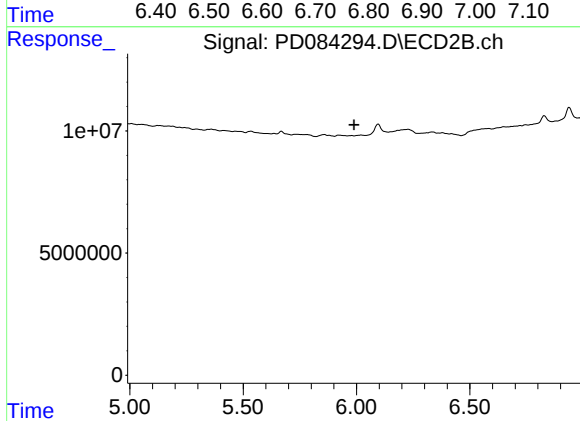


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.990 min
Response: 0
Conc: N.D.

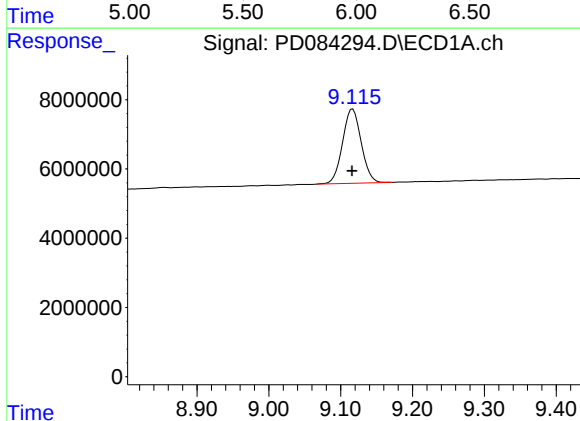

#27 Decachlorobiphenyl

R.T.: 9.117 min
Delta R.T.: 0.000 min
Response: 38694486
Conc: 22.25 ng/ml

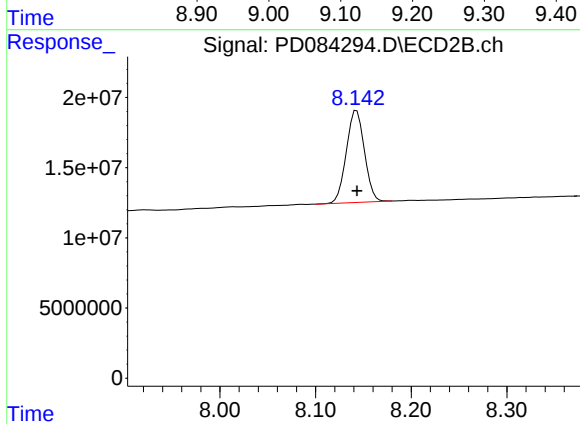

#27 Decachlorobiphenyl

R.T.: 8.143 min
Delta R.T.: 0.000 min
Response: 86975800
Conc: 23.14 ng/ml