

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081224\
 Data File : PD084328.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2024 22:35
 Operator : AR\AJ
 Sample : PB162607BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:08:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.585	2.930	16094467	100.3E6	19.197	19.061
27)	SA Decachlor...	9.116	8.142	37361879	70398334	21.481	18.733
Target Compounds							
6)	B beta-BHC	0.000	4.045f	0	9006958	N.D.	2.504
7)	B delta-BHC	4.813	0.000	1283131	0	0.743	N.D. #
9)	A Endosulfan I	6.111	0.000	604553	0	0.380	N.D. #
11)	B cis-Chlor...	6.111f	0.000	604553	0	0.351	N.D. #
12)	B 4,4'-DDE	6.245	0.000	454663	0	0.260	N.D. #
13)	MA Dieldrin	6.396	0.000	558275	0	0.311	N.D. #
17)	MA 4,4'-DDT	7.104f	0.000	3505794	0	2.586	N.D. #
19)	B Endosulfa...	7.123f	0.000	2084879	0	1.373	N.D. #
24)	Toxaphene-3	7.104	0.000	3505794	0	77.021	N.D. #
25)	Toxaphene-4	7.123f	0.000	2084879	0	62.142	N.D. #
26)	Toxaphene-5	0.000	7.439f	0	58088318	N.D.	1059.257


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081224\
Data File : PD084328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 22:35
Operator : AR\AJ
Sample : PB162607BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 01:08:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

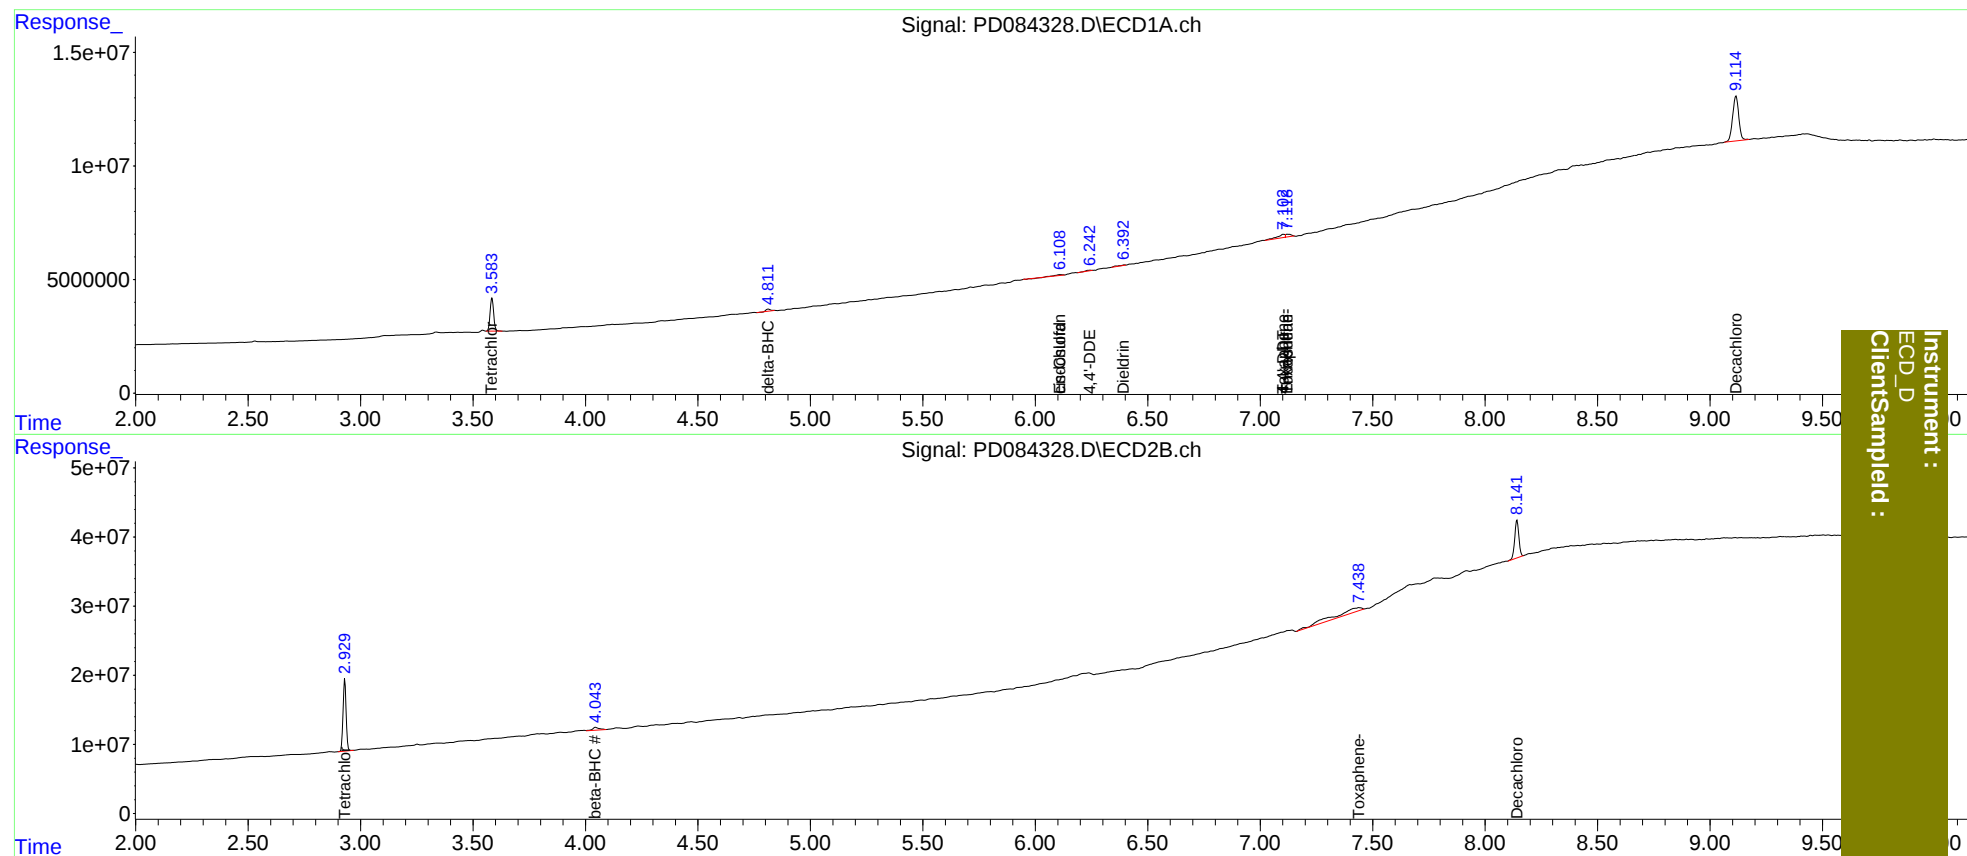


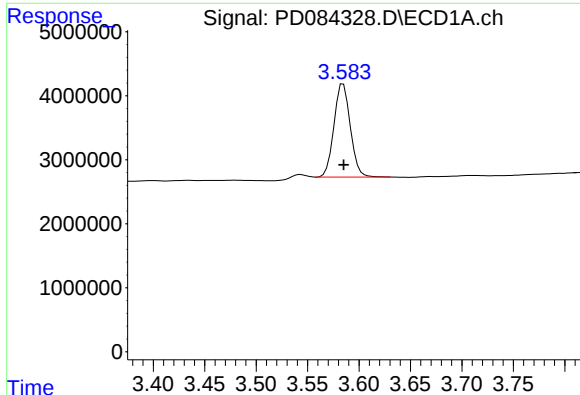

#1 Tetrachloro-m-xylene


R.T.: 3.585 min
Delta R.T.: 0.000 min
Response: 16094467
Conc: 19.20 ng/ml

Instrument :
ECD_D
ClientSampleId :

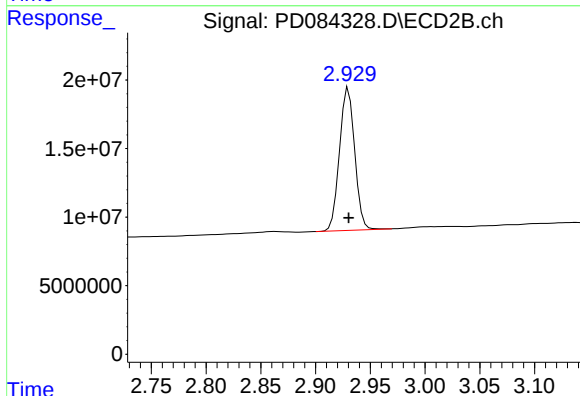


#1 Tetrachloro-m-xylene

R.T.: 2.930 min
Delta R.T.: 0.000 min
Response: 100337383
Conc: 19.06 ng/ml

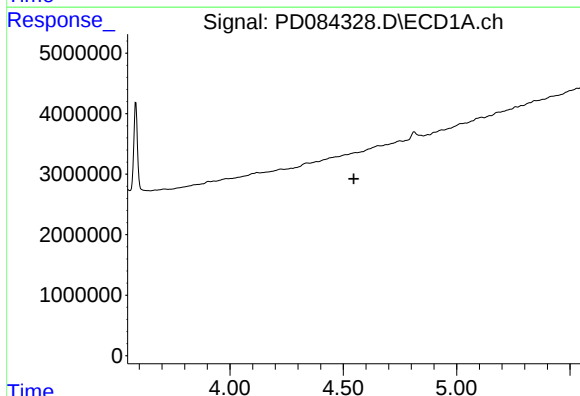


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.546 min
Response: 0
Conc: N.D.

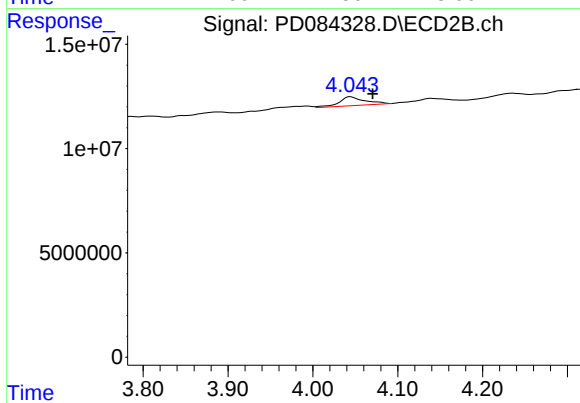

#6 beta-BHC


R.T.: 4.045 min
Delta R.T.: -0.026 min
Response: 9006958
Conc: 2.50 ng/ml

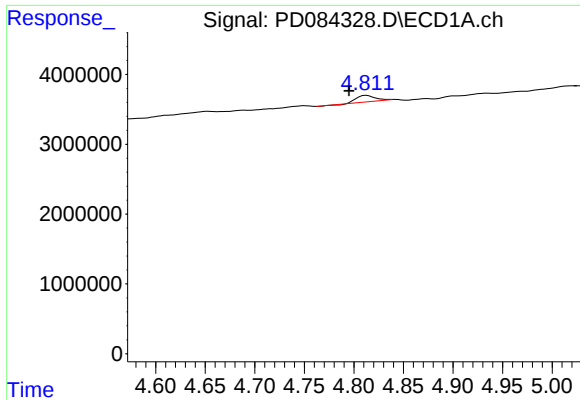

#7 delta-BHC


R.T.: 4.813 min
Delta R.T.: 0.018 min
Response: 1283131
Conc: 0.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

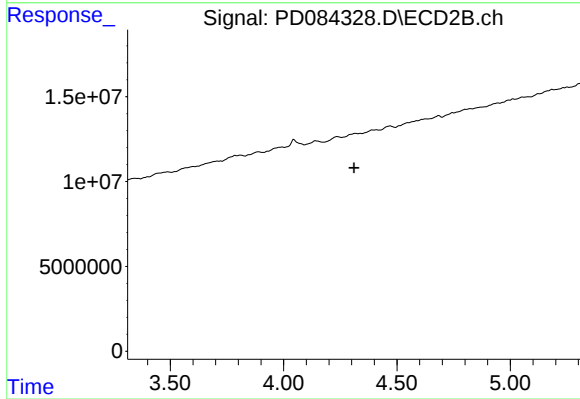


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.311 min
Response: 0
Conc: N.D.

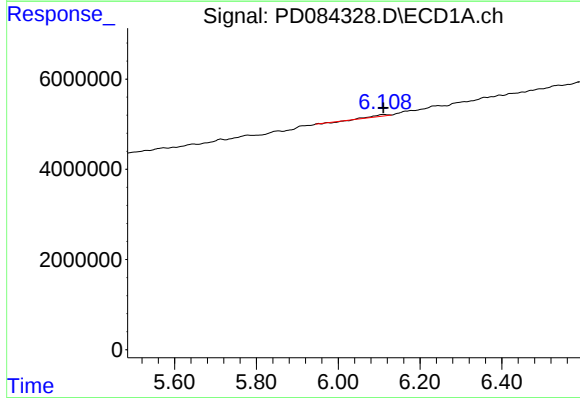


#9 Endosulfan I

R.T.: 6.111 min
Delta R.T.: 0.000 min
Response: 604553
Conc: 0.38 ng/ml

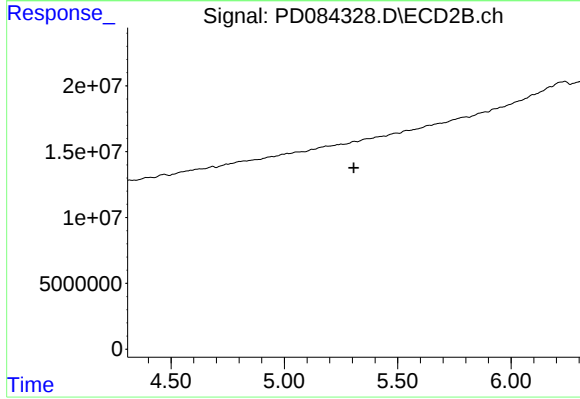

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.306 min
Response: 0
Conc: N.D.

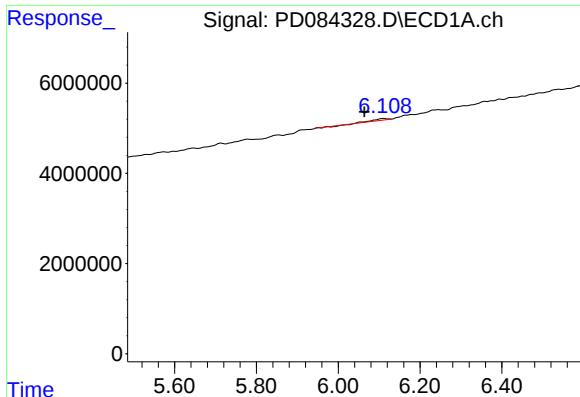

#11 cis-Chlordane


R.T.: 6.111 min
Delta R.T.: 0.047 min
Response: 604553
Conc: 0.35 ng/ml

Instrument :
ECD_D
ClientSampleId :

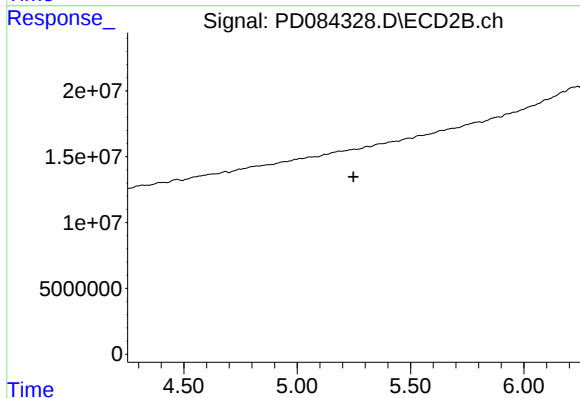


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.249 min
Response: 0
Conc: N.D.

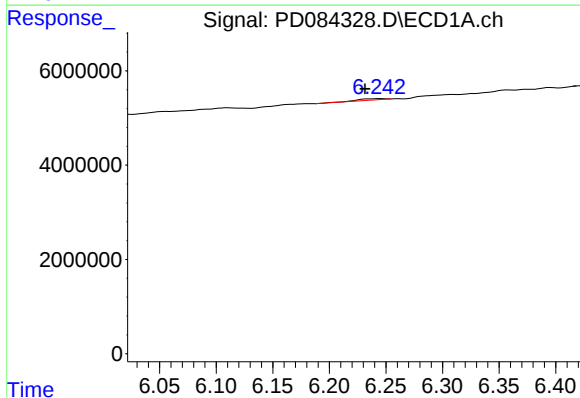


#12 4,4'-DDE

R.T.: 6.245 min
Delta R.T.: 0.014 min
Response: 454663
Conc: 0.26 ng/ml

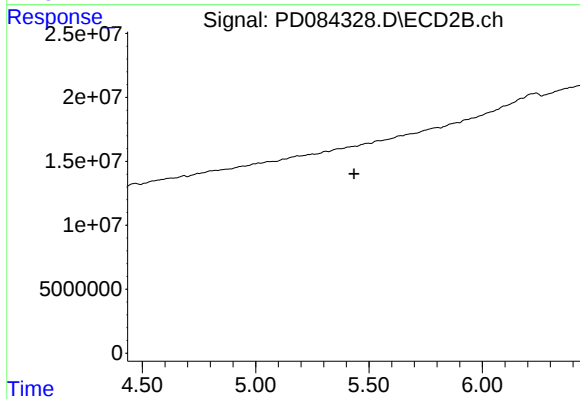

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 5.434 min
Response: 0
Conc: N.D.

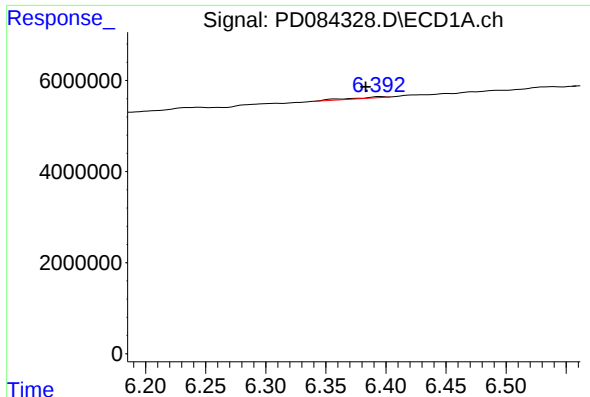

#13 Dieldrin


R.T.: 6.396 min
Delta R.T.: 0.013 min
Response: 558275
Conc: 0.31 ng/ml

Instrument :
ECD_D
ClientSampleId :

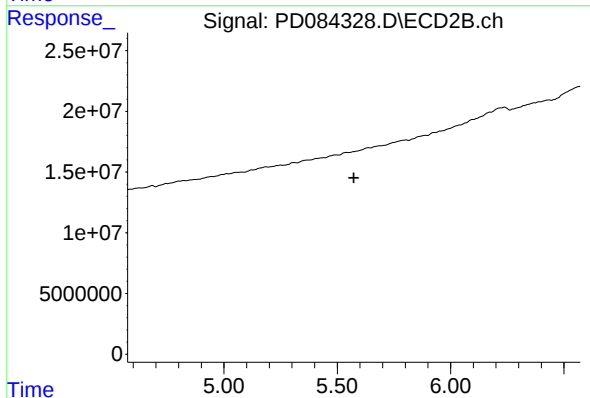


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.573 min
Response: 0
Conc: N.D.

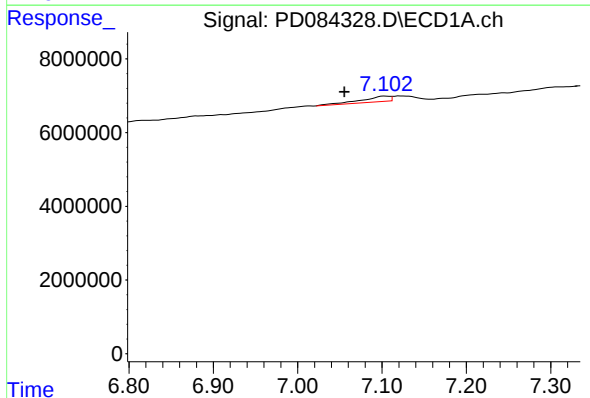


#17 4,4'-DDT

R.T.: 7.104 min
Delta R.T.: 0.048 min
Response: 3505794
Conc: 2.59 ng/ml

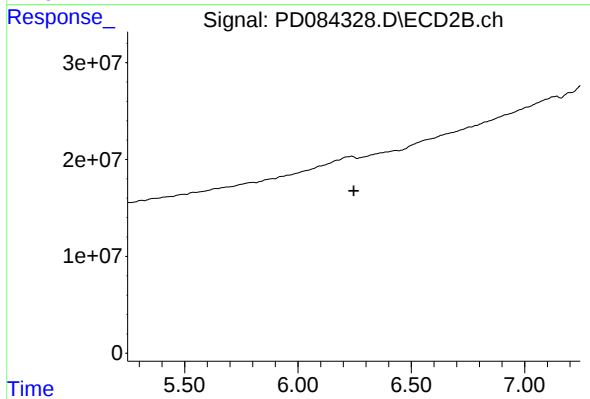

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

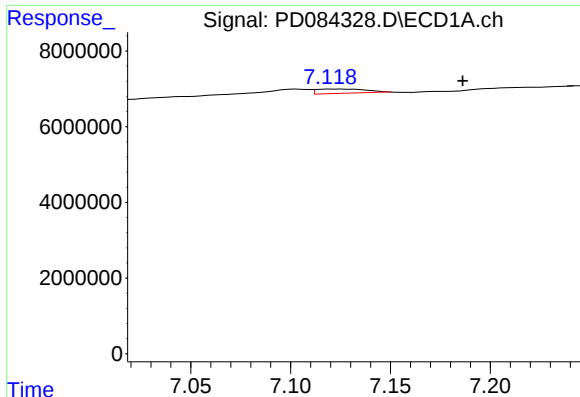

#19 Endosulfan Sulfate


R.T.: 7.123 min
Delta R.T.: -0.064 min
Response: 2084879
Conc: 1.37 ng/ml

Instrument :
ECD_D
ClientSampleId :

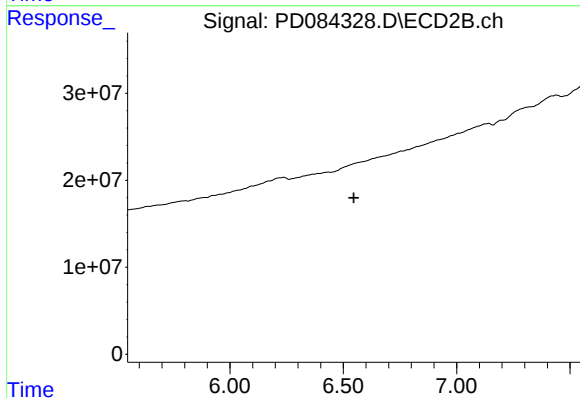


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.546 min
Response: 0
Conc: N.D.

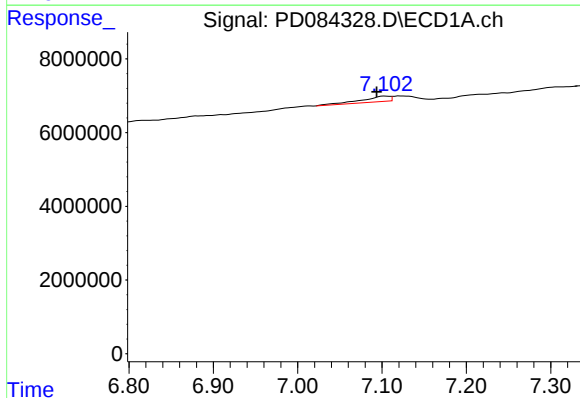


#24 Toxaphene-3

R.T.: 7.104 min
Delta R.T.: 0.010 min
Response: 3505794
Conc: 77.02 ng/ml

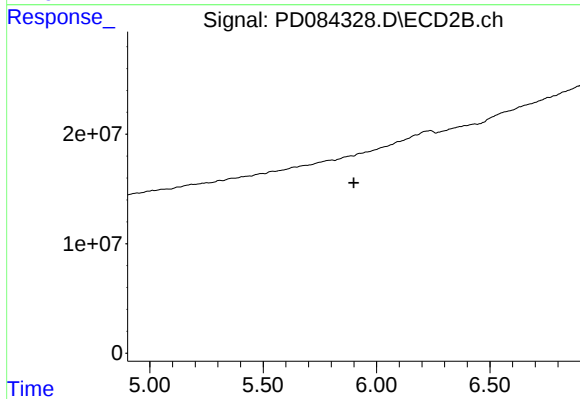

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T. : 5.899 min
Response: 0
Conc: N.D.

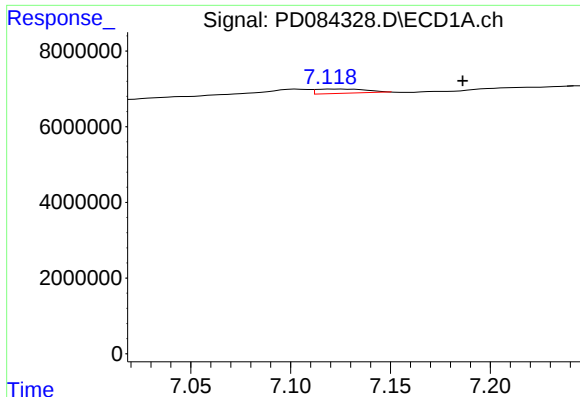

#25 Toxaphene-4


R.T.: 7.123 min
Delta R.T.: -0.064 min
Response: 2084879
Conc: 62.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

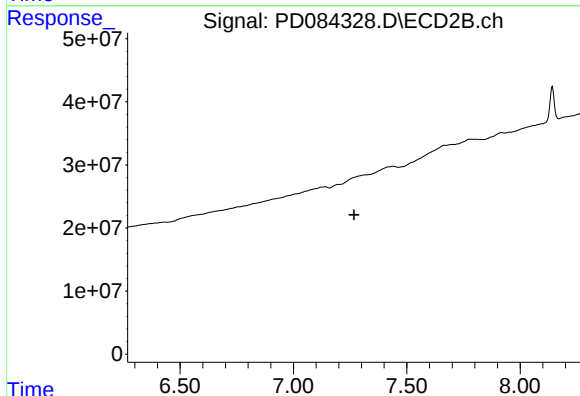


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T. : 7.267 min
Response: 0
Conc: N.D.

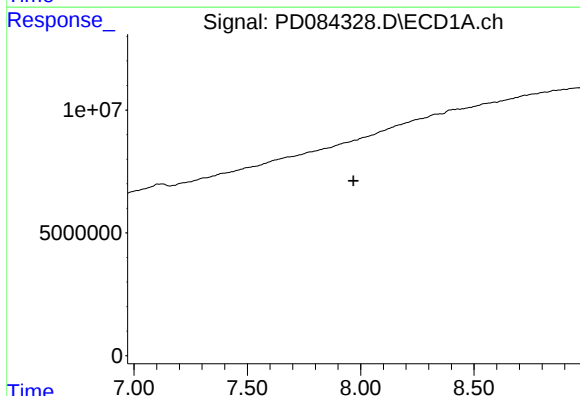


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T. : 7.968 min
Response: 0
Conc: N.D.

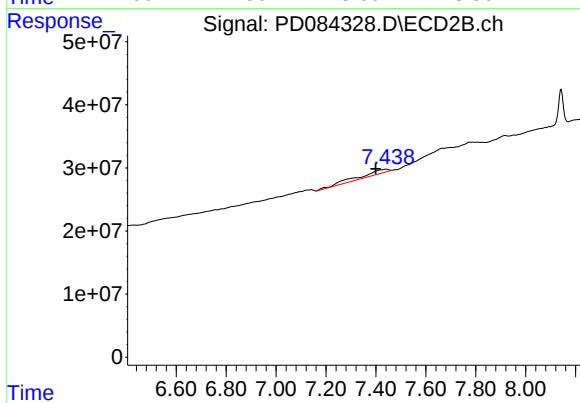

#26 Toxaphene-5


R.T.: 7.439 min
Delta R.T.: 0.040 min
Response: 58088318
Conc: 1059.26 ng/ml

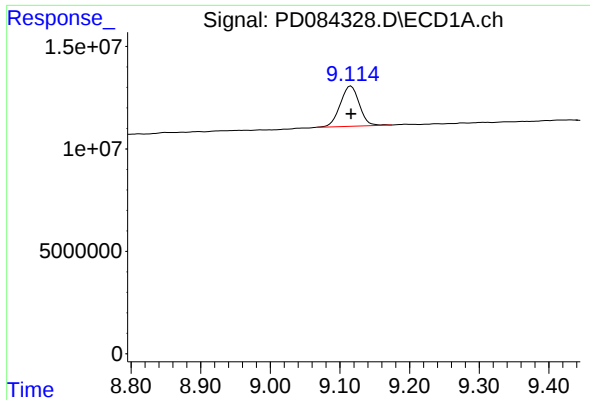

#27 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: 0.000 min
Response: 37361879
Conc: 21.48 ng/ml

Instrument :
ECD_D
ClientSampleId :

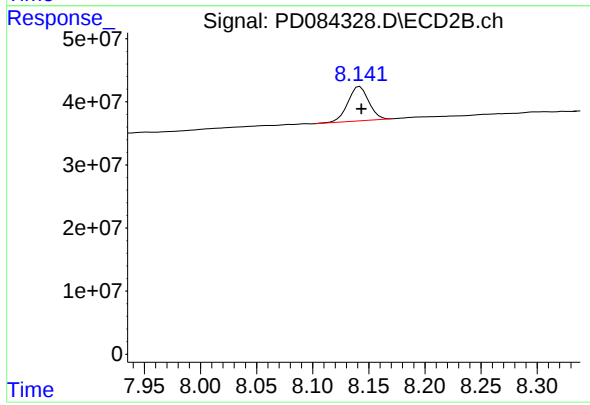

#27 Decachlorobiphenyl

R.T.: 8.142 min
Delta R.T.: -0.002 min
Response: 70398334
Conc: 18.73 ng/ml