

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081224\
 Data File : PD084336.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 00:22
 Operator : AR\AJ
 Sample : P3480-10
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E0AA6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:02:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.585	2.930	17875318	106.7E6	21.321	20.276
27)	SA Decachlor...	9.115	8.141	39860876	79957587	22.918	21.277
Target Compounds							
2)	A alpha-BHC	0.000	3.422	0	8528365	N.D.	1.046
7)	B delta-BHC	4.812	0.000	1783013	0	1.032	N.D. #
9)	A Endosulfan I	6.109	0.000	526655	0	0.331	N.D. #
11)	B cis-Chlor...	6.109f	0.000	526655	0	0.306	N.D. #
15)	B Endosulfa...	6.811	0.000	940107	0	0.570	N.D. #
17)	MA 4,4'-DDT	7.092f	0.000	1199474	0	0.885	N.D. #
18)	B Endrin al...	6.938	0.000	1492315	0	1.313	N.D. #
19)	B Endosulfa...	7.121f	0.000	1413722	0	0.931	N.D. #
24)	Toxaphene-3	7.092	0.000	1199474	0	26.352	N.D. #
25)	Toxaphene-4	7.121f	0.000	1413722	0	42.138	N.D. #
26)	Toxaphene-5	8.034f	7.390	11423917	37086756	460.468	676.287 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081224\
Data File : PD084336.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 00:22
Operator : AR\AJ
Sample : P3480-10
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:02:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

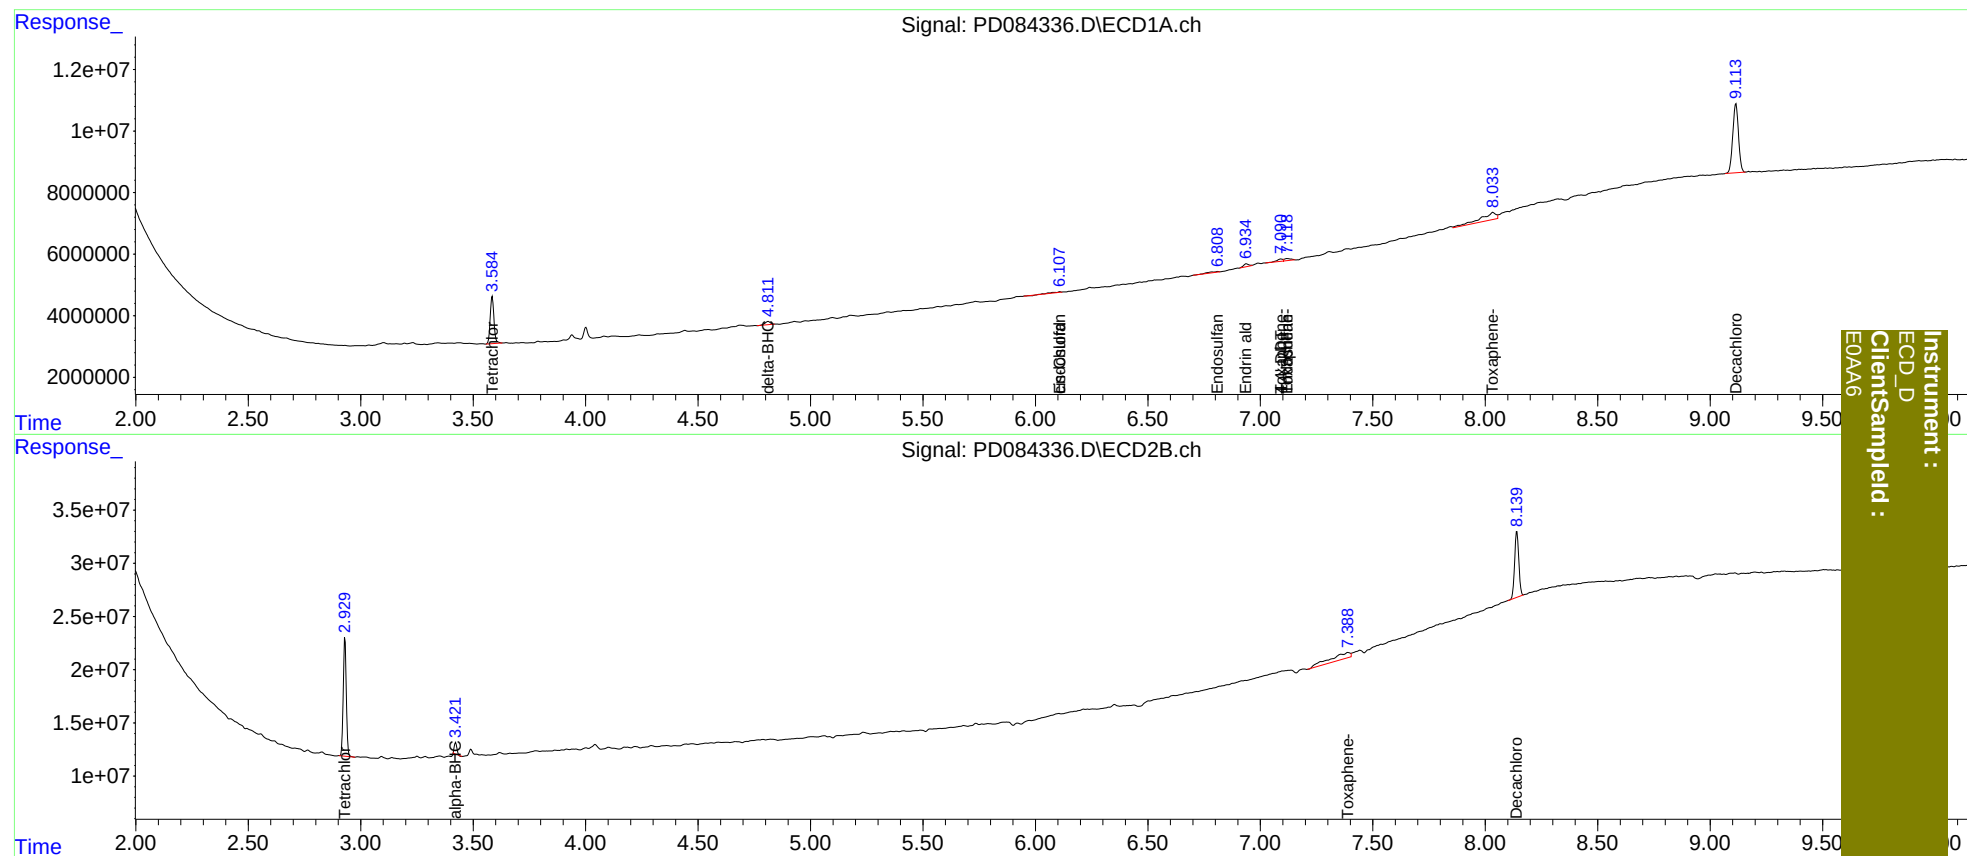


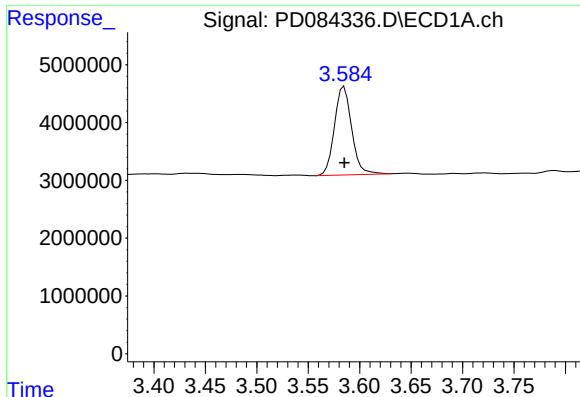

#1 Tetrachloro-m-xylene


R.T.: 3.585 min
Delta R.T.: 0.000 min
Response: 17875318
Conc: 21.32 ng/ml

Instrument :
ECD_D
ClientSampleId :
E0AA6

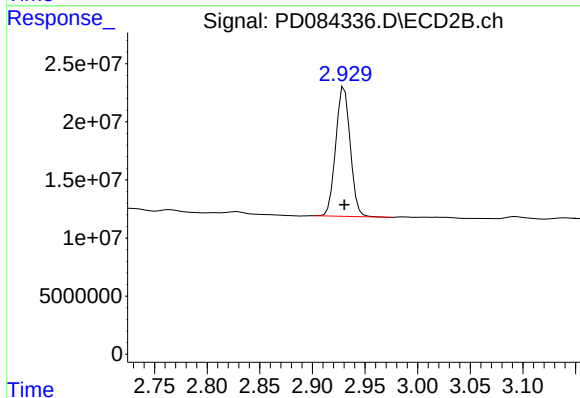


#1 Tetrachloro-m-xylene

R.T.: 2.930 min
Delta R.T.: 0.000 min
Response: 106737349
Conc: 20.28 ng/ml

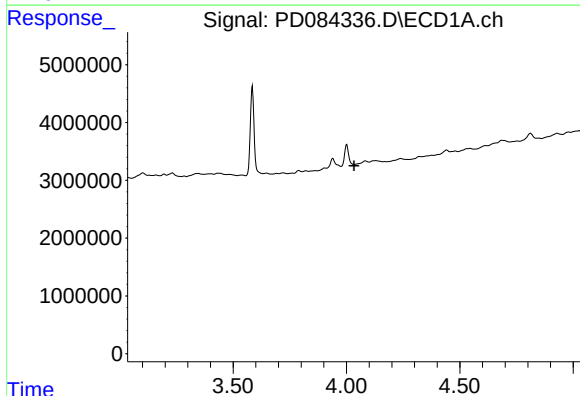


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 4.033 min
Response: 0
Conc: N.D.

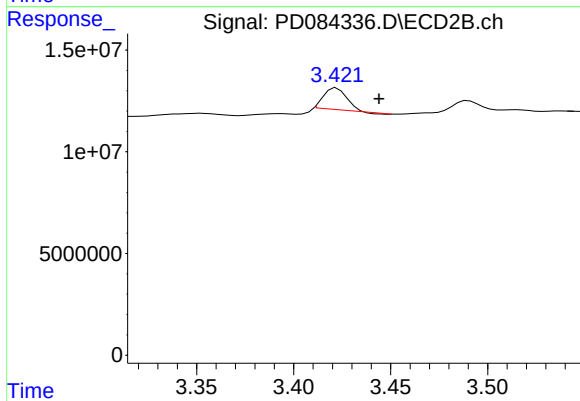

#2 alpha-BHC


R.T.: 3.422 min
Delta R.T.: -0.022 min
Response: 8528365
Conc: 1.05 ng/ml

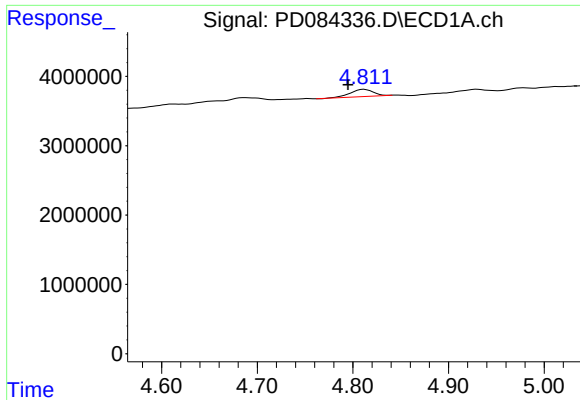

#7 delta-BHC


R.T.: 4.812 min
Delta R.T.: 0.017 min
Response: 1783013
Conc: 1.03 ng/ml

Instrument :
ECD_D
ClientSampleId :
E0AA6

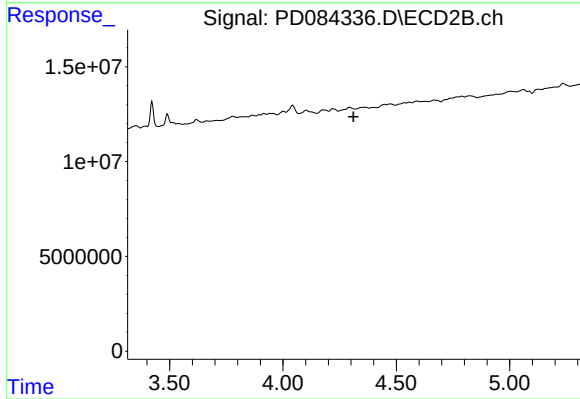


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.311 min
Response: 0
Conc: N.D.

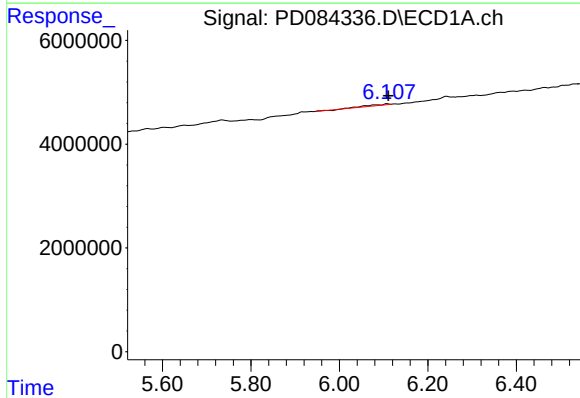


#9 Endosulfan I

R.T.: 6.109 min
Delta R.T.: -0.002 min
Response: 526655
Conc: 0.33 ng/ml

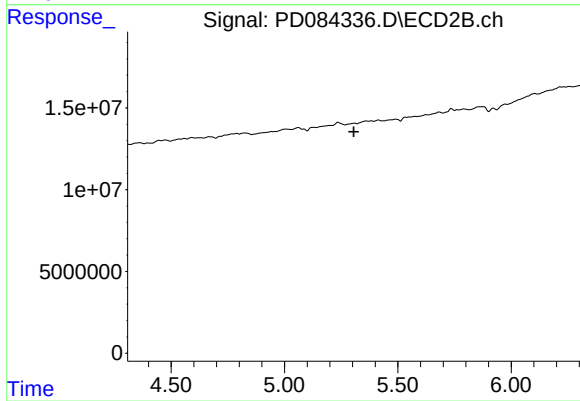

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.306 min
Response: 0
Conc: N.D.

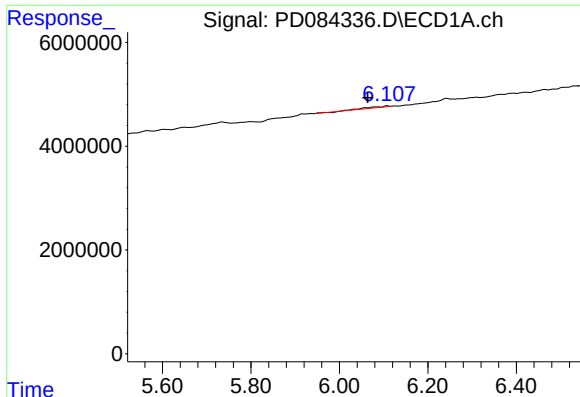

#11 cis-Chlordane


R.T.: 6.109 min
Delta R.T.: 0.045 min
Response: 526655
Conc: 0.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
E0AA6

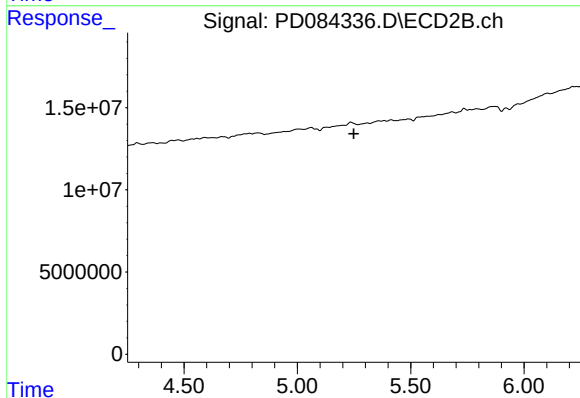


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.249 min
Response: 0
Conc: N.D.

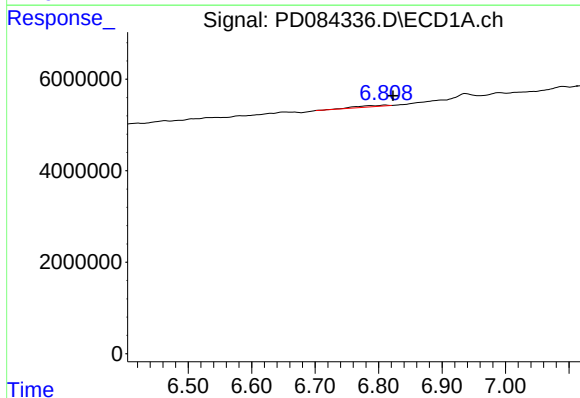


#15 Endosulfan II

R.T.: 6.811 min
Delta R.T.: -0.012 min
Response: 940107
Conc: 0.57 ng/ml

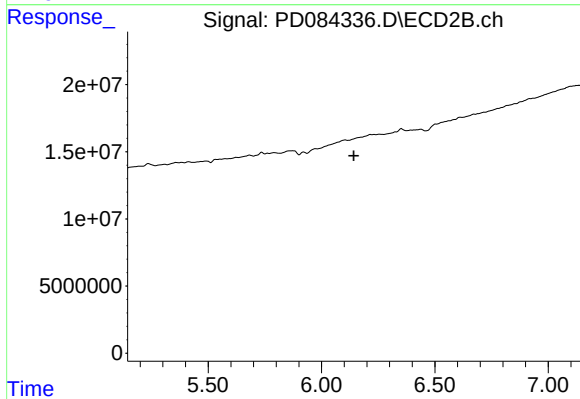

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.142 min
Response: 0
Conc: N.D.

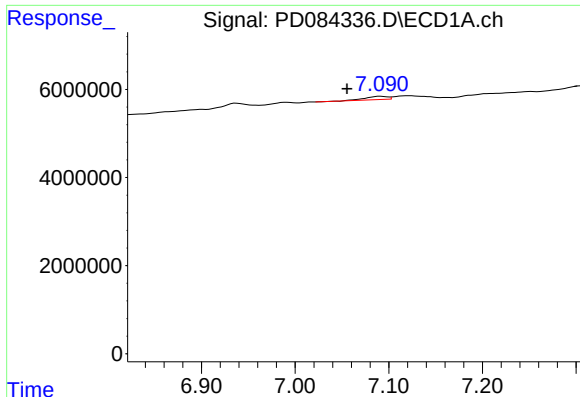

#17 4,4'-DDT


R.T.: 7.092 min
Delta R.T.: 0.036 min
Response: 1199474
Conc: 0.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
E0AA6

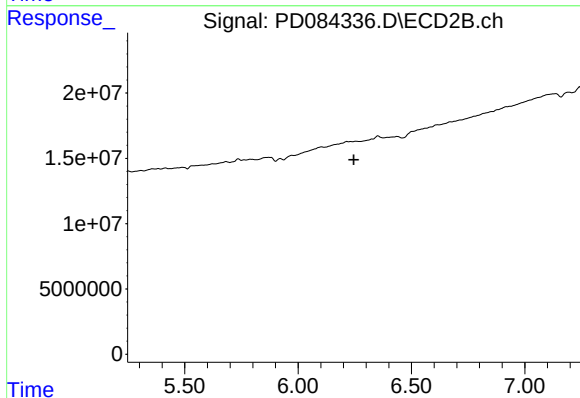


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

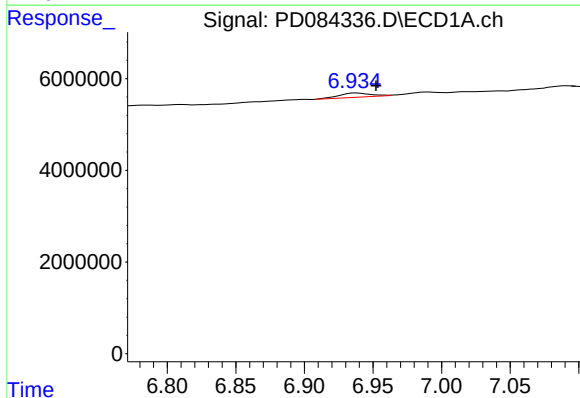


#18 Endrin aldehyde

R.T.: 6.938 min
Delta R.T.: -0.014 min
Response: 1492315
Conc: 1.31 ng/ml

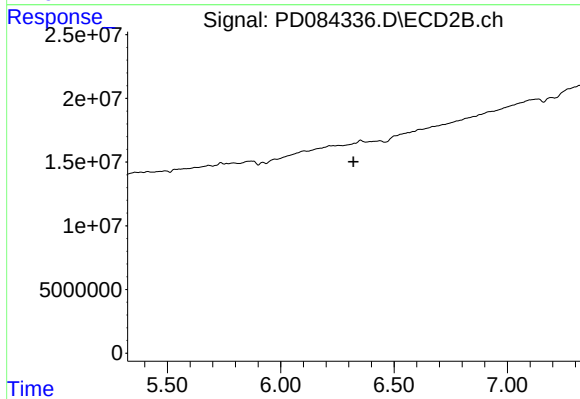

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.321 min
Response: 0
Conc: N.D.

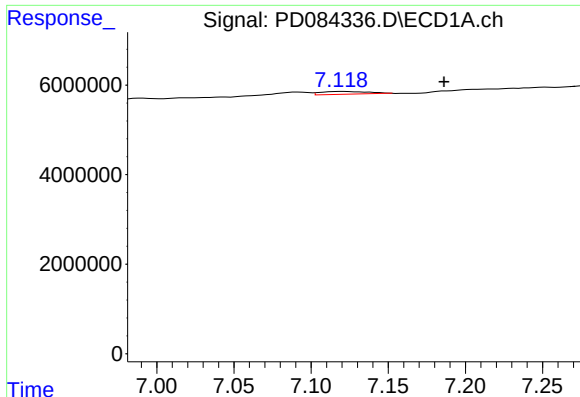

#19 Endosulfan Sulfate


R.T.: 7.121 min
Delta R.T.: -0.065 min
Response: 1413722
Conc: 0.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
E0AA6

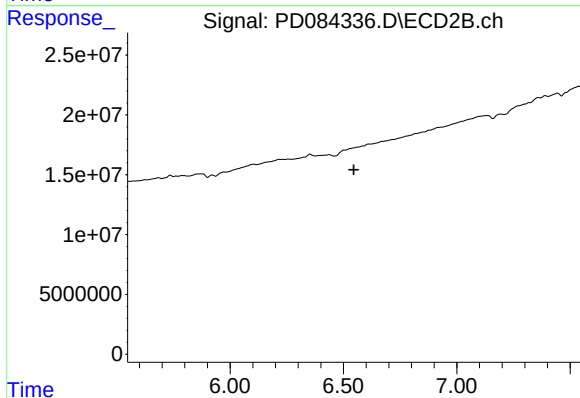


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.546 min
Response: 0
Conc: N.D.

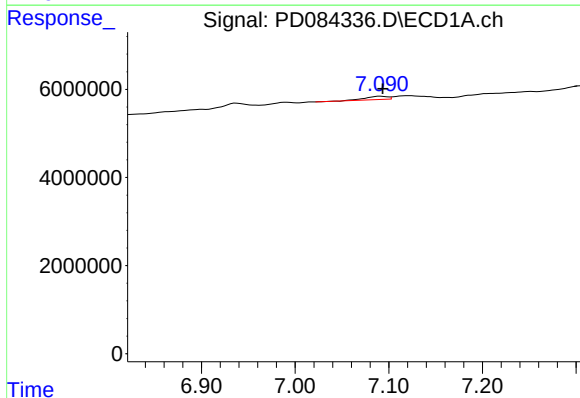


#24 Toxaphene-3

R.T.: 7.092 min
Delta R.T.: -0.002 min
Response: 1199474
Conc: 26.35 ng/ml

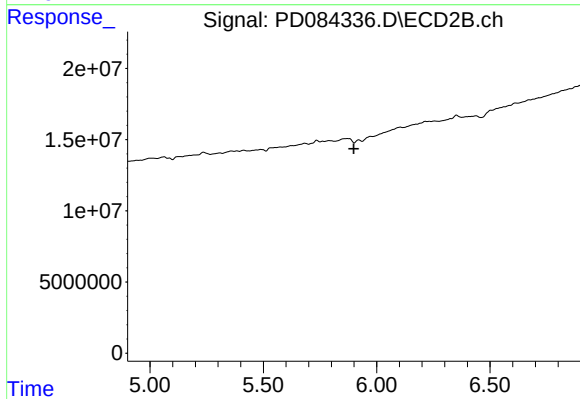

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T. : 5.899 min
Response: 0
Conc: N.D.

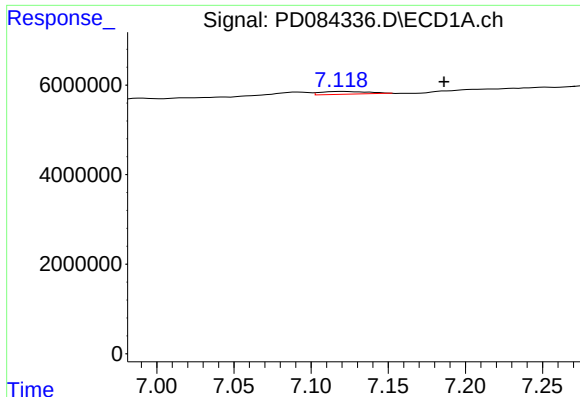

#25 Toxaphene-4


R.T.: 7.121 min
Delta R.T.: -0.065 min
Response: 1413722
Conc: 42.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
E0AA6

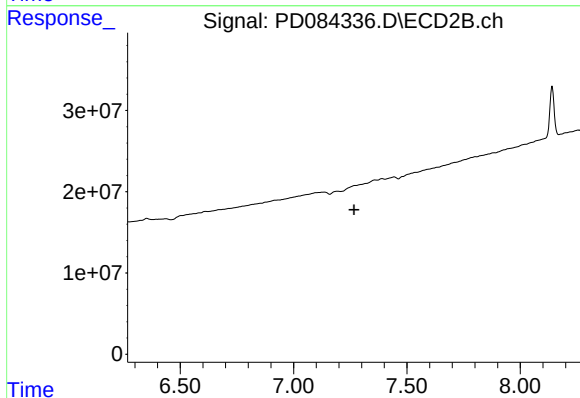


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T.: 7.267 min
Response: 0
Conc: N.D.

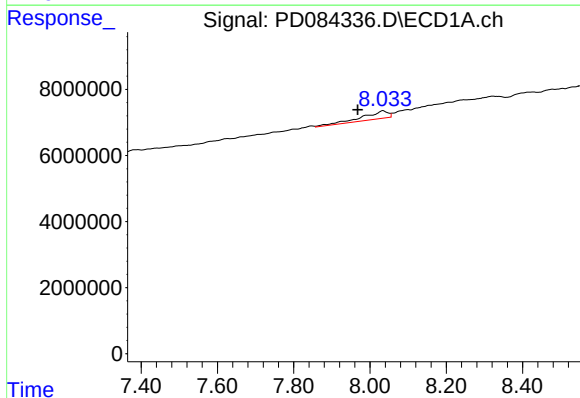


#26 Toxaphene-5

R.T.: 8.034 min
Delta R.T.: 0.066 min
Response: 11423917
Conc: 460.47 ng/ml

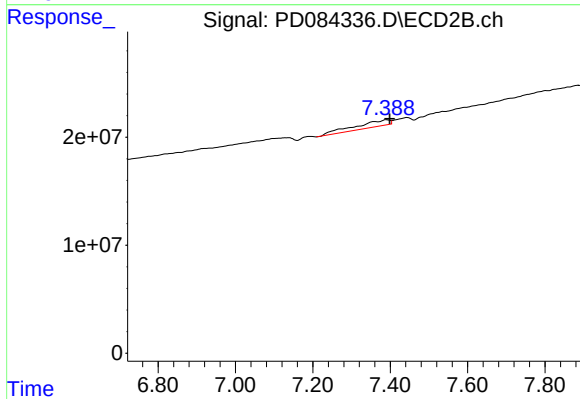

#26 Toxaphene-5


R.T.: 7.390 min
Delta R.T.: -0.010 min
Response: 37086756
Conc: 676.29 ng/ml

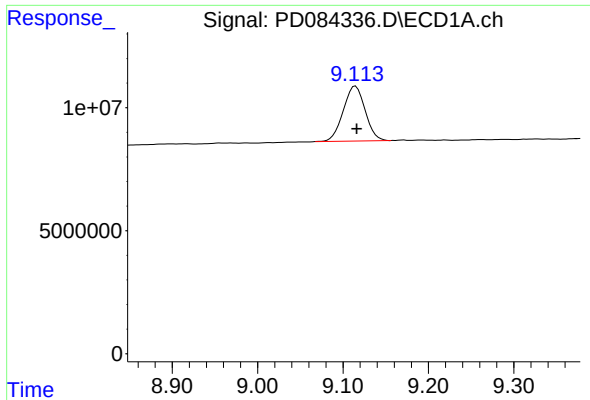

#27 Decachlorobiphenyl

R.T.: 9.115 min
Delta R.T.: -0.001 min
Response: 39860876
Conc: 22.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
E0AA6

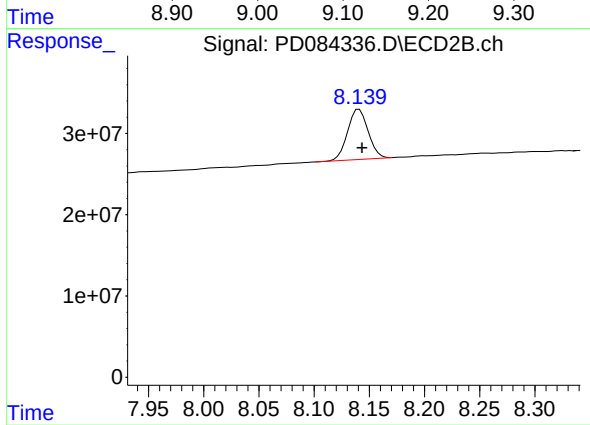

#27 Decachlorobiphenyl

R.T.: 8.141 min
Delta R.T.: -0.003 min
Response: 79957587
Conc: 21.28 ng/ml