

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081224\
 Data File : PD084308.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2024 18:08
 Operator : AR\AJ
 Sample : P3439-02MSRX
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DCVW9MSRX

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/22/2024
 Supervised By :Ankita Jodhani 08/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:01:24 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.570	2.934	53161790	112.5E6	63.411m	21.379m#
27)	SA Decachlor...	9.104	8.163	9927422	93216701	5.708m	24.805 #
Target Compounds							
2)	A alpha-BHC	4.034	3.444	203.0E6	548.3E6	134.094	67.264 #
3)	MA gamma-BHC...	4.309f	3.778	94988.2E6	813.3E6	60986.212m	105.525m#
4)	MA Heptachlor	4.965	4.138	93339562	248.6E6	53.479m	32.980m#
5)	MB Aldrin	5.309	4.427	129.3E6	372.0E6	73.283	50.756 #
6)	B beta-BHC	4.541	4.071	31765891	28502833	43.966m	7.925m#
7)	B delta-BHC	4.796	4.312	310.7E6	675.0E6	179.932	80.472 #
8)	B Heptachlo...	5.729	4.929	110.9E6	260.5E6	65.257	39.038 #
9)	A Endosulfan I	6.108	5.308	304.7E6	385.3E6	191.284m	64.942 #
10)	B trans-Chl...	5.981	5.183	215.9E6	249.5E6	130.784	39.156 #
11)	B cis-Chlor...	6.061	5.255	37296688	338.2E6	21.675m	53.743 #
12)	B 4,4'-DDE	6.229	5.434	243.0E6	451.7E6	138.954m	74.062m#
13)	MA Dieldrin	6.384	5.574	331.1E6	578.9E6	184.284m	94.107m#
14)	MA Endrin	6.612	5.849	76250465	716.5E6	50.900m	129.776 #
15)	B Endosulfa...	6.819	6.150	294.1E6	500.1E6	178.396m	96.308m#
16)	A 4,4'-DDD	6.737	5.986	147.1E6	331.4E6	114.361m	67.544 #
17)	MA 4,4'-DDT	7.054	6.220	509.4E6	3714.5E6	375.719m	749.848m#
18)	B Endrin al...	6.953	6.320	362.0E6	434.3E6	318.499m	116.067m#
19)	B Endosulfa...	7.183	6.545	142.8E6	296.1E6	94.071m	63.412m#
20)	A Methoxychlor	7.526	6.819	430.9E6	584.0E6	540.298	271.194 #
21)	B Endrin ke...	7.667	7.056	212.5E6	319.2E6	128.291	61.302 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081224\
Data File : PD084308.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2024 18:08
Operator : AR\AJ
Sample : P3439-02MSRX
Misc :
ALS Vial : 33 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 01:01:24 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

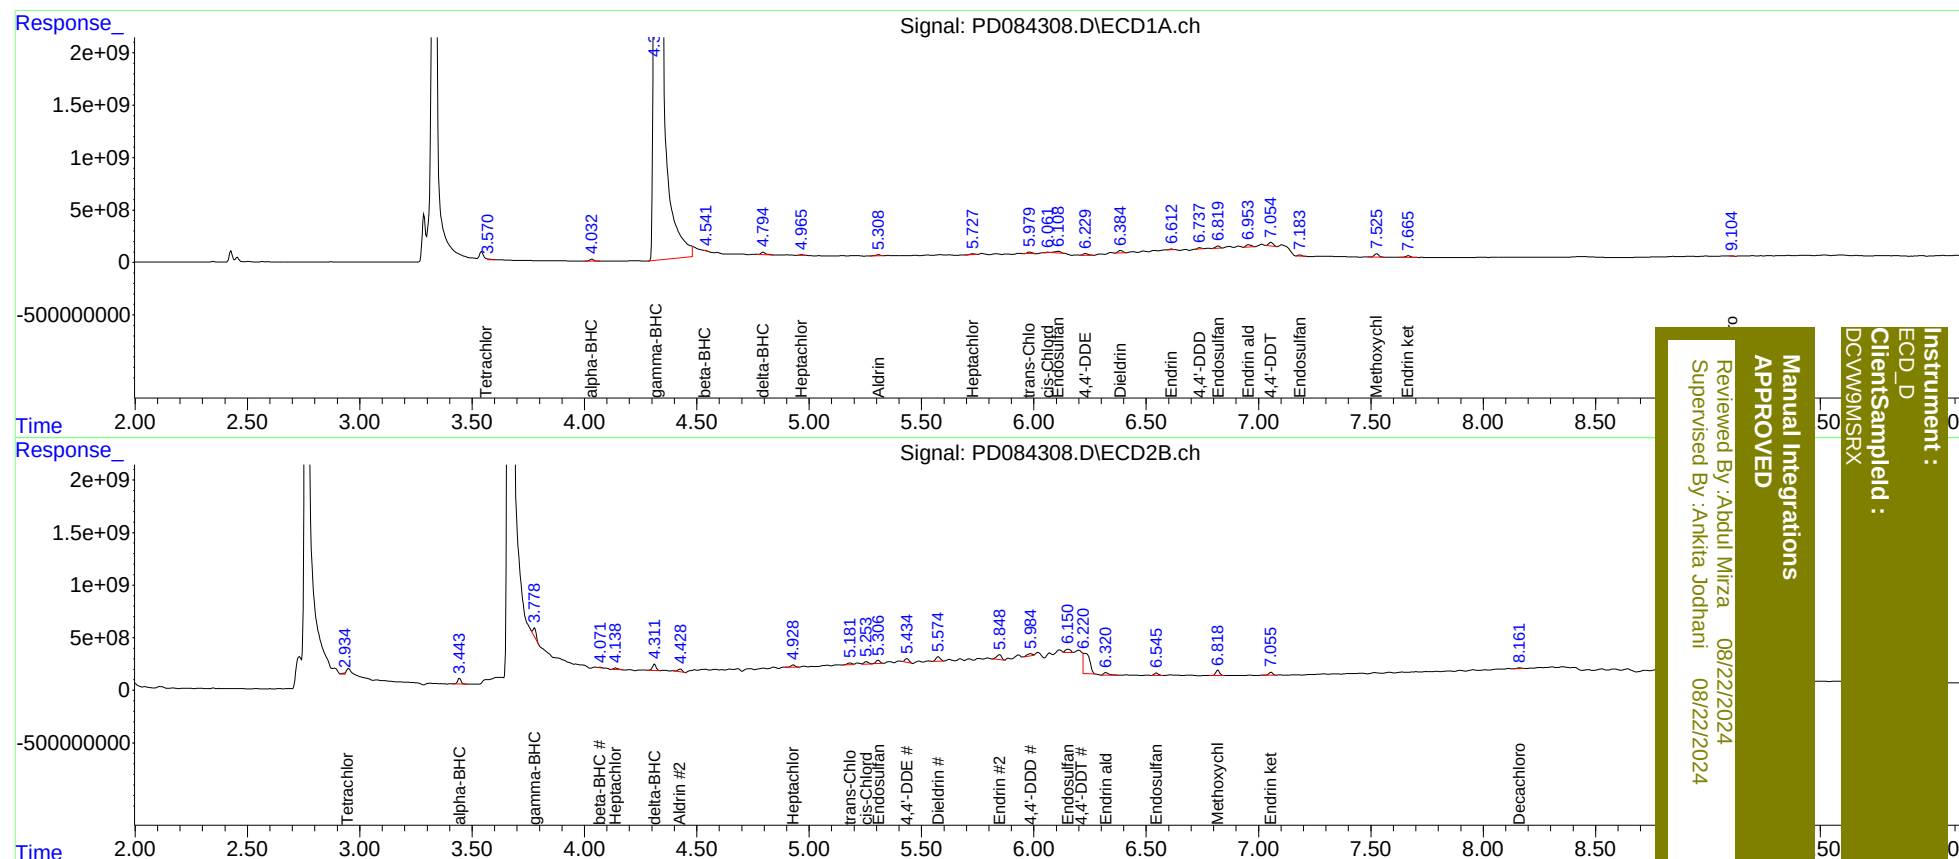

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 08/22/2024
Supervised By: Ankita Jodhani 08/22/2024

Instrument :
ECD_D
Client Sampled :
DCW/MSRX