

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081224\
 Data File : PD084337.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 00:36
 Operator : AR\AJ
 Sample : P3480-11MS
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E0AA6MS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/14/2024
 Supervised By :Ankita Jodhani 08/14/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:02:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.585	2.930	17342360	104.3E6	20.686	19.820
2)	SA Decachlor...	9.115	8.141	39536700	81394302	22.731	21.659
Target Compounds							
2)	A alpha-BHC	4.032	3.442	84536742	403.4E6	55.854m	49.486m
3)	MA gamma-BHC...	4.364	3.779	88571537	374.5E6	56.866	48.591
4)	MA Heptachlor	4.964	4.137	95287100	337.6E6	54.595	44.803
5)	MB Aldrin	5.307	4.425	96294098	332.5E6	54.563	45.364
6)	B beta-BHC	4.546	4.072	35550073	159.1E6	49.204	44.251
7)	B delta-BHC	4.795	4.311	95414275	383.4E6	55.251	45.705
8)	B Heptachlo...	5.726	4.929	92571067	300.9E6	54.464	45.102
9)	A Endosulfan I	6.110	5.305	91292316	271.7E6	57.310	45.787m
10)	B trans-Chl...	5.981	5.183	92303542	300.1E6	55.902	47.098
11)	B cis-Chlor...	6.062	5.249	94225999	292.6E6	54.759	46.490
12)	B 4,4'-DDE	6.230	5.433	190.2E6	556.5E6	108.756	91.246
13)	MA Dieldrin	6.383	5.573	207.5E6	573.1E6	115.502	93.155
14)	MA Endrin	6.611	5.850	174.9E6	524.2E6	116.785	94.948
15)	B Endosulfa...	6.821	6.141	176.0E6	477.7E6	106.730	91.999
16)	A 4,4'-DDD	6.739	5.989	147.2E6	459.5E6	114.427	93.658
17)	MA 4,4'-DDT	7.055	6.245	145.7E6	457.4E6	107.478	92.343
18)	B Endrin al...	6.950	6.320	126.0E6	348.4E6	110.885	93.110
19)	B Endosulfa...	7.184	6.545	167.9E6	427.5E6	110.586	91.555
20)	A Methoxychlor	7.526	6.819	424.3E6	953.5E6	532.017	442.770
21)	B Endrin ke...	7.666	7.056	182.6E6	494.2E6	110.247	94.903

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081224\
Data File : PD084337.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 00:36
Operator : AR\AJ
Sample : P3480-11MS
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:02:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

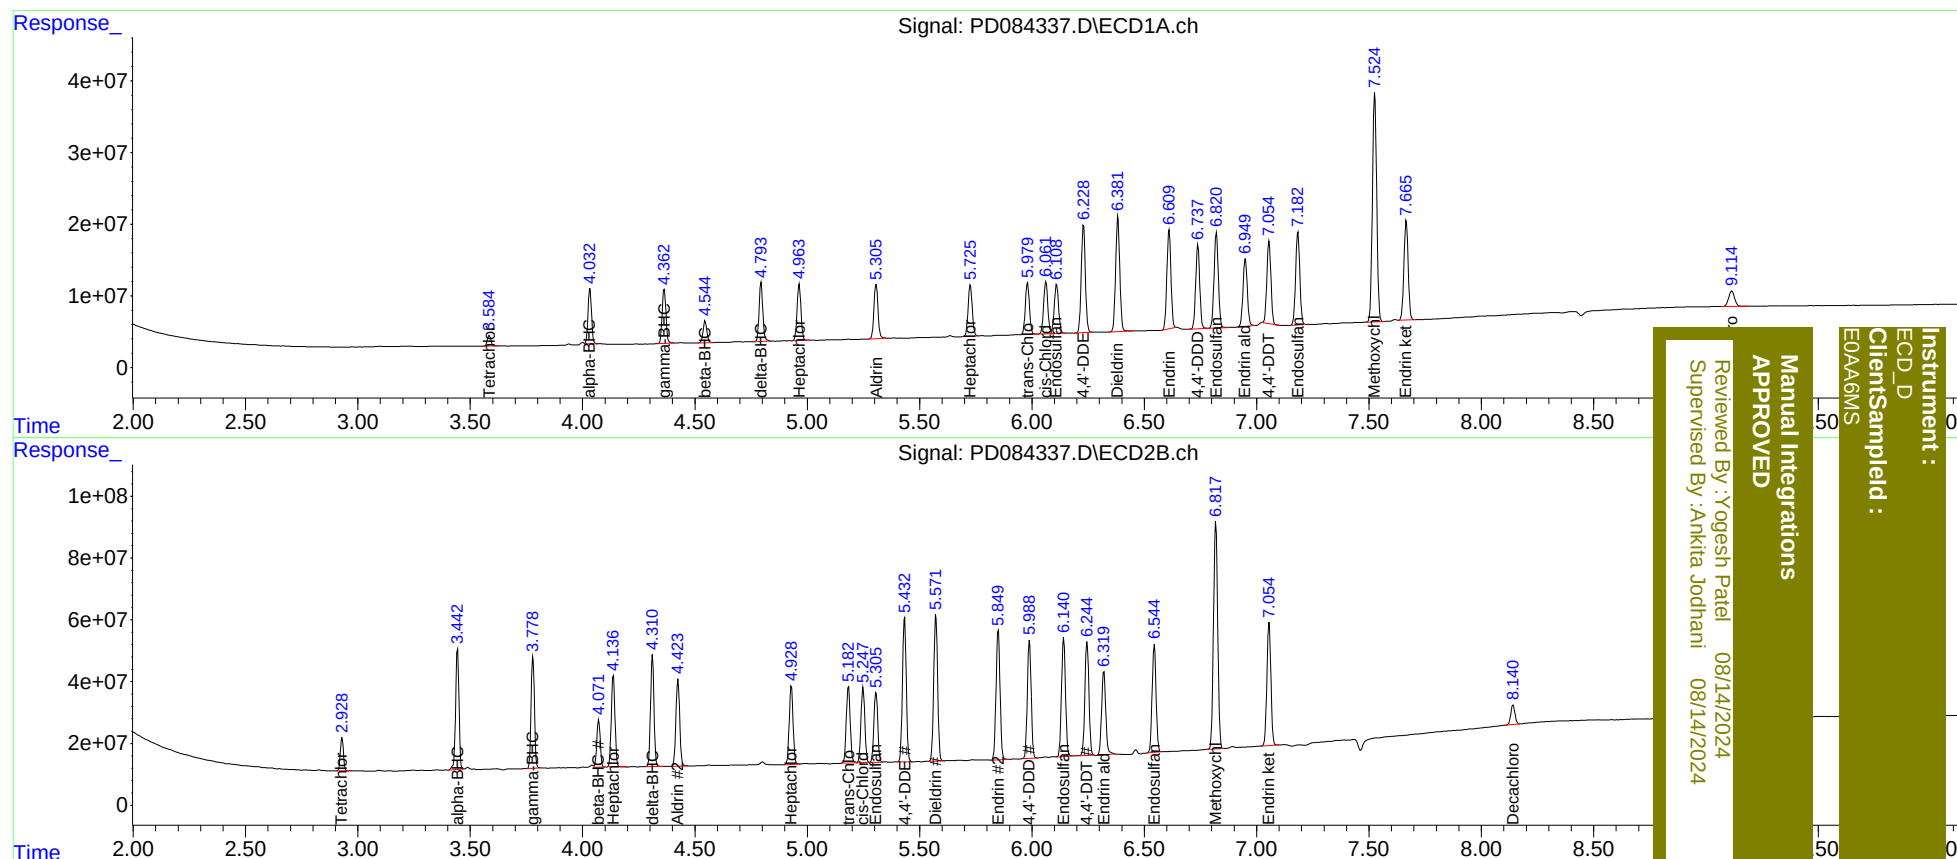

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 08/14/2024
Supervised By : Ankita Jodhani 08/14/2024

Instrument :
ECD_D
Client Sampled :
E0AA6MS