

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081224\
 Data File : PD084338.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 00:49
 Operator : AR\AJ
 Sample : P3480-12MSD
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E0AA6MSD

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/14/2024
 Supervised By :Ankita Jodhani 08/14/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 04:03:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
 Quant Title : GC Extractables
 QLast Update : Mon Aug 12 16:40:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.585	2.930	17428500	105.7E6	20.788	20.079
2)	SA Decachlor...	9.114	8.141	39524759	81452199	22.724	21.675
Target Compounds							
2)	A alpha-BHC	4.032	3.442	83626947	402.5E6	55.253m	49.372m
3)	MA gamma-BHC...	4.363	3.779	88927705	376.0E6	57.095	48.786
4)	MA Heptachlor	4.964	4.137	95473674	338.7E6	54.702	44.936
5)	MB Aldrin	5.306	4.425	96055658	330.7E6	54.428	45.127
6)	B beta-BHC	4.546	4.072	35724091	158.0E6	49.444	43.942
7)	B delta-BHC	4.794	4.311	94010863	383.3E6	54.438	45.692
8)	B Heptachlo...	5.725	4.929	92200145	300.3E6	54.246	44.998
9)	A Endosulfan I	6.109	5.304	90730897	270.8E6	56.957	45.647m
10)	B trans-Chl...	5.980	5.183	91501087	301.4E6	55.416	47.293
11)	B cis-Chlor...	6.062	5.248	93743656	293.0E6	54.479	46.560
12)	B 4,4'-DDE	6.229	5.433	188.9E6	556.2E6	107.970	91.207
13)	MA Dieldrin	6.382	5.572	205.9E6	572.2E6	114.613	93.011
14)	MA Endrin	6.610	5.849	174.7E6	522.7E6	116.624	94.686
15)	B Endosulfa...	6.820	6.141	174.7E6	476.9E6	105.982	91.847
16)	A 4,4'-DDD	6.738	5.989	146.1E6	458.5E6	113.585	93.455
17)	MA 4,4'-DDT	7.055	6.245	142.7E6	453.5E6	105.280	91.551
18)	B Endrin al...	6.949	6.319	125.8E6	347.3E6	110.685	92.831
19)	B Endosulfa...	7.183	6.544	167.6E6	428.1E6	110.396	91.687
20)	A Methoxychlor	7.525	6.817	420.5E6	947.8E6	527.270	440.160
21)	B Endrin ke...	7.665	7.054	181.8E6	494.8E6	109.791	95.016

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD081224\
Data File : PD084338.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 00:49
Operator : AR\AJ
Sample : P3480-12MSD
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 04:03:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD081224CLP.M
Quant Title : GC Extractables
QLast Update : Mon Aug 12 16:40:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

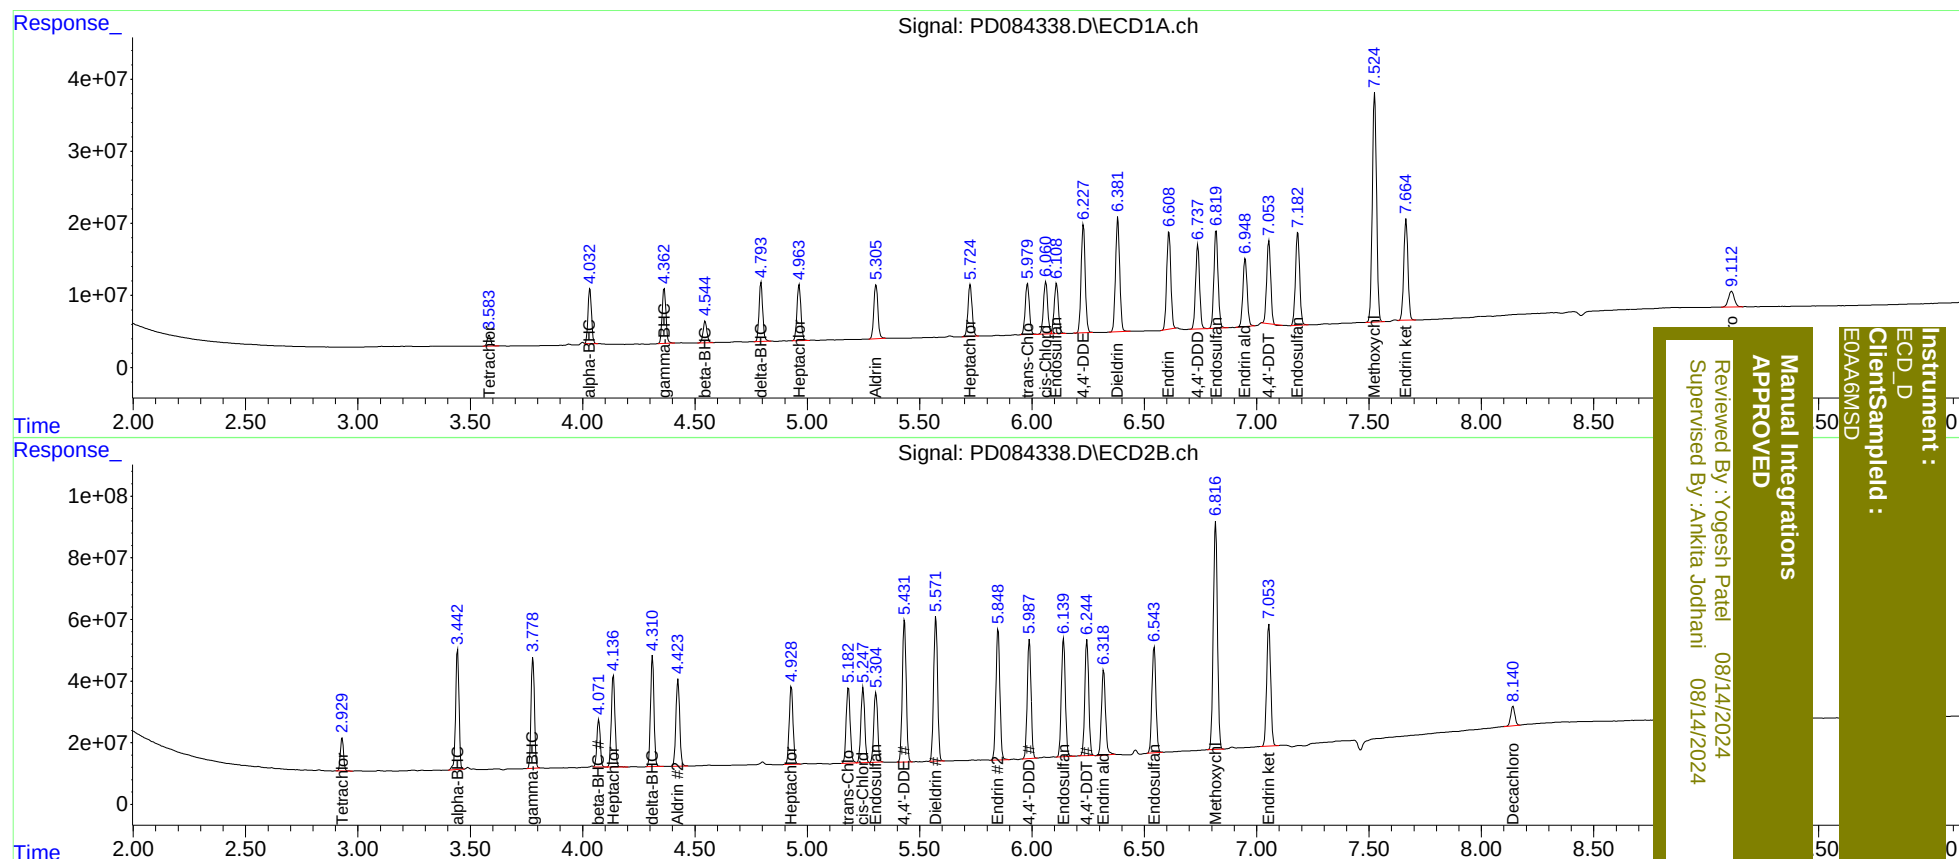

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 08/14/2024
Supervised By : Ankita Jodhani 08/14/2024

Instrument :
ECD_D
Client Sampled :
E0AA6MSD